

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
 Data File : PD078537.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 19:34
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 00:52:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 00:50:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.757	13809002	10627349	5.266	4.841
28)	SA Decachlor...	9.077	7.893	19333201	11047981	5.694	5.259
Target Compounds							
23)	Chlordane-1	4.704	3.753	6630671	3644766	50.797	50.530
24)	Chlordane-2	5.235	4.328	7877694	4046192	56.525	53.331
25)	Chlordane-3	5.946	4.958	28329919	12292870	48.321	47.969
26)	Chlordane-4	6.029	5.021	35459256	12257875	50.351	49.132
27)	Chlordane-5	6.881	5.917	5266846	3727399	47.197	42.417



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
Data File : PD078537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 19:34
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 00:52:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 00:50:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

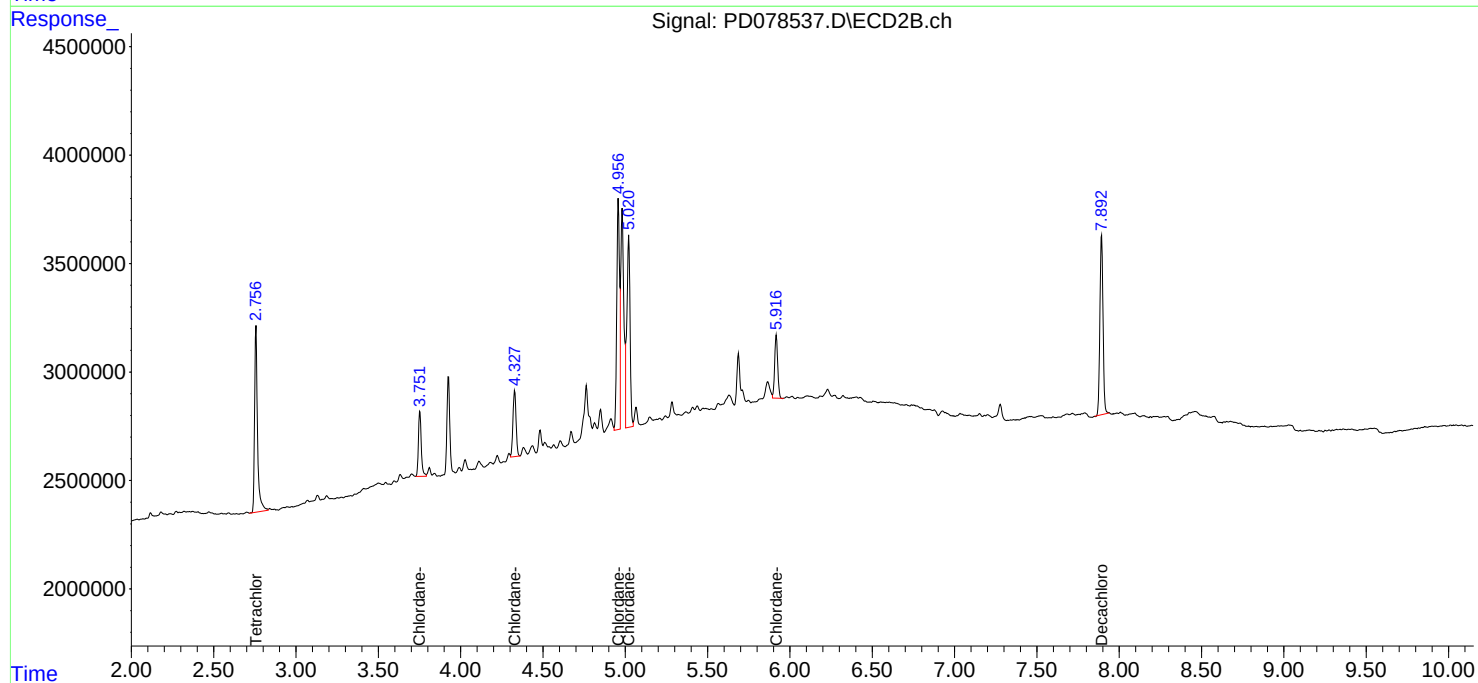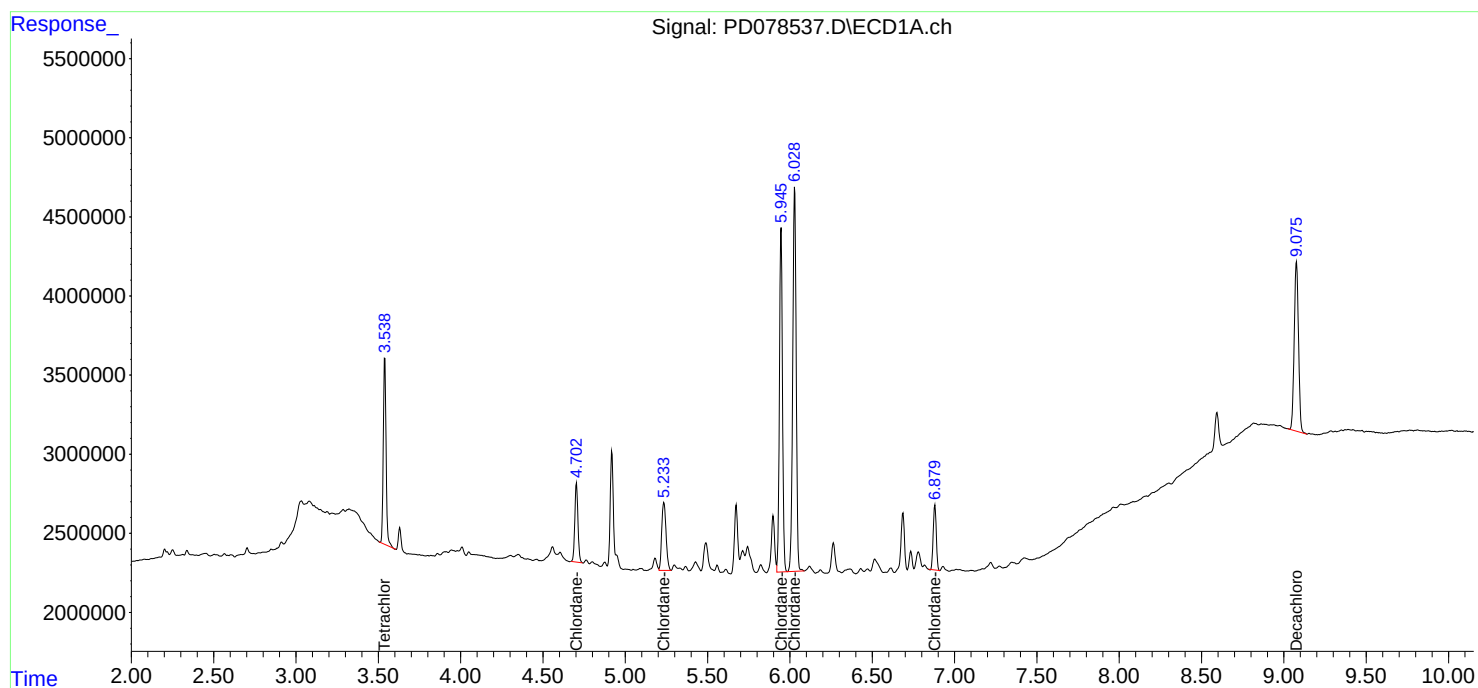


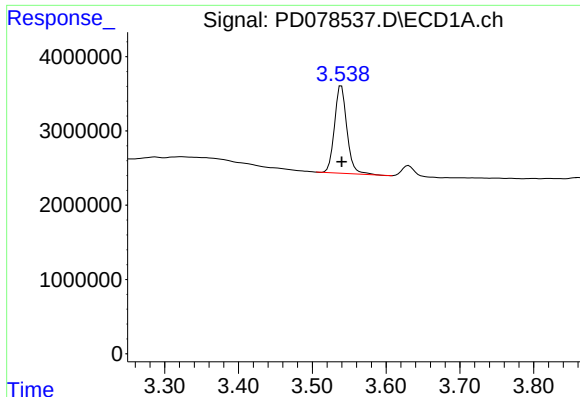

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 13809002
Conc: 5.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

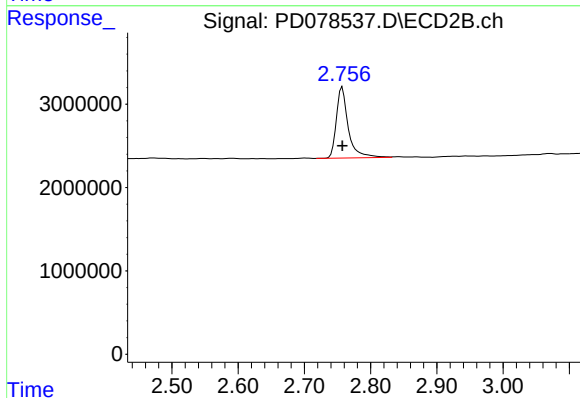


#1 Tetrachloro-m-xylene

R.T.: 2.757 min
Delta R.T.: 0.000 min
Response: 10627349
Conc: 4.84 ng/ml

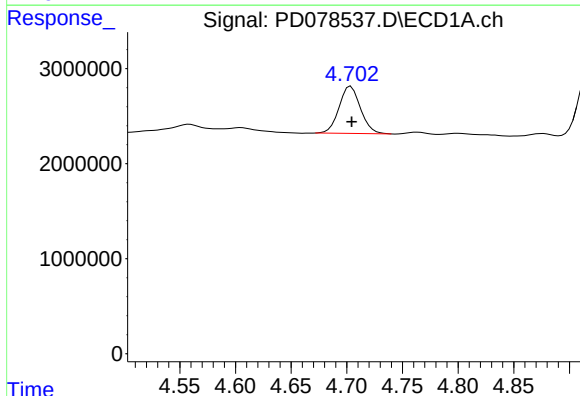


#23 Chlordane-1

R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 6630671
Conc: 50.80 ng/ml

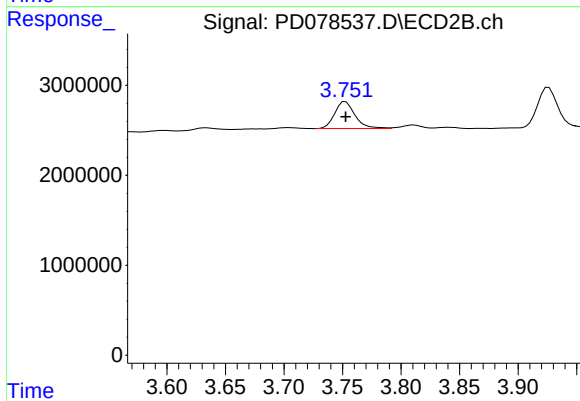

#23 Chlordane-1


R.T.: 3.753 min
Delta R.T.: 0.000 min
Response: 3644766
Conc: 50.53 ng/ml

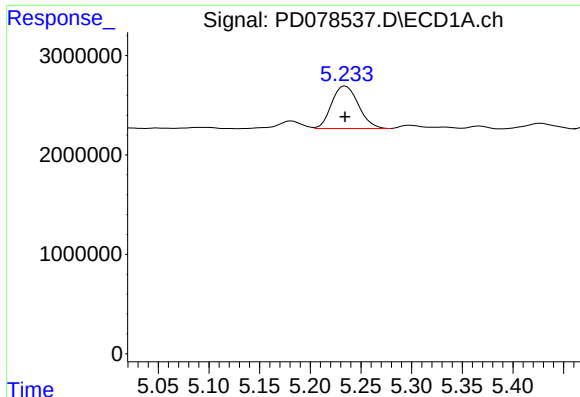

#24 Chlordane-2


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 7877694
Conc: 56.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

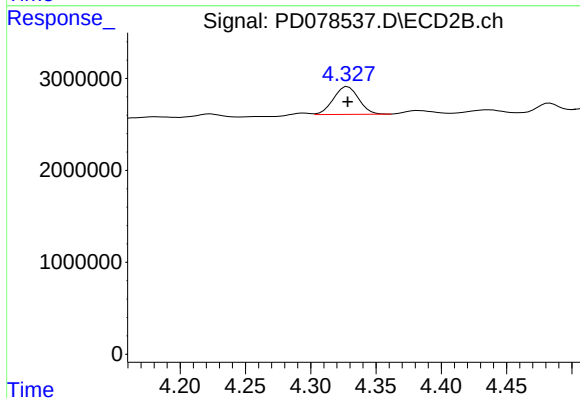


#24 Chlordane-2

R.T.: 4.328 min
Delta R.T.: 0.000 min
Response: 4046192
Conc: 53.33 ng/ml

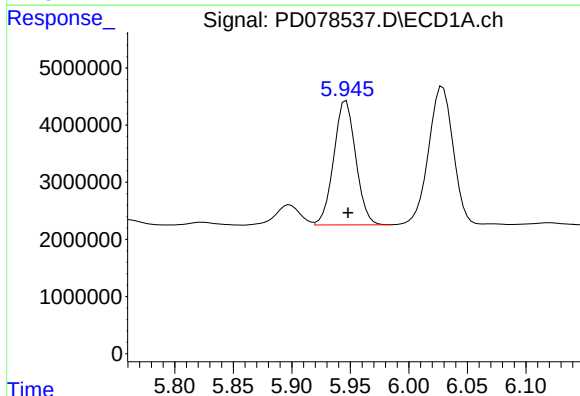


#25 Chlordane-3

R.T.: 5.946 min
Delta R.T.: -0.002 min
Response: 28329919
Conc: 48.32 ng/ml

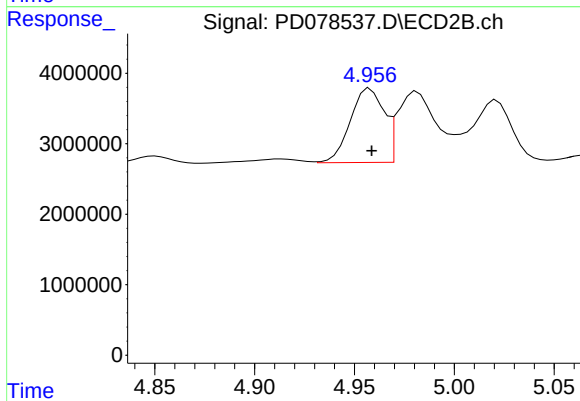

#25 Chlordane-3


R.T.: 4.958 min
Delta R.T.: 0.000 min
Response: 12292870
Conc: 47.97 ng/ml

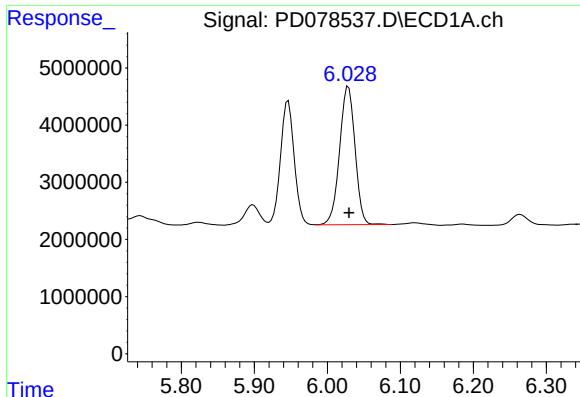

#26 Chlordane-4


R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 35459256
Conc: 50.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

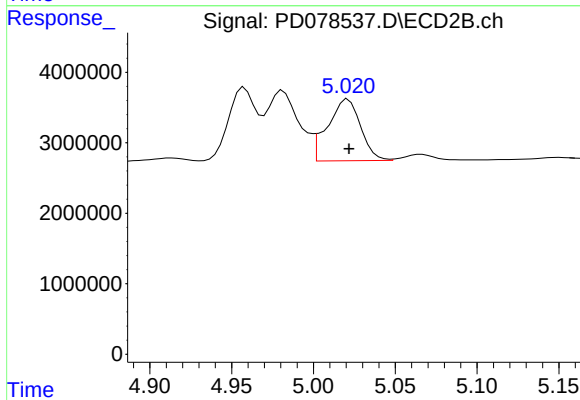


#26 Chlordane-4

R.T.: 5.021 min
Delta R.T.: 0.000 min
Response: 12257875
Conc: 49.13 ng/ml

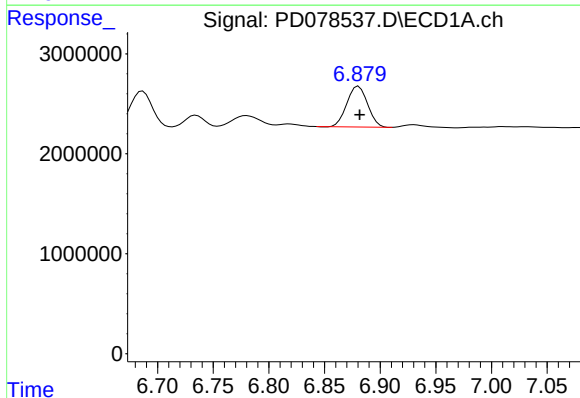


#27 Chlordane-5

R.T.: 6.881 min
Delta R.T.: -0.001 min
Response: 5266846
Conc: 47.20 ng/ml

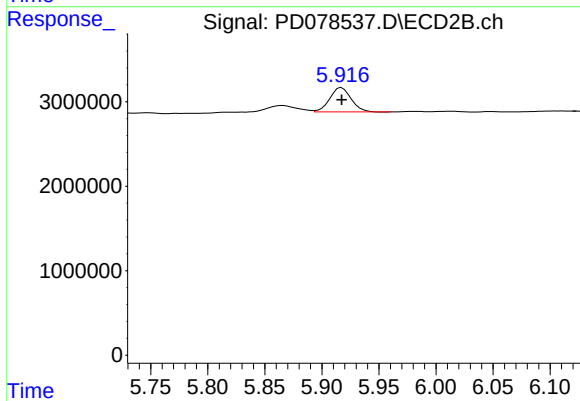

#27 Chlordane-5


R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 3727399
Conc: 42.42 ng/ml

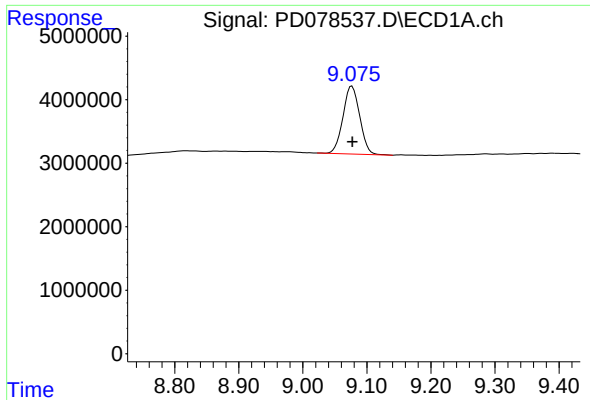

#28 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: 0.000 min
Response: 19333201
Conc: 5.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

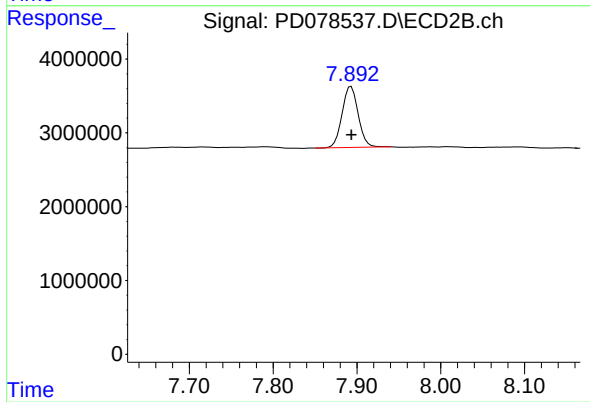

#28 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 11047981
Conc: 5.26 ng/ml