

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
 Data File : PD078527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 17:21
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:28:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 01:10:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.757	52354435	36735422	18.136	17.987
28)	SA Decachlor...	9.077	7.893	68095857	40516871	18.362	17.856
Target Compounds							
9)	A Endosulfan I	6.076	5.078	34779065	21853216	8.902	8.690
10)	B gamma-Chl...	5.947	4.957	38465445	24234865	9.160	9.018
12)	B 4,4'-DDE	6.199	5.210	72442583	45831687	18.099	18.013
13)	MA Dieldrin	6.352	5.342	72895707	48423643	17.376	17.346
19)	B Endosulfa...	7.168	6.315	57564579	39316935	17.916	17.722
20)	A Methoxychlor	7.508	6.591	152.6E6	99432965	91.418	91.137
21)	B Endrin ke...	7.655	6.820	64031000	45654508	17.822	17.395



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
Data File : PD078527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 17:21
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:28:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 01:10:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

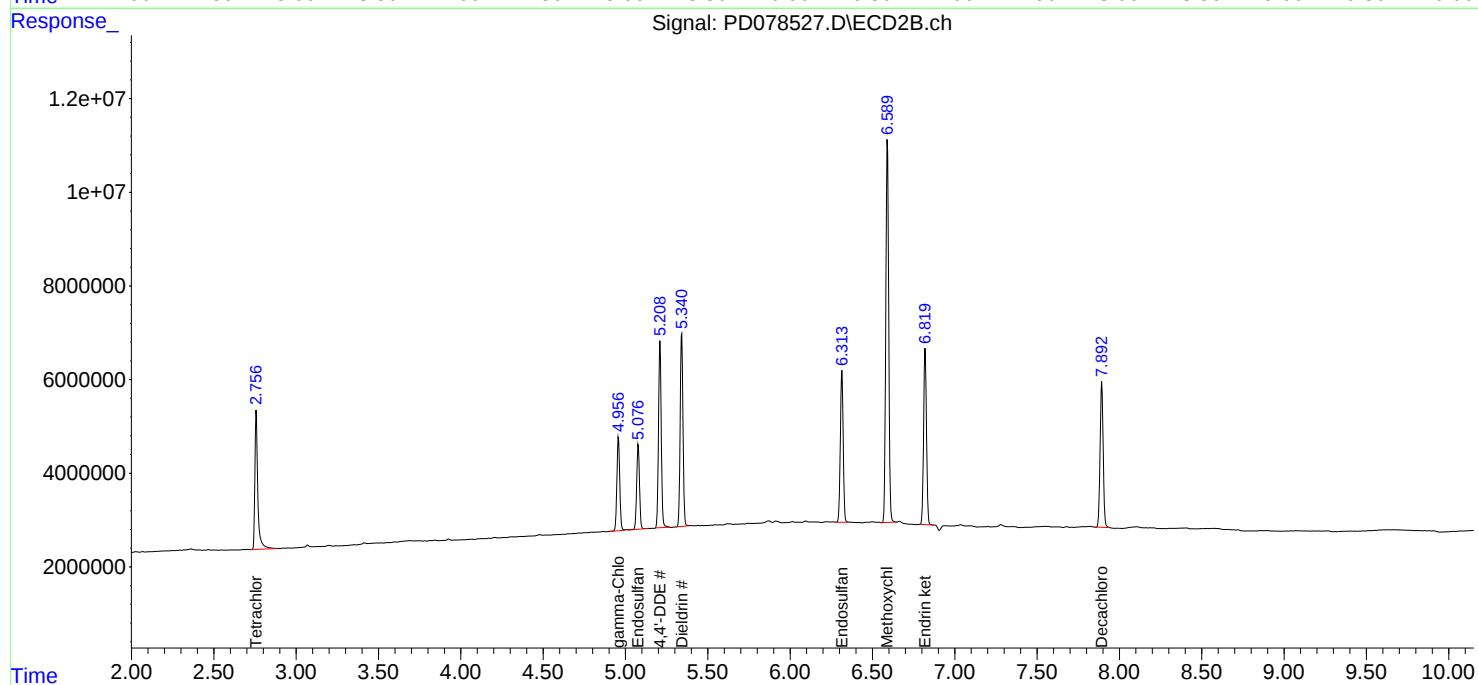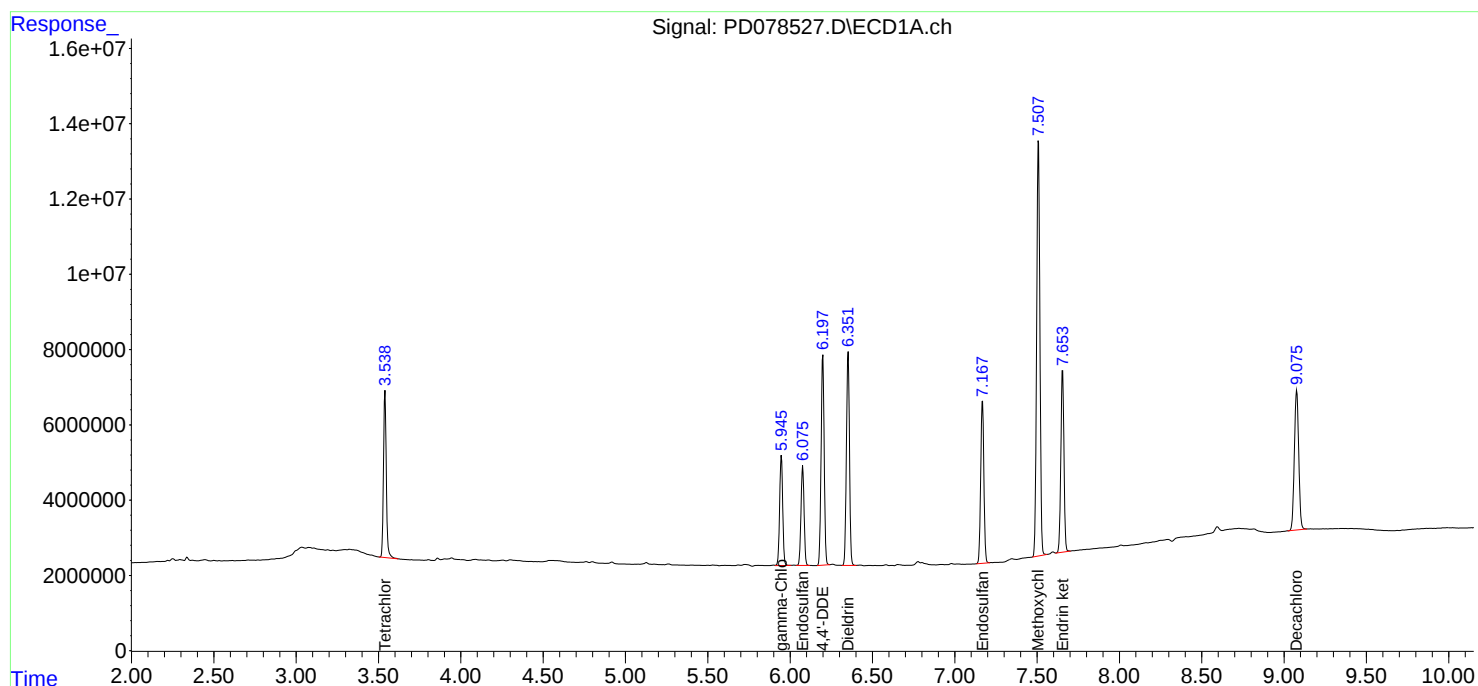


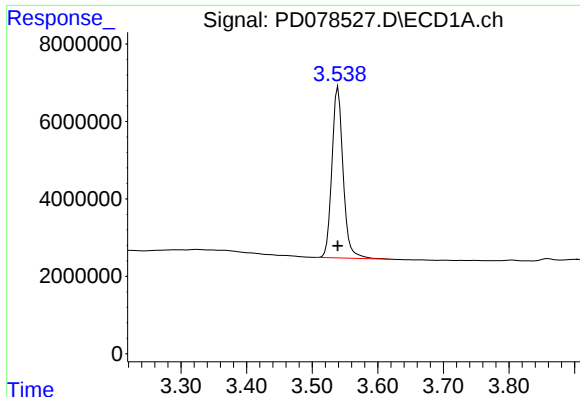

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 52354435
Conc: 18.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

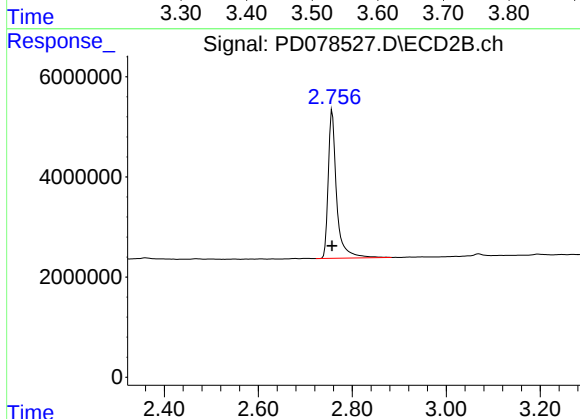


#1 Tetrachloro-m-xylene

R.T.: 2.757 min
Delta R.T.: 0.000 min
Response: 36735422
Conc: 17.99 ng/ml

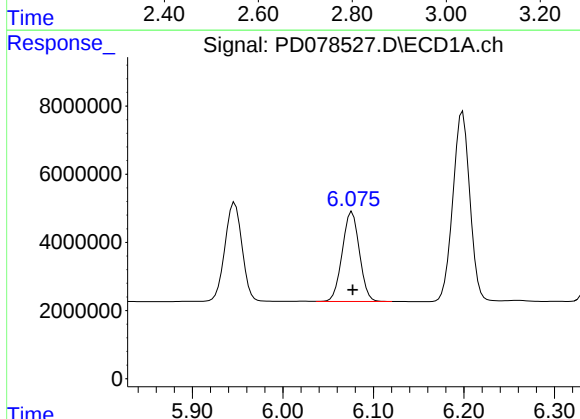


#9 Endosulfan I

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 34779065
Conc: 8.90 ng/ml

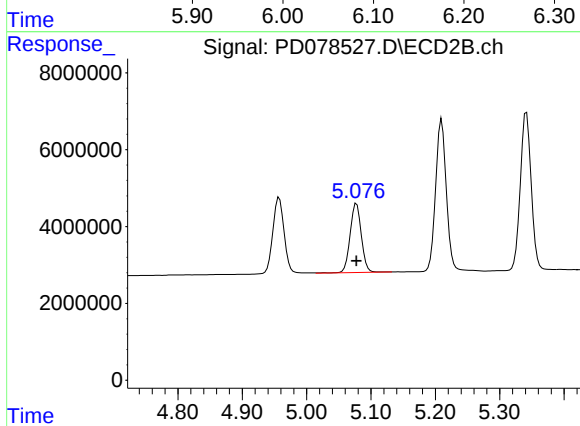

#9 Endosulfan I


R.T.: 5.078 min
Delta R.T.: 0.000 min
Response: 21853216
Conc: 8.69 ng/ml

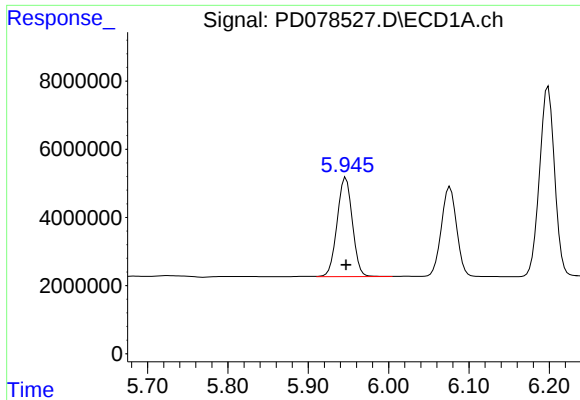

#10 gamma-Chlordane


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 38465445
Conc: 9.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

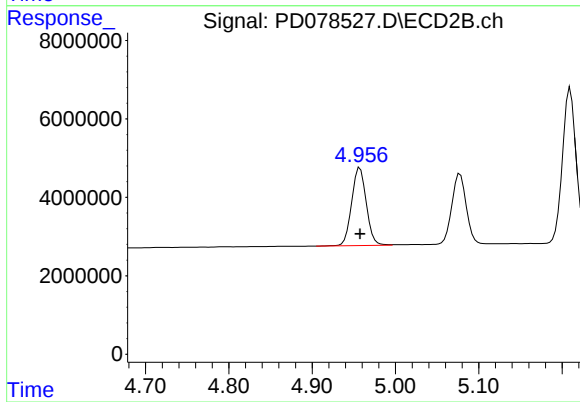


#10 gamma-Chlordane

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 24234865
Conc: 9.02 ng/ml

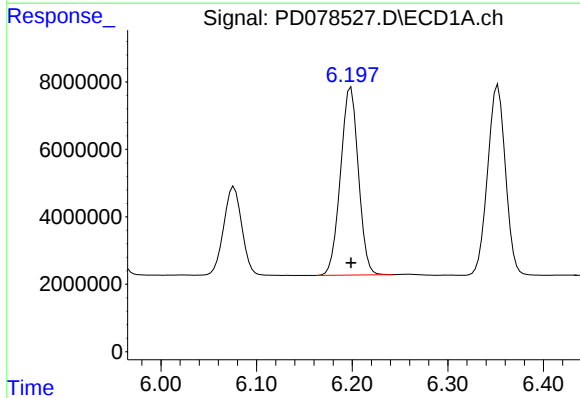


#12 4,4'-DDE

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 72442583
Conc: 18.10 ng/ml

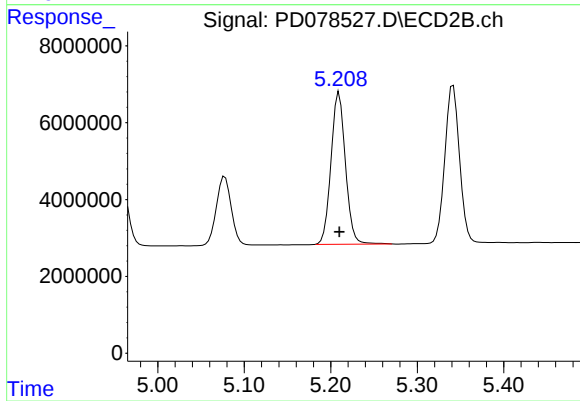

#12 4,4'-DDE


R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 45831687
Conc: 18.01 ng/ml

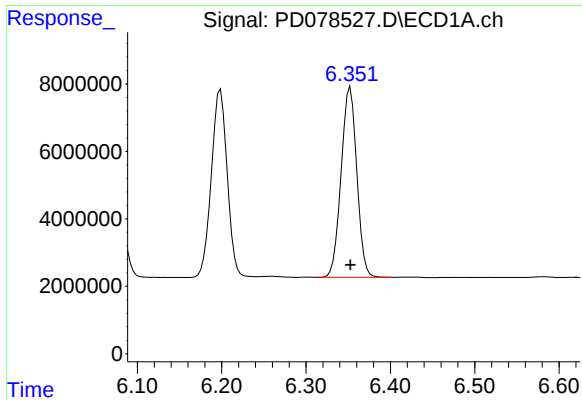

#13 Dieldrin


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 72895707
Conc: 17.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

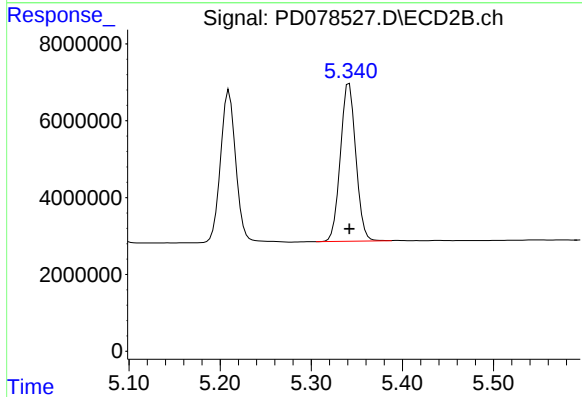


#13 Dieldrin

R.T.: 5.342 min
Delta R.T.: 0.000 min
Response: 48423643
Conc: 17.35 ng/ml

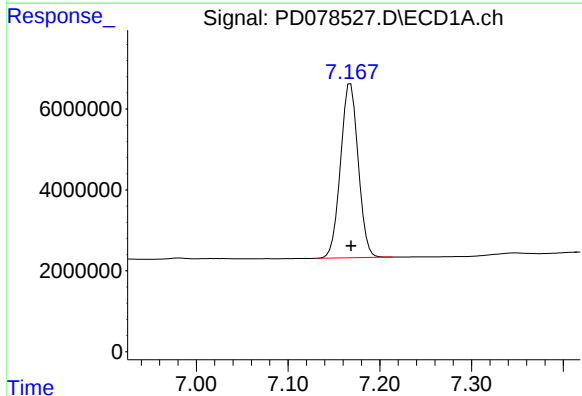


#19 Endosulfan Sulfate

R.T.: 7.168 min
Delta R.T.: 0.000 min
Response: 57564579
Conc: 17.92 ng/ml

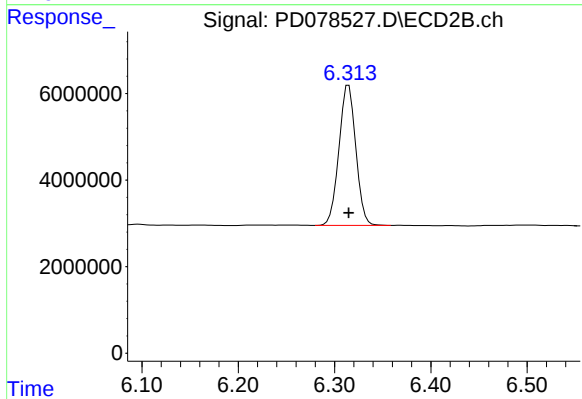

#19 Endosulfan Sulfate


R.T.: 6.315 min
Delta R.T.: 0.000 min
Response: 39316935
Conc: 17.72 ng/ml

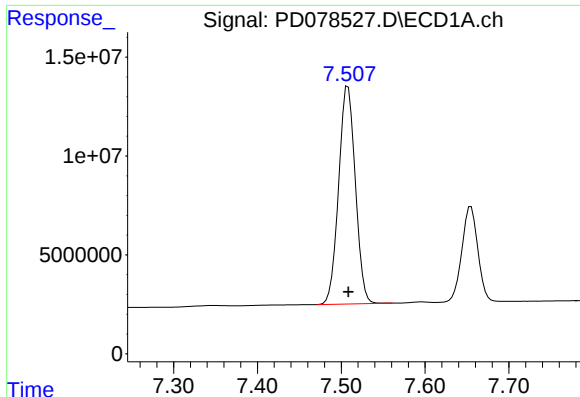

#20 Methoxychlor


R.T.: 7.508 min
Delta R.T.: 0.000 min
Response: 152570506
Conc: 91.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

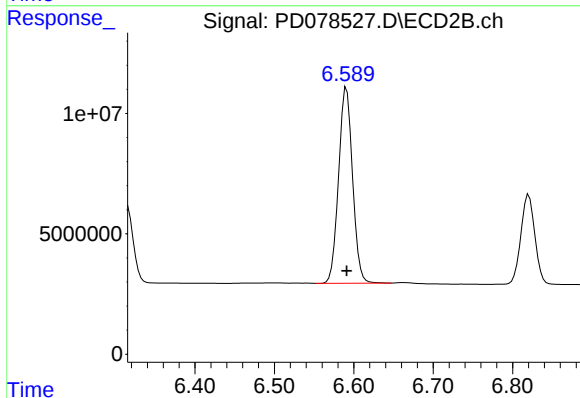


#20 Methoxychlor

R.T.: 6.591 min
Delta R.T.: 0.000 min
Response: 99432965
Conc: 91.14 ng/ml

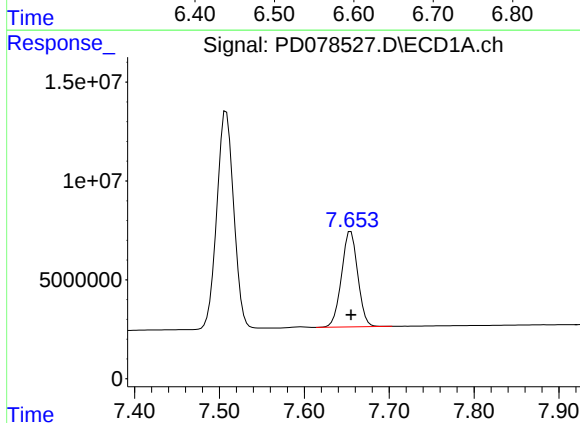


#21 Endrin ketone

R.T.: 7.655 min
Delta R.T.: 0.000 min
Response: 64031000
Conc: 17.82 ng/ml

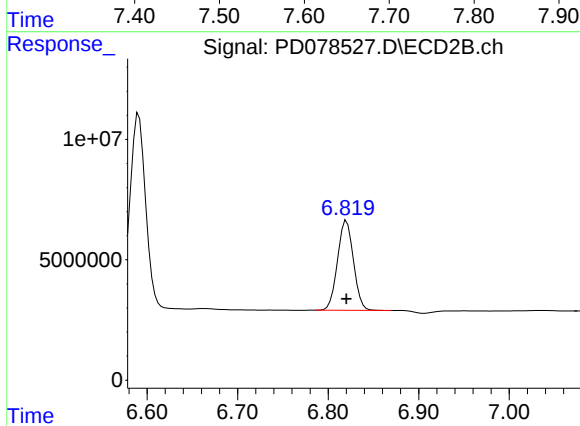

#21 Endrin ketone


R.T.: 6.820 min
Delta R.T.: 0.000 min
Response: 45654508
Conc: 17.39 ng/ml

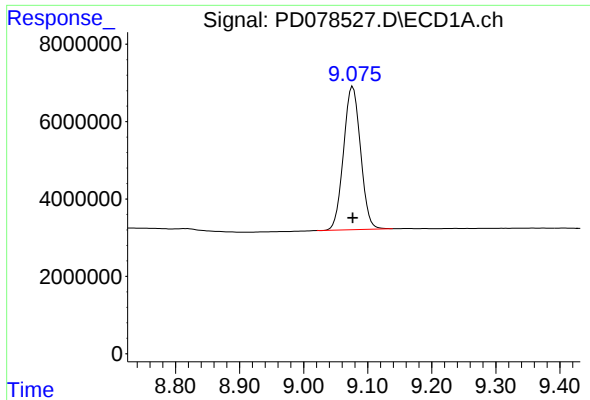

#28 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: 0.000 min
Response: 68095857
Conc: 18.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

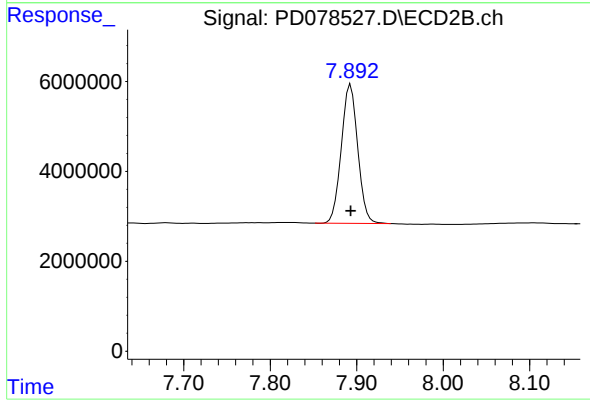

#28 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 40516871
Conc: 17.86 ng/ml