

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
 Data File : PD078553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 00:02
 Operator : AR\AJ
 Sample : 04667-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 FRAC-TANK-A2970

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/03/2023
 Supervised By : Ankita Jodhani 10/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:30:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 01:10:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.538	2.758	39297116	27481798	13.613m	13.456
2) SA Decachlor...	9.077	7.893	45479054	27243454	12.263	12.006

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
Data File : PD078553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 00:02
Operator : AR\AJ
Sample : 04667-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
FRAC-TANK-A2970


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/03/2023
Supervised By : Ankita Jodhani 10/03/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:30:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 01:10:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

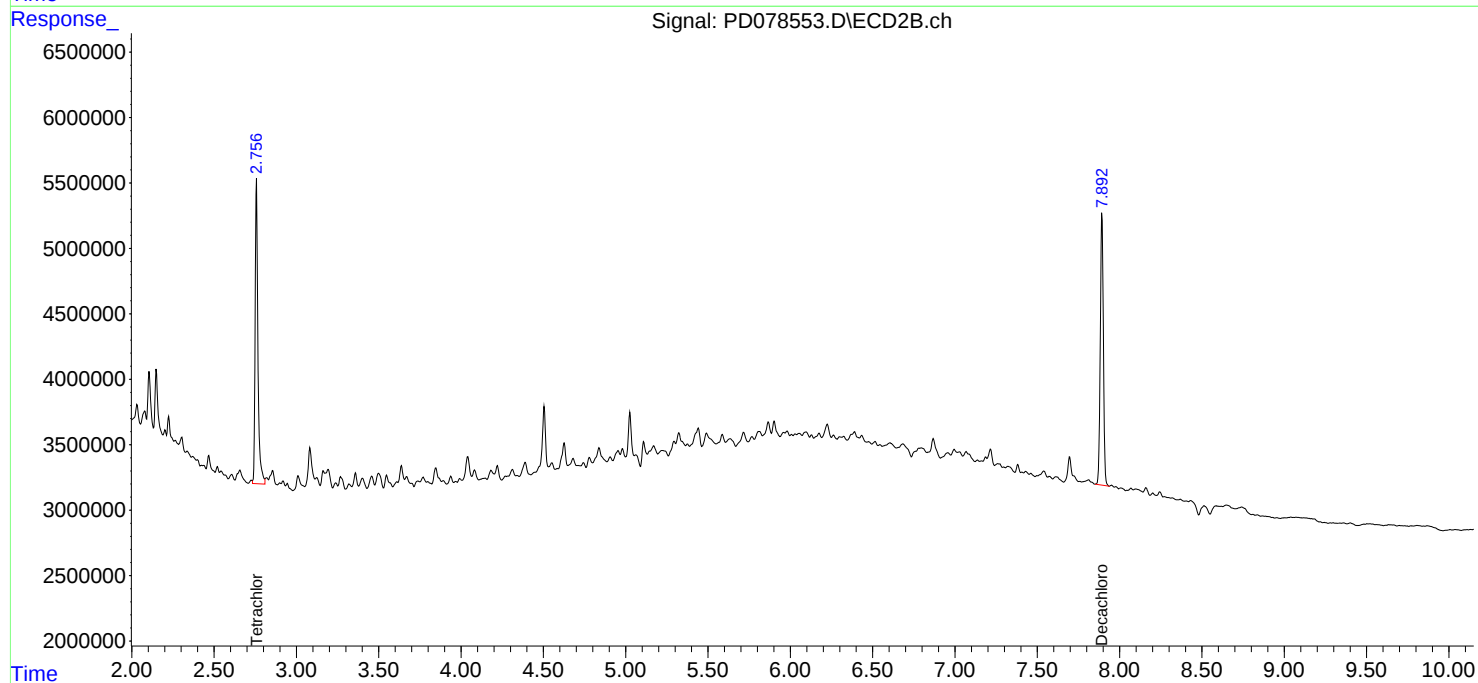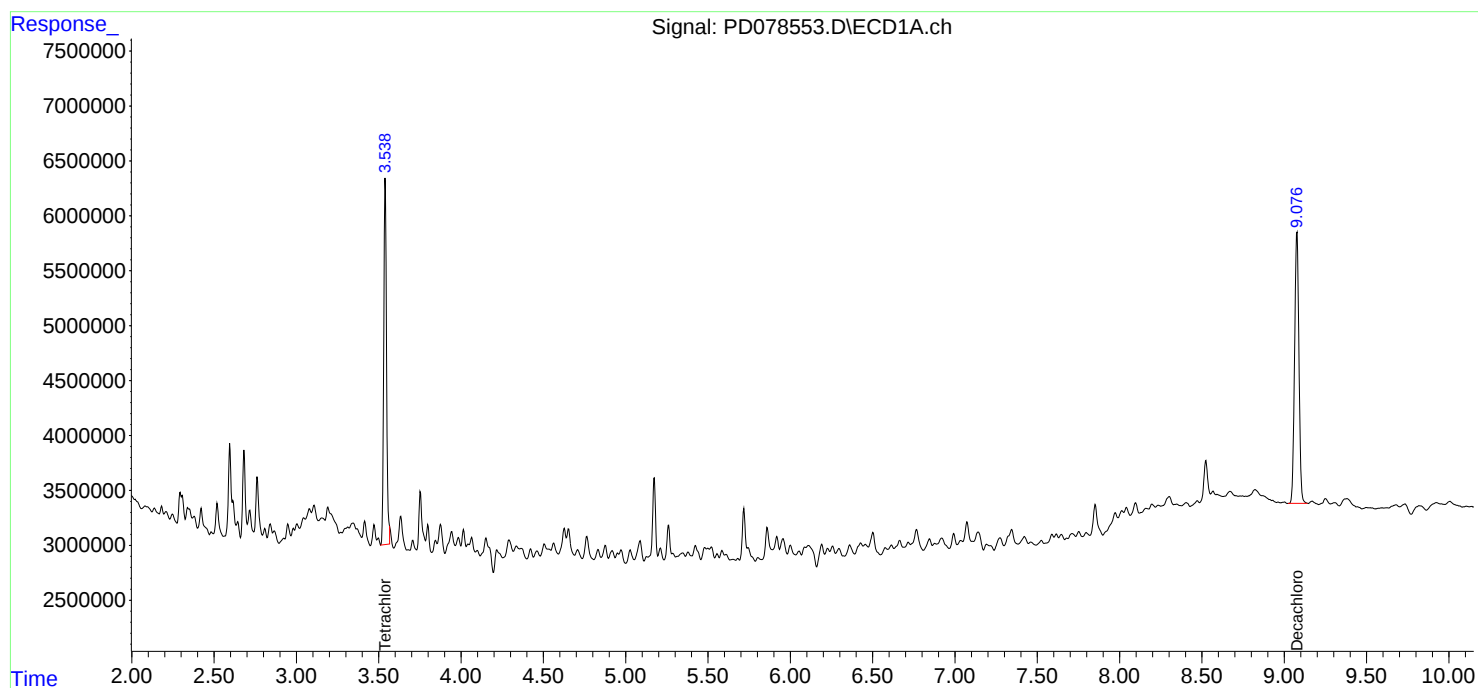

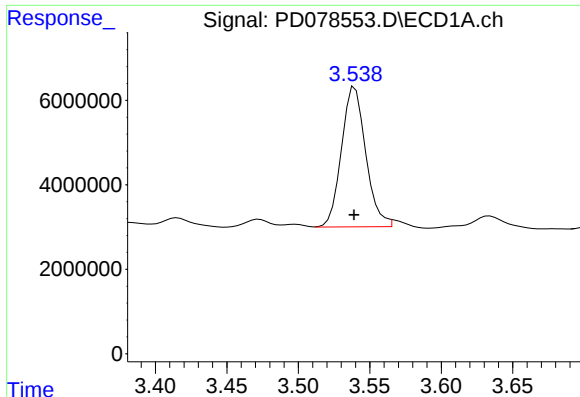


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 39297116
Conc: 13.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
FRAC-TANK-A2970


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2023
Supervised By :Ankita Jodhani 10/03/2023

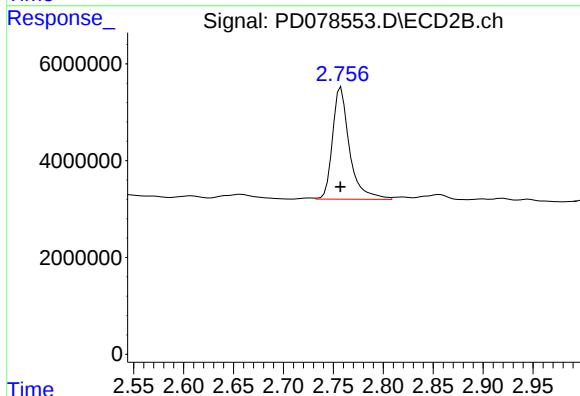


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: 0.000 min
Response: 27481798
Conc: 13.46 ng/ml

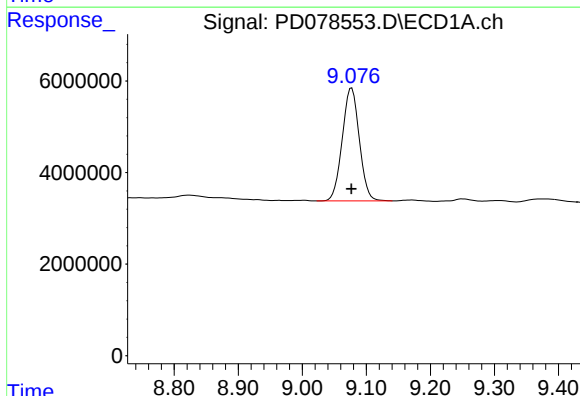

#28 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: 0.000 min
Response: 45479054
Conc: 12.26 ng/ml

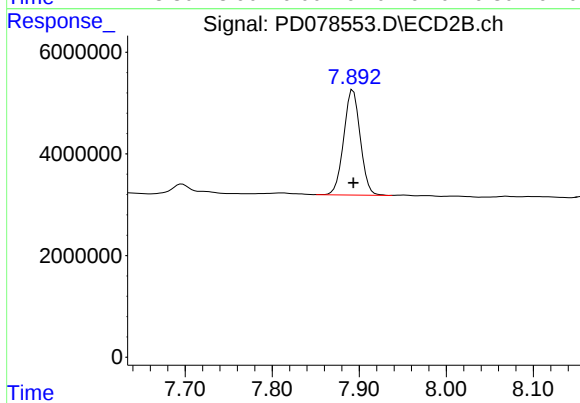

#28 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 27243454
Conc: 12.01 ng/ml