

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
 Data File : PD078555.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 00:29
 Operator : AR\AJ
 Sample : 04686-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WASTE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/03/2023
 Supervised By : Ankita Jodhani 10/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:31:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 01:10:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.760	21401592	9571373	7.414m	4.686 #
28)	SA Decachlor...	9.078	7.894	39130344	25196529	10.551	11.104
Target Compounds							
10)	B gamma-Chl...	5.948	4.959	513.0E6	178.0E6	122.179	66.232 #
11)	B alpha-Chl...	6.029	5.023	1146.3E6	406.0E6	272.081	151.183 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
Data File : PD078555.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 00:29
Operator : AR\AJ
Sample : 04686-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
WASTE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/03/2023
Supervised By : Ankita Jodhani 10/03/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:31:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 01:10:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

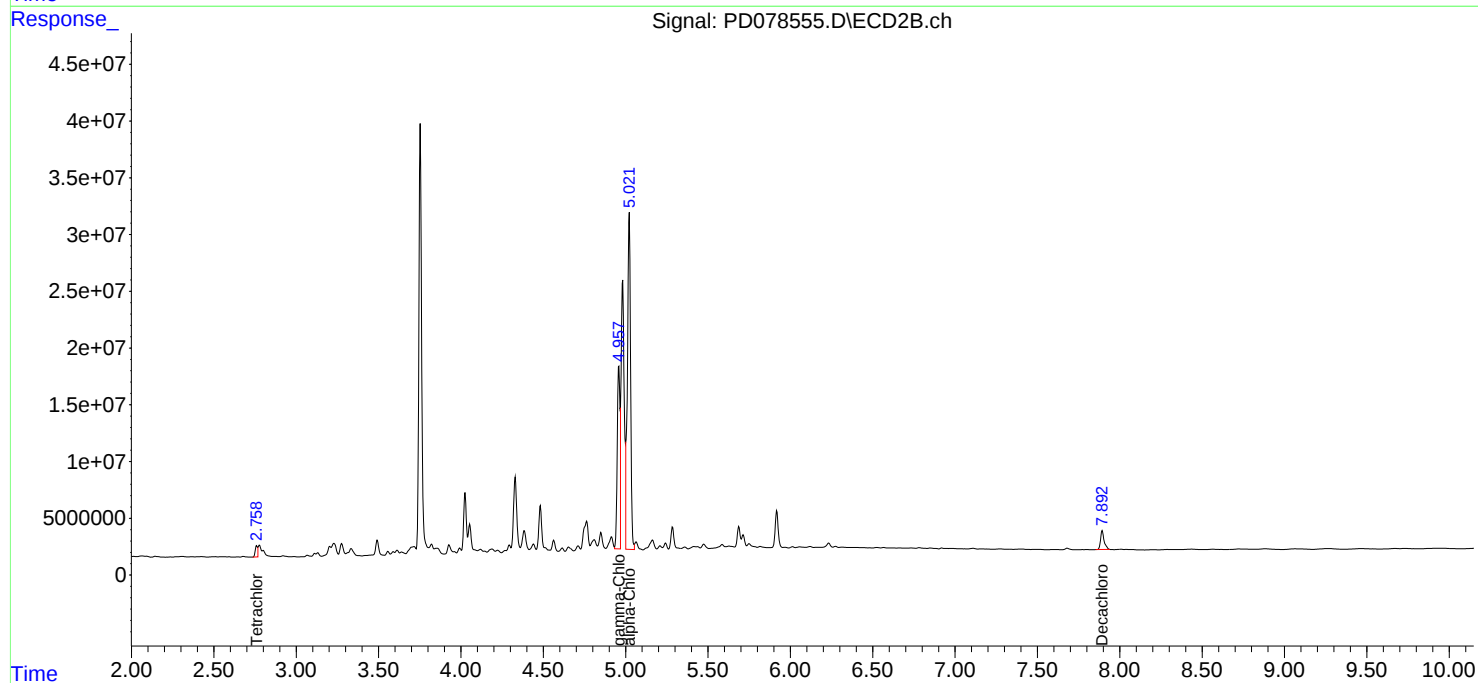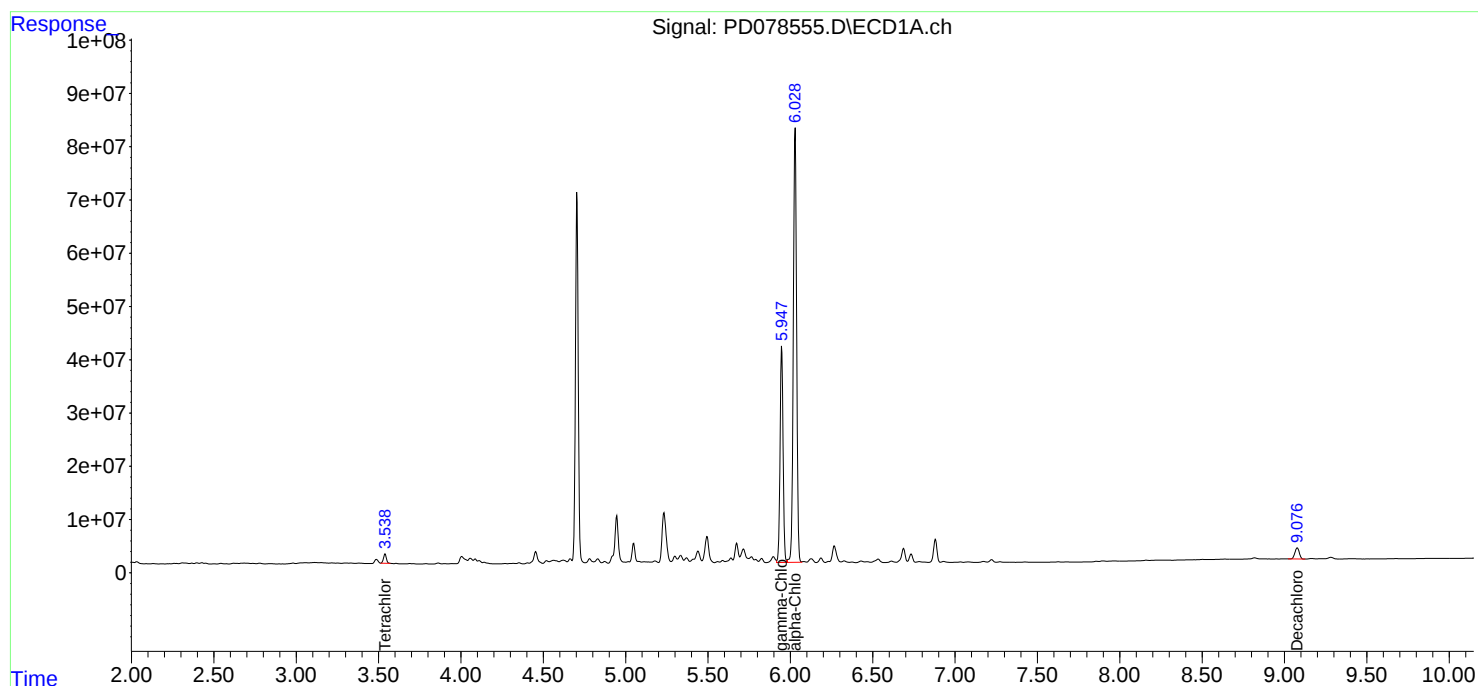

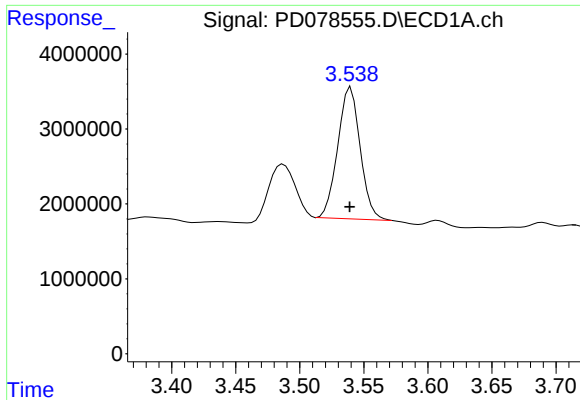


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 21401592
Conc: 7.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
WASTE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2023
Supervised By :Ankita Jodhani 10/03/2023

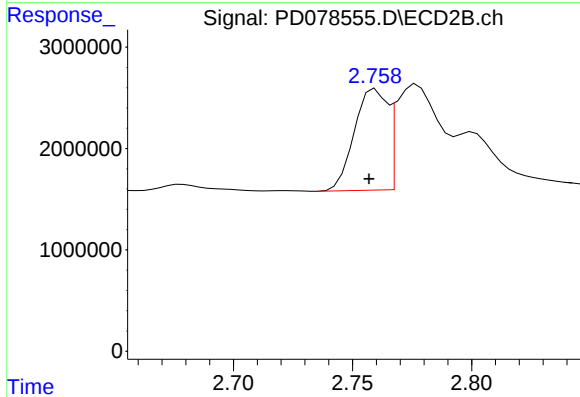


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.003 min
Response: 9571373
Conc: 4.69 ng/ml

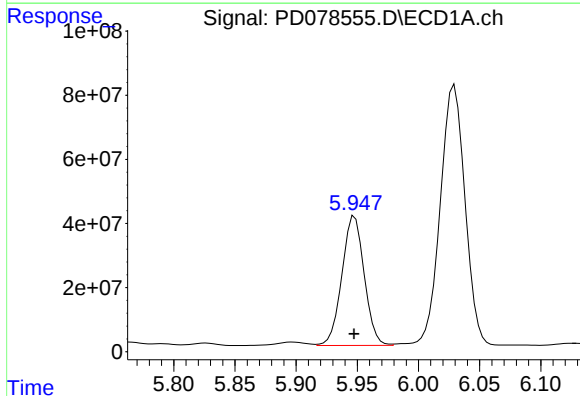


#10 gamma-Chlordane

R.T.: 5.948 min
Delta R.T.: 0.000 min
Response: 513044662
Conc: 122.18 ng/ml

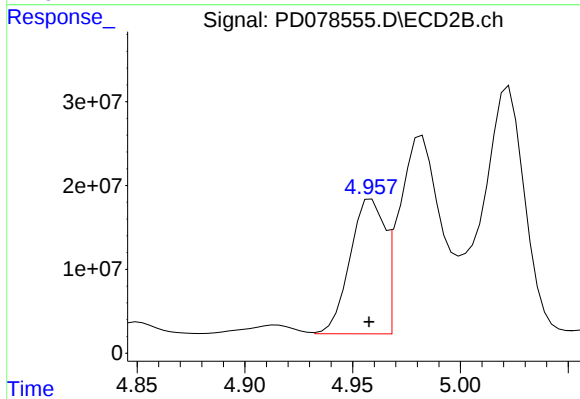

#10 gamma-Chlordane

R.T.: 4.959 min
Delta R.T.: 0.001 min
Response: 177989974
Conc: 66.23 ng/ml

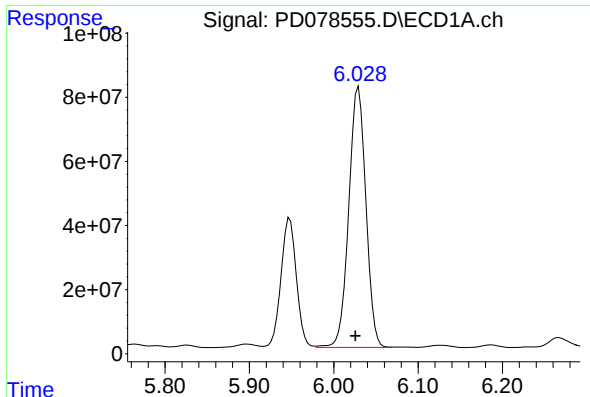


#11 alpha-Chlordane

R.T.: 6.029 min
Delta R.T.: 0.004 min
Response: 1146327394
Conc: 272.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
WASTE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2023
Supervised By :Ankita Jodhani 10/03/2023

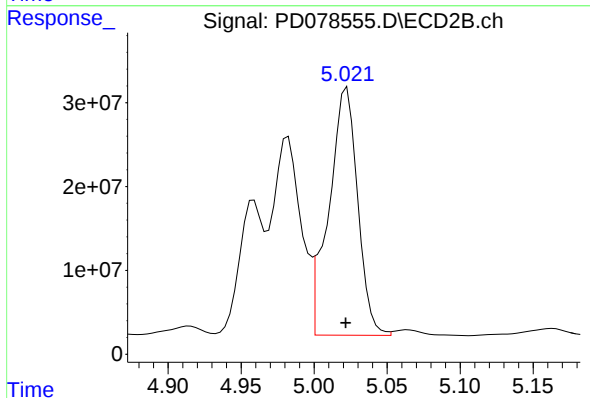


#11 alpha-Chlordane

R.T.: 5.023 min
Delta R.T.: 0.000 min
Response: 405958291
Conc: 151.18 ng/ml

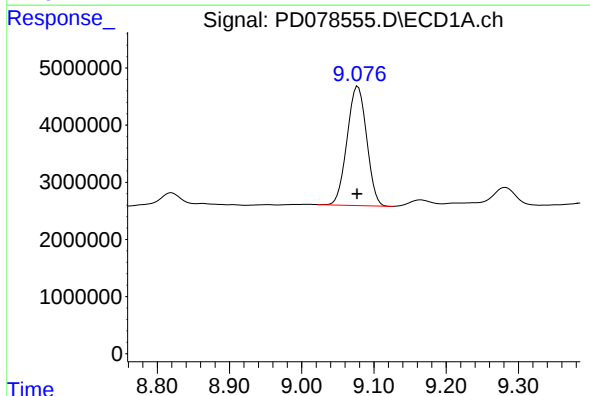

#28 Decachlorobiphenyl

R.T.: 9.078 min
Delta R.T.: 0.001 min
Response: 39130344
Conc: 10.55 ng/ml

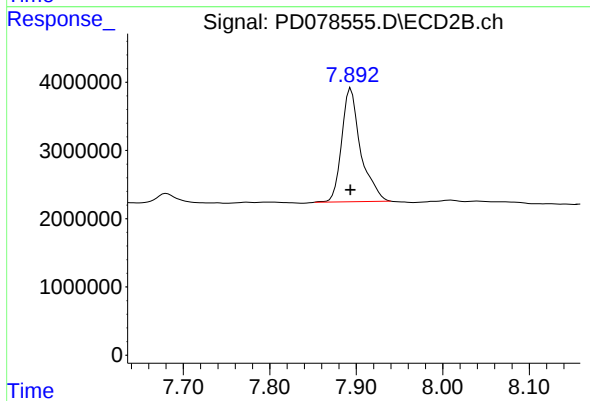

#28 Decachlorobiphenyl

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 25196529
Conc: 11.10 ng/ml