

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100324\
 Data File : PD085888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2024 14:37
 Operator : AR\AJ
 Sample : P4022-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC37

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/03/2024
 Supervised By :Ankita Jodhani 10/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:36:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 08:04:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.437	2.885	32315743	12520.2E6	28.247m	2952.500m#
2) SA Decachlor...	8.887	8.059	28256550	47747493	15.537	12.990
Target Compounds						
2) A alpha-BHC	3.880	3.382	123.2E6	388.4E6	59.167m	61.552m
7) B delta-BHC	4.643	4.248	134.9E6	349.7E6	70.187m	58.929
11) B cis-Chlor...	5.889	5.188	18237645	34117812	9.452	6.213 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100324\
Data File : PD085888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2024 14:37
Operator : AR\AJ
Sample : P4022-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:36:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

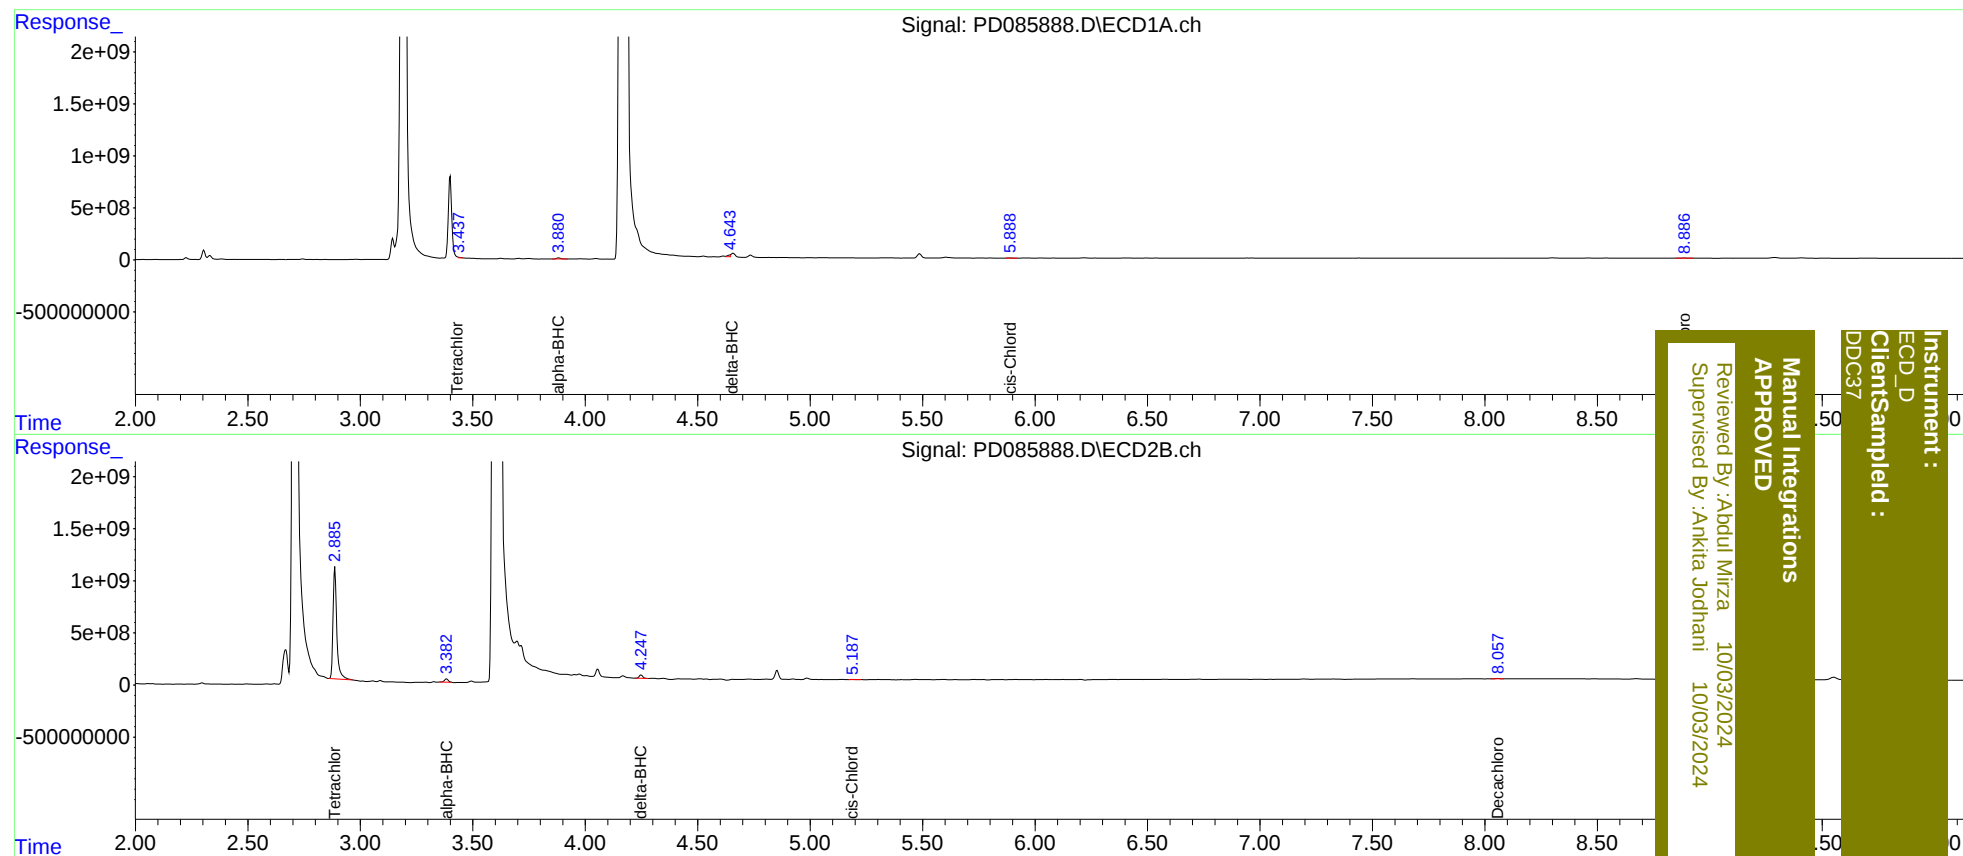

Instrument :
ECD_D
ClientSampled :
DDC37

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2024
Supervised By :Ankita Jodhani 10/03/2024