

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100324\
 Data File : PD085893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2024 15:45
 Operator : AR\AJ
 Sample : P4022-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DD6D6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/04/2024
 Supervised By : Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:37:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 08:04:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.443	2.886	30558961	4214.3E6	26.711m	993.804m#
27) SA Decachlor...	8.887	8.058	38182807	72764701	20.996m	19.796m
Target Compounds						
2) A alpha-BHC	3.882	3.384	606.8E6	1178.4E6	291.464	186.762 #
5) MB Aldrin	5.147	4.349	39054098	86640548	18.606m	14.744
7) B delta-BHC	4.640	4.248	800.7E6	1146.8E6	416.729	193.242 #
19) B Endosulfa...	7.021	6.476	21663492	12619800	13.757m	2.954 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100324\
Data File : PD085893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2024 15:45
Operator : AR\AJ
Sample : P4022-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:37:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

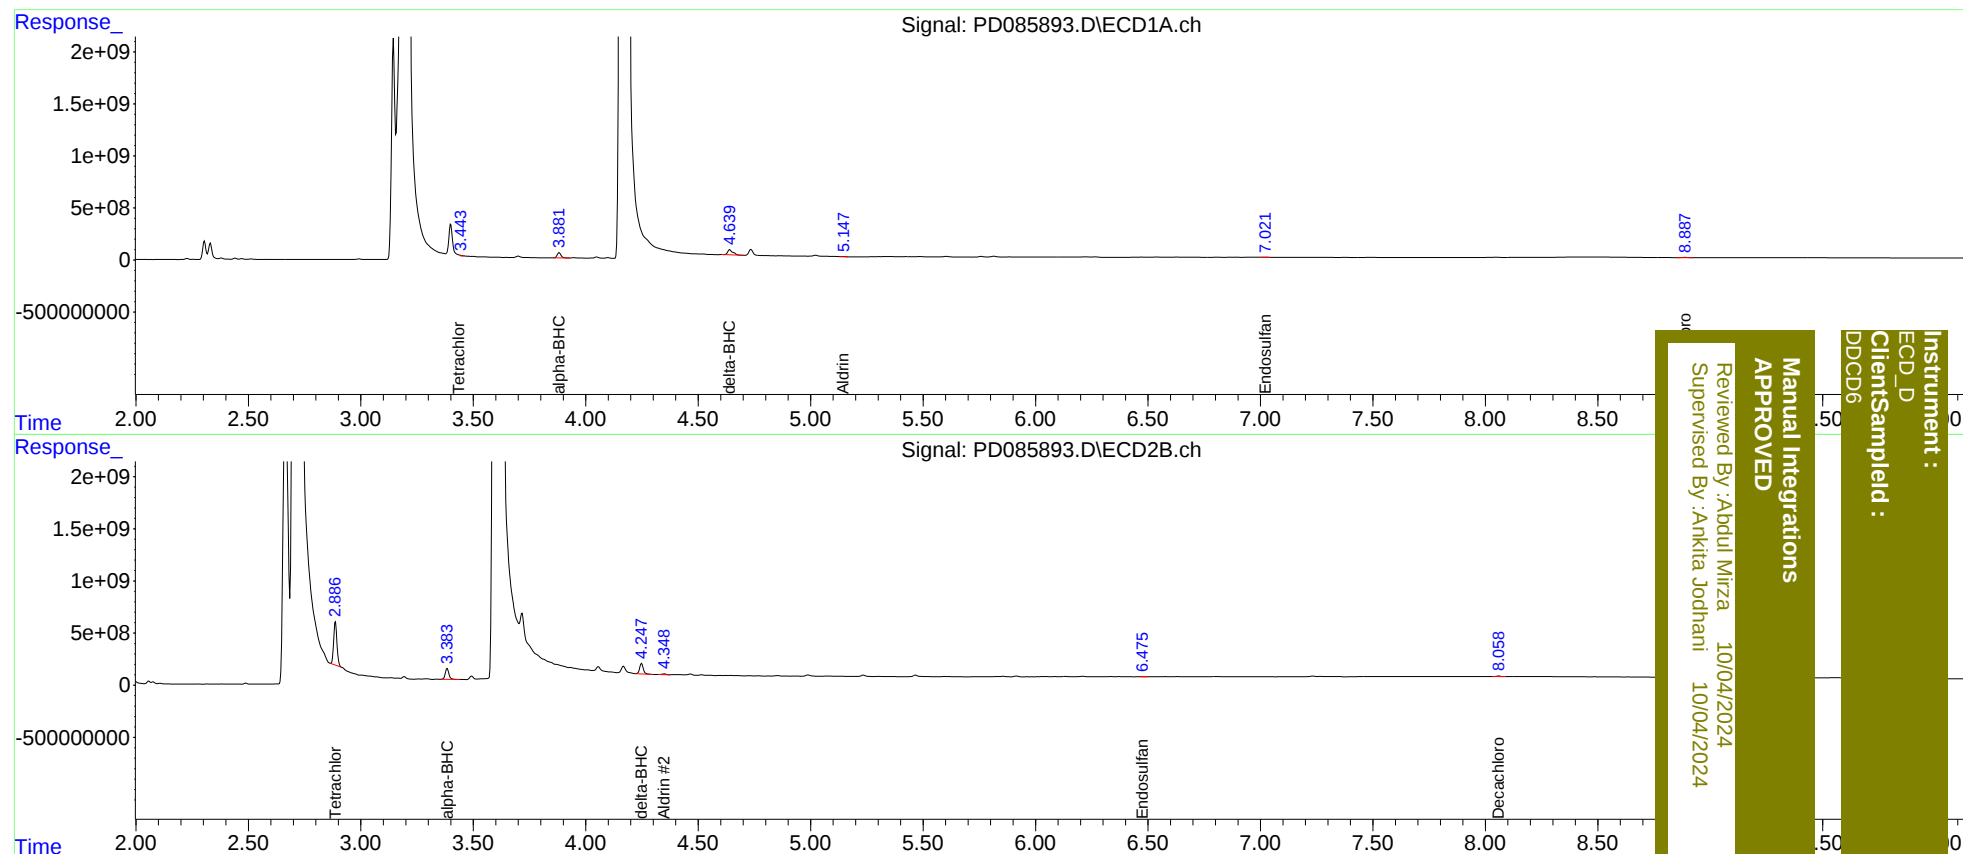

Reviewed By: Abdul Mirza 10/04/2024
Supervised By: Ankita Jodhani 10/04/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDCD6