

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100324\
 Data File : PD085895.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2024 16:12
 Operator : AR\AJ
 Sample : P4022-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCA6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/04/2024
 Supervised By : Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:38:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 08:04:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	2.886	28122272	2795.1E6	24.581m	659.144m#
27)	SA Decachlor...	8.888	8.060	34817535	69028445	19.145	18.779
Target Compounds							
2)	A alpha-BHC	3.882	3.384	280.3E6	532.8E6	134.640	84.446 #
7)	B delta-BHC	4.639	4.248	300.0E6	592.7E6	156.154m	99.871 #
16)	A 4,4'-DDD	6.562	5.916	3877998	17574028	3.110m	4.492m#
19)	B Endosulfa...	7.018	6.481	11502683	17725352	7.305m	4.149 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100324\
Data File : PD085895.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2024 16:12
Operator : AR\AJ
Sample : P4022-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:38:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

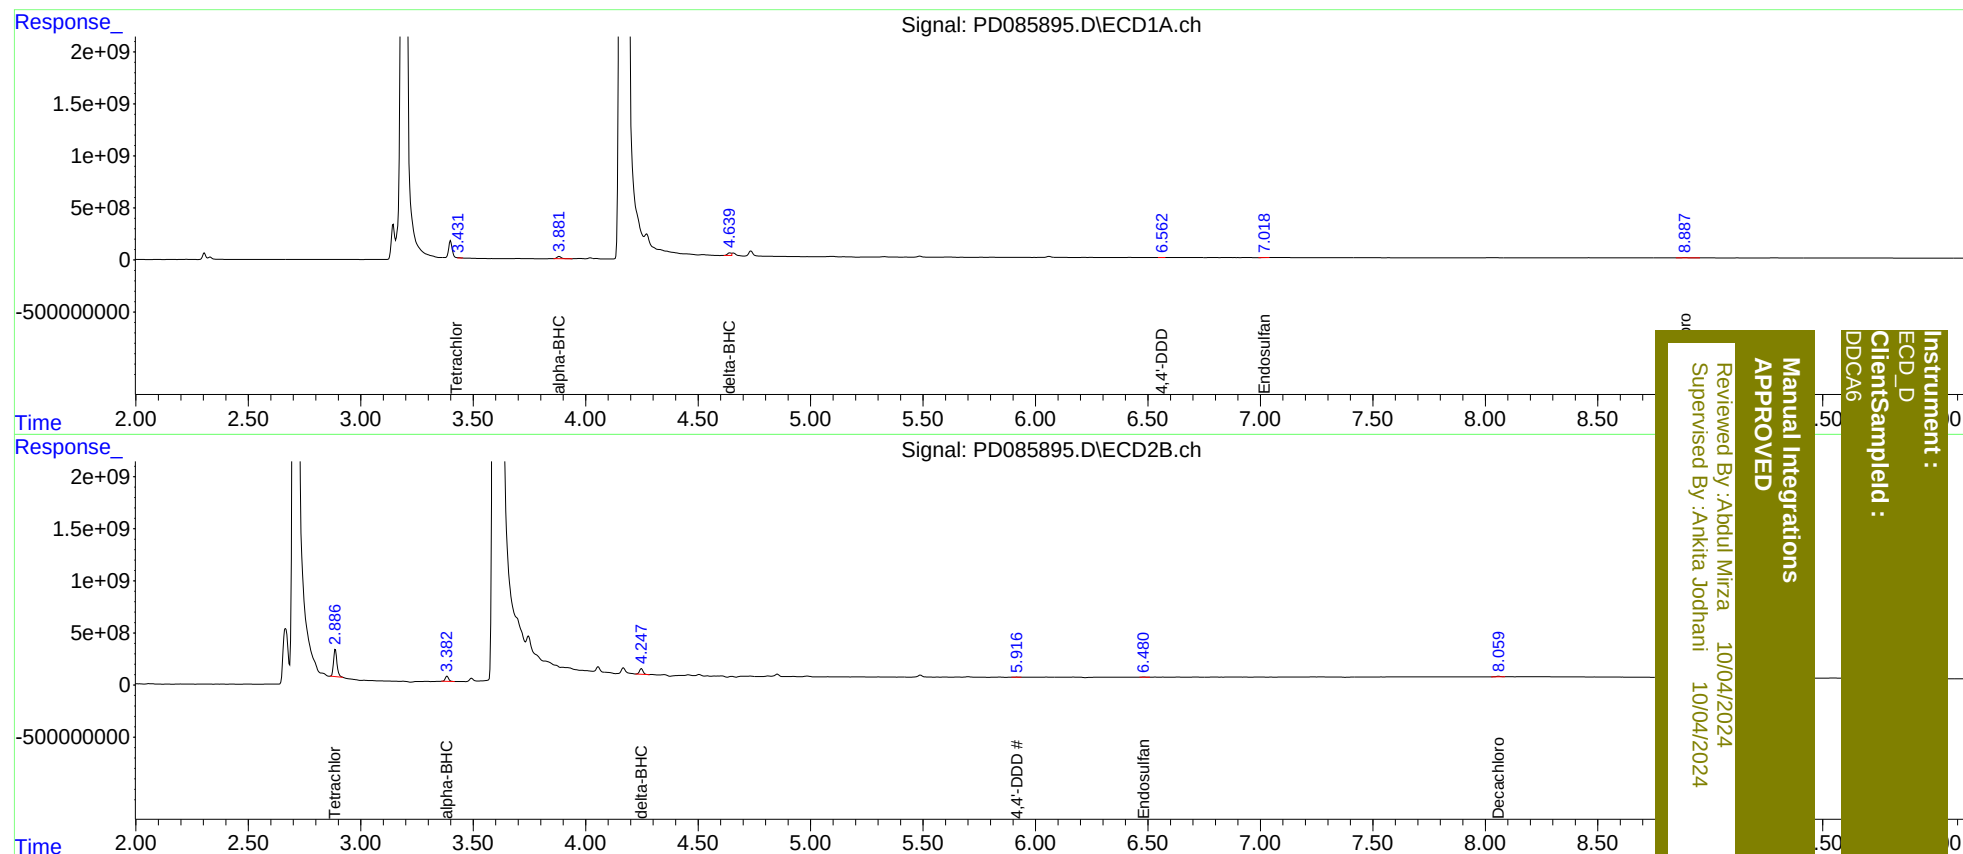

Reviewed By: Abdul Mirza 10/04/2024
Supervised By: Ankita Jodhani 10/04/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DDCA6