

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100419\
 Data File : PD055178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2019 08:55
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 00:56:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) A	alpha-BHC	3.769f	0.000	970632	0	0.874	N.D.	#
3) MA	gamma-BHC...	4.004	0.000	54286	0	<MDL	N.D.	#
4) MA	Heptachlor	4.295	0.000	422096	0	0.456	N.D.	#
5) MB	Aldrin	4.529	0.000	317433	0	0.326	N.D.	#
7) B	delta-BHC	4.442	0.000	28971	0	<MDL	N.D.	#
8) B	Heptachlo...	4.963	0.000	2135677	0	2.327	N.D.	#
9) A	Endosulfan I	5.258	0.000	121192	0	0.137	N.D.	#
10) B	trans-Chl...	5.198	0.000	61464	0	<MDL	N.D.	#
11) B	cis-Chlor...	5.258	0.000	121192	0	0.132	N.D.	#
12) B	4,4'-DDE	5.421	0.000	100850	0	0.112	N.D.	#
14) MA	Endrin	5.744f	0.000	560760	0	0.674	N.D.	#
19) B	Endosulfa...	6.487f	0.000	104970	0	0.129	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100419\
Data File : PD055178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2019 08:55
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 00:56:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

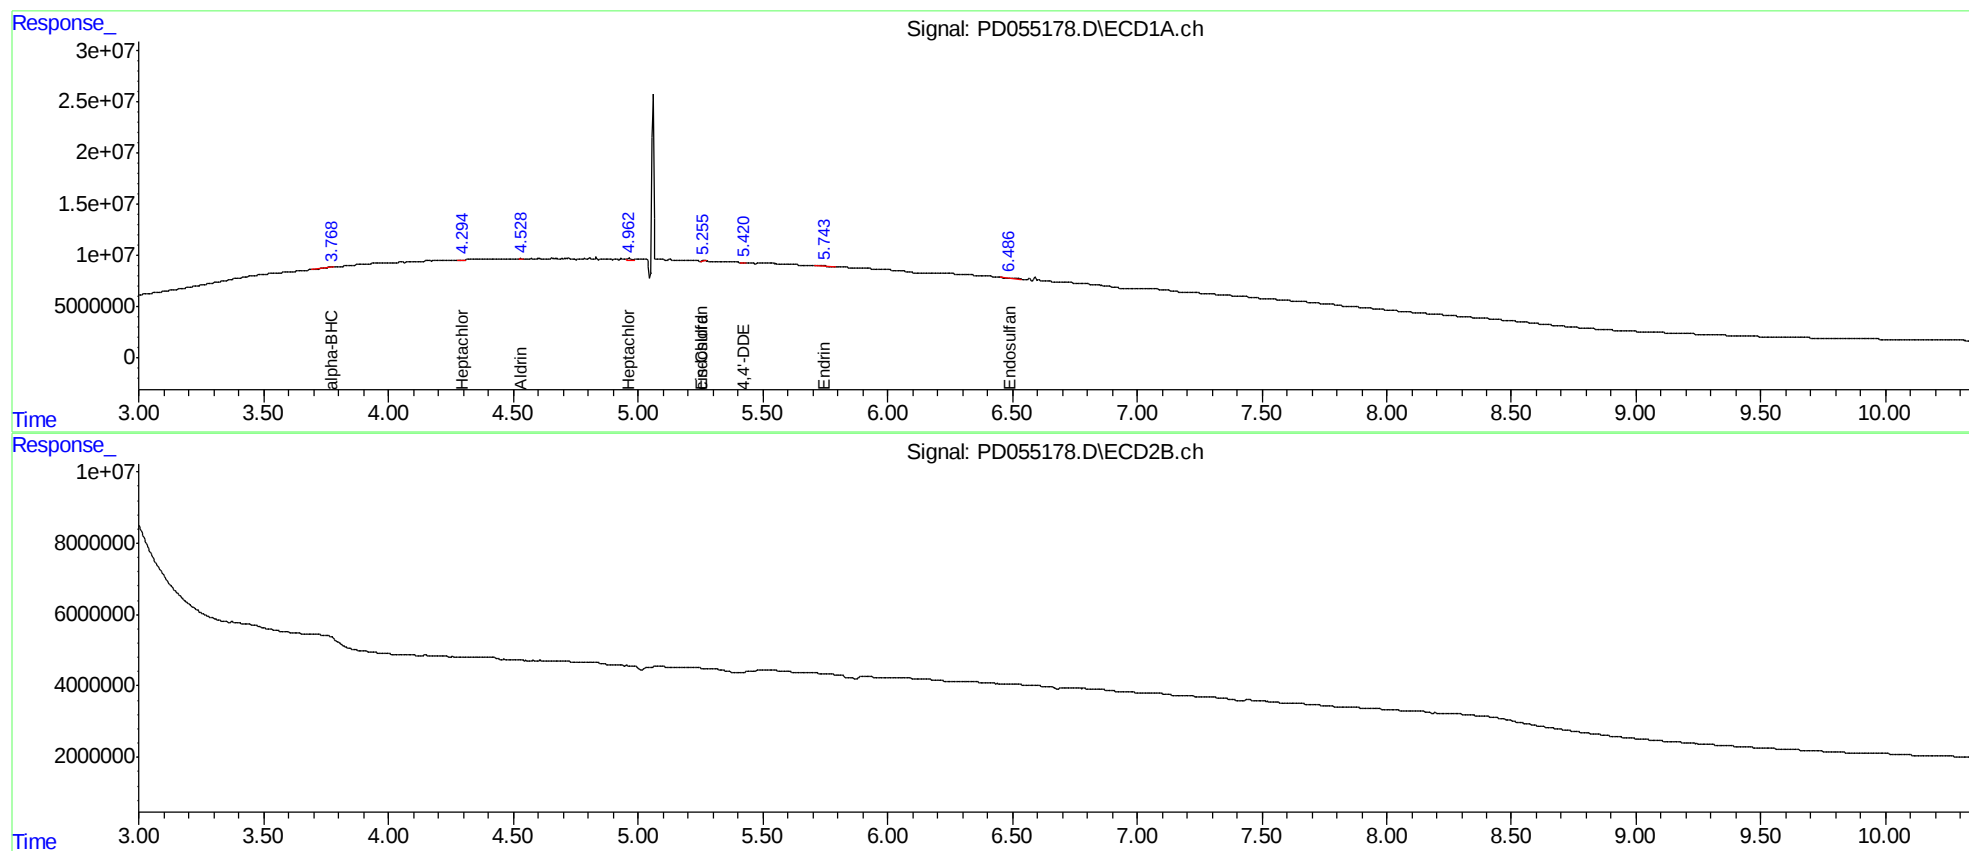


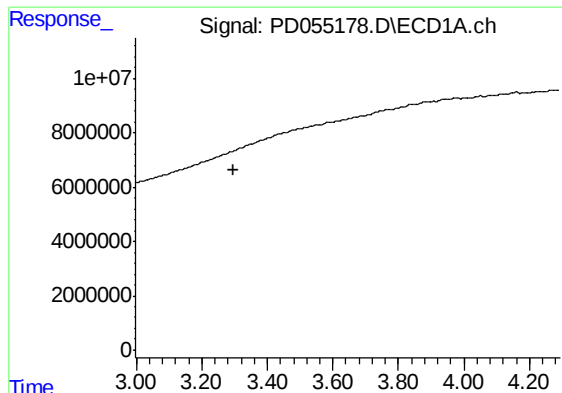

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.295 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

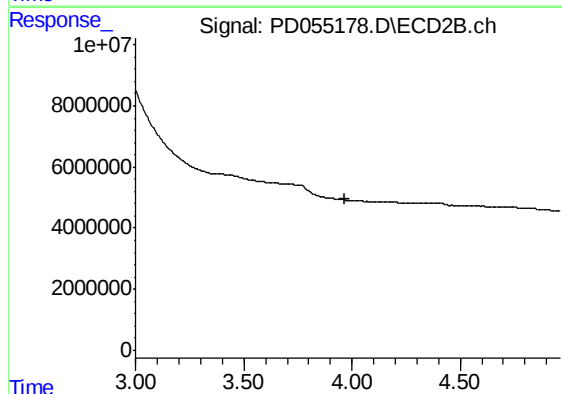


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.966 min
Response: 0
Conc: N.D.

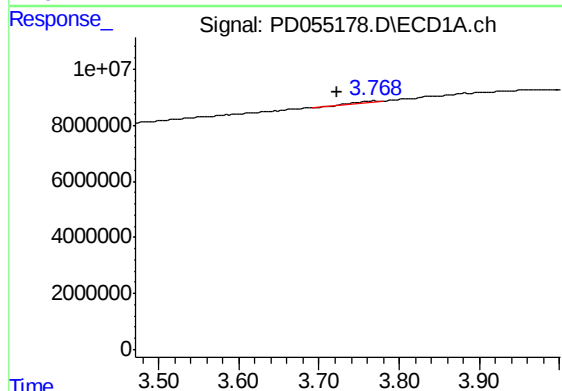


#2 alpha-BHC

R.T.: 3.769 min
Delta R.T.: 0.047 min
Response: 970632
Conc: 0.87 ng/ml

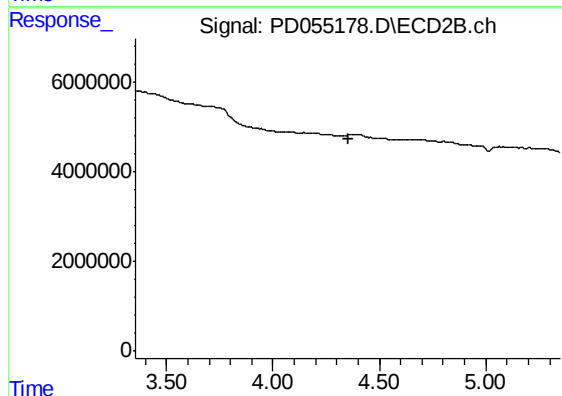

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.353 min
Response: 0
Conc: N.D.

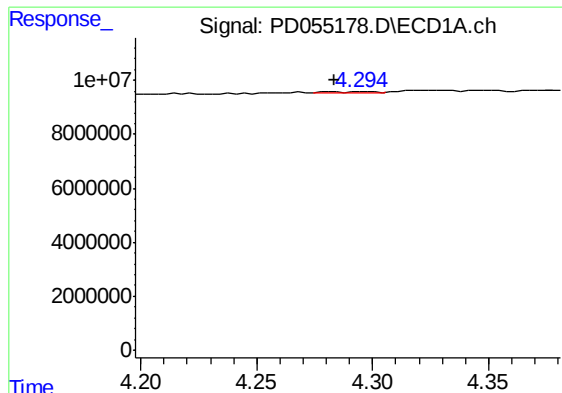

#4 Heptachlor


R.T.: 4.295 min
Delta R.T.: 0.011 min
Response: 422096
Conc: 0.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

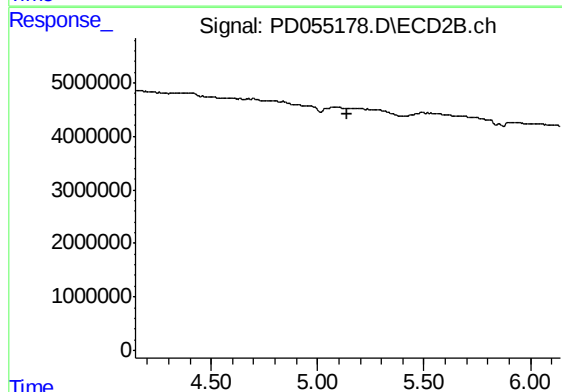


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.142 min
Response: 0
Conc: N.D.

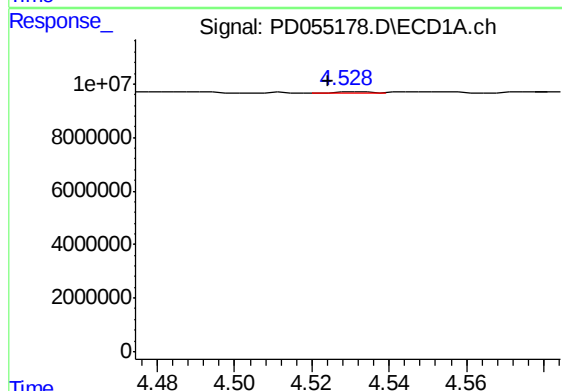


#5 Aldrin

R.T.: 4.529 min
Delta R.T.: 0.005 min
Response: 317433
Conc: 0.33 ng/ml

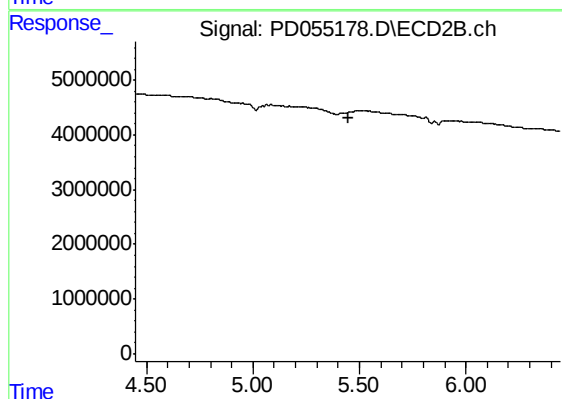

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.447 min
Response: 0
Conc: N.D.

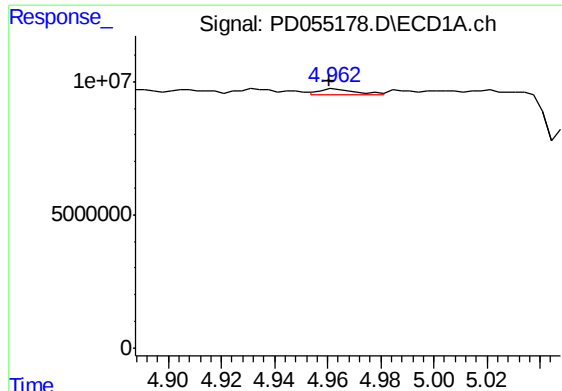

#8 Heptachlor epoxide


R.T.: 4.963 min
Delta R.T.: 0.002 min
Response: 2135677
Conc: 2.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

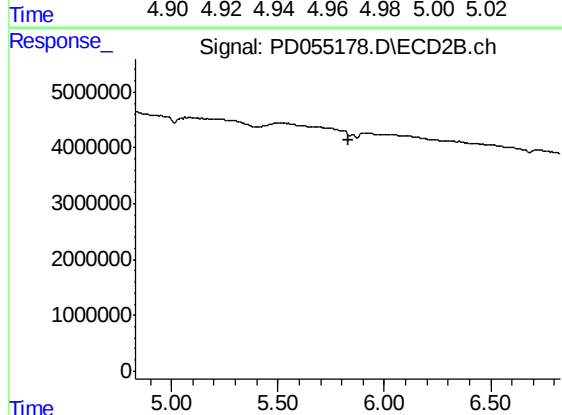


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.831 min
Response: 0
Conc: N.D.

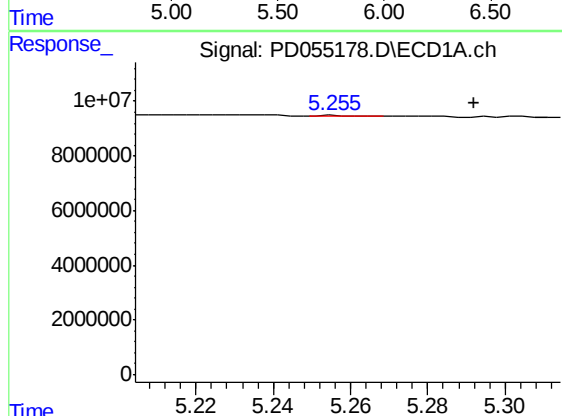


#9 Endosulfan I

R.T.: 5.258 min
Delta R.T.: -0.034 min
Response: 121192
Conc: 0.14 ng/ml

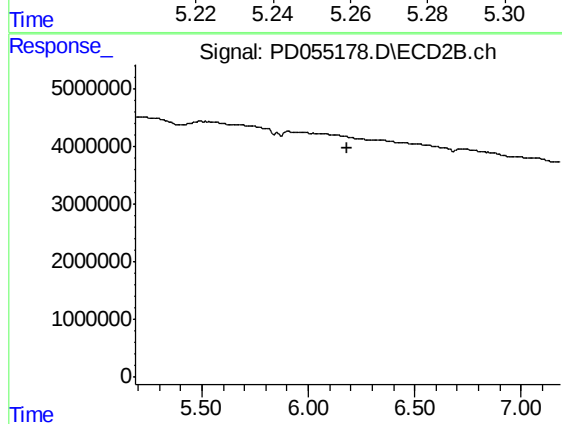

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.185 min
Response: 0
Conc: N.D.

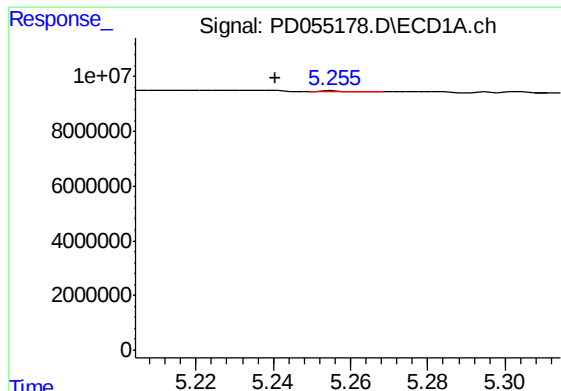

#11 cis-Chlordane


R.T.: 5.258 min
Delta R.T.: 0.017 min
Response: 121192
Conc: 0.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

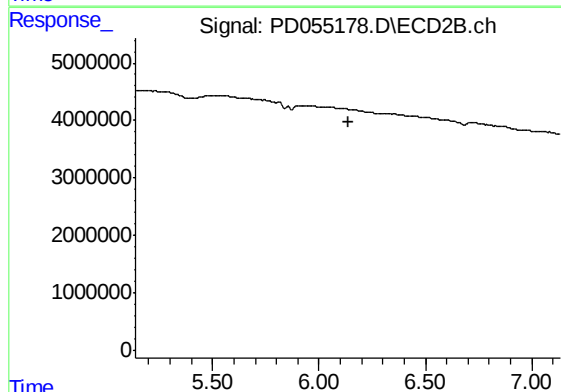


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.136 min
Response: 0
Conc: N.D.

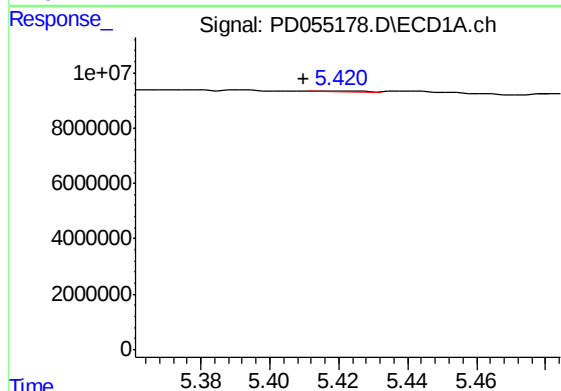


#12 4,4'-DDE

R.T.: 5.421 min
Delta R.T.: 0.011 min
Response: 100850
Conc: 0.11 ng/ml

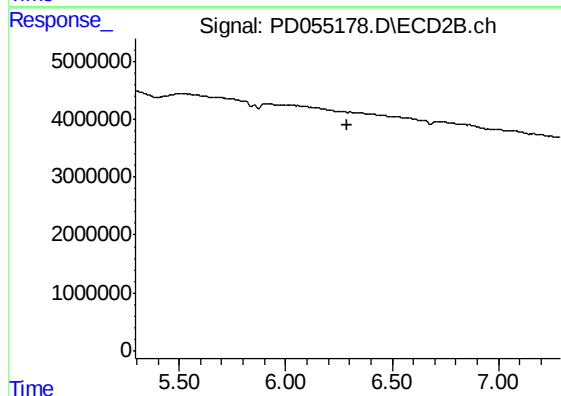

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.293 min
Response: 0
Conc: N.D.

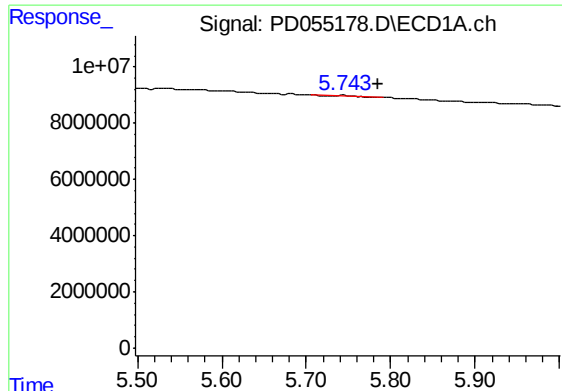

#14 Endrin


R.T.: 5.744 min
Delta R.T.: -0.041 min
Response: 560760
Conc: 0.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

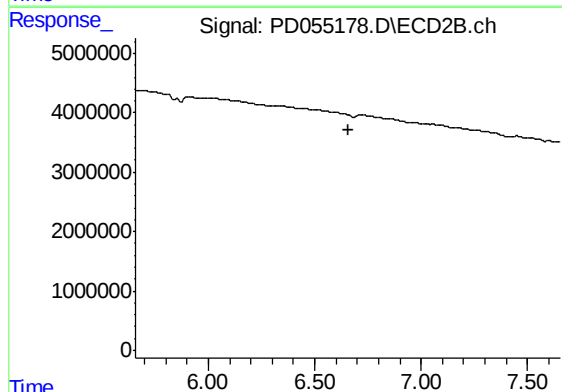


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.658 min
Response: 0
Conc: N.D.

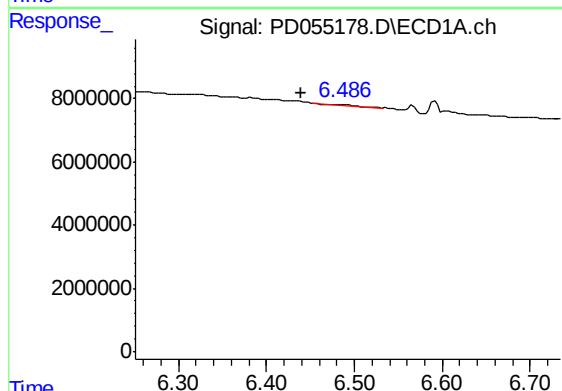


#19 Endosulfan Sulfate

R.T.: 6.487 min
Delta R.T.: 0.048 min
Response: 104970
Conc: 0.13 ng/ml

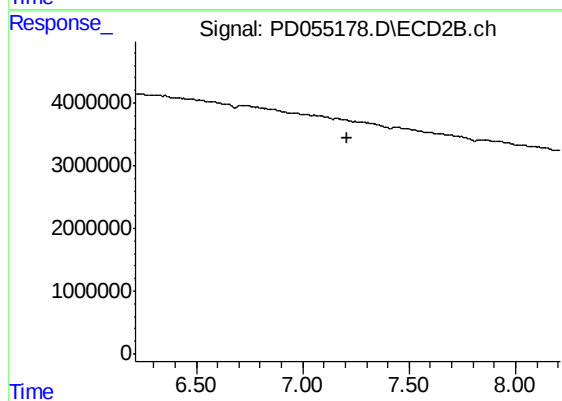

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.212 min
Response: 0
Conc: N.D.

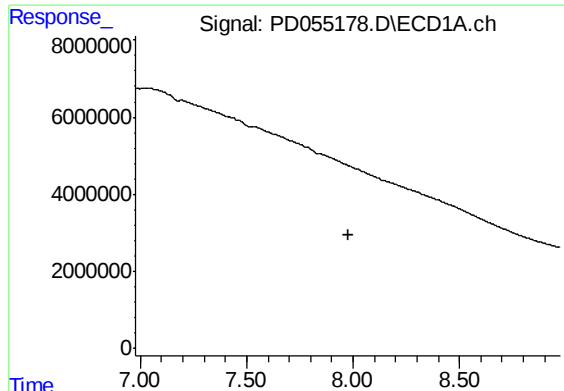

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.977 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

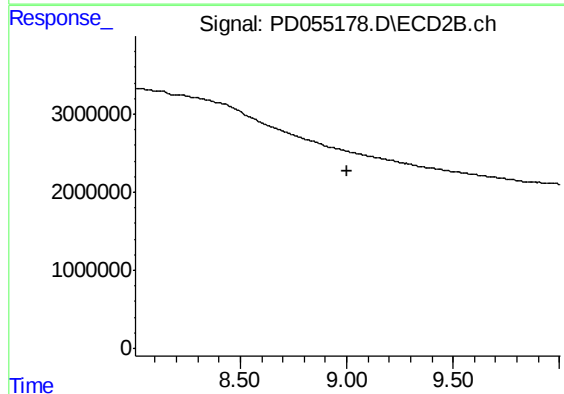

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.005 min
Response: 0
Conc: N.D.