

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100423\
 Data File : PD078629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 20:09
 Operator : AR\AJ
 Sample : 04685-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PP-20230928-B6A-7.5-15

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/04/2023
 Supervised By :Ankita Jodhani 10/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 21:37:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 01:10:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.756	22216593	19524031	7.696m	9.559m
28)	SA Decachlor...	9.077	7.893	39858893	23575683	10.748	10.390
Target Compounds							
12)	B 4,4'-DDE	6.196	5.208	1614809	967739	0.403	0.380m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100423\
Data File : PD078629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 20:09
Operator : AR\AJ
Sample : 04685-07
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PP-20230928-B6A-7.5-15


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/04/2023
Supervised By : Ankita Jodhani 10/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 21:37:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 01:10:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

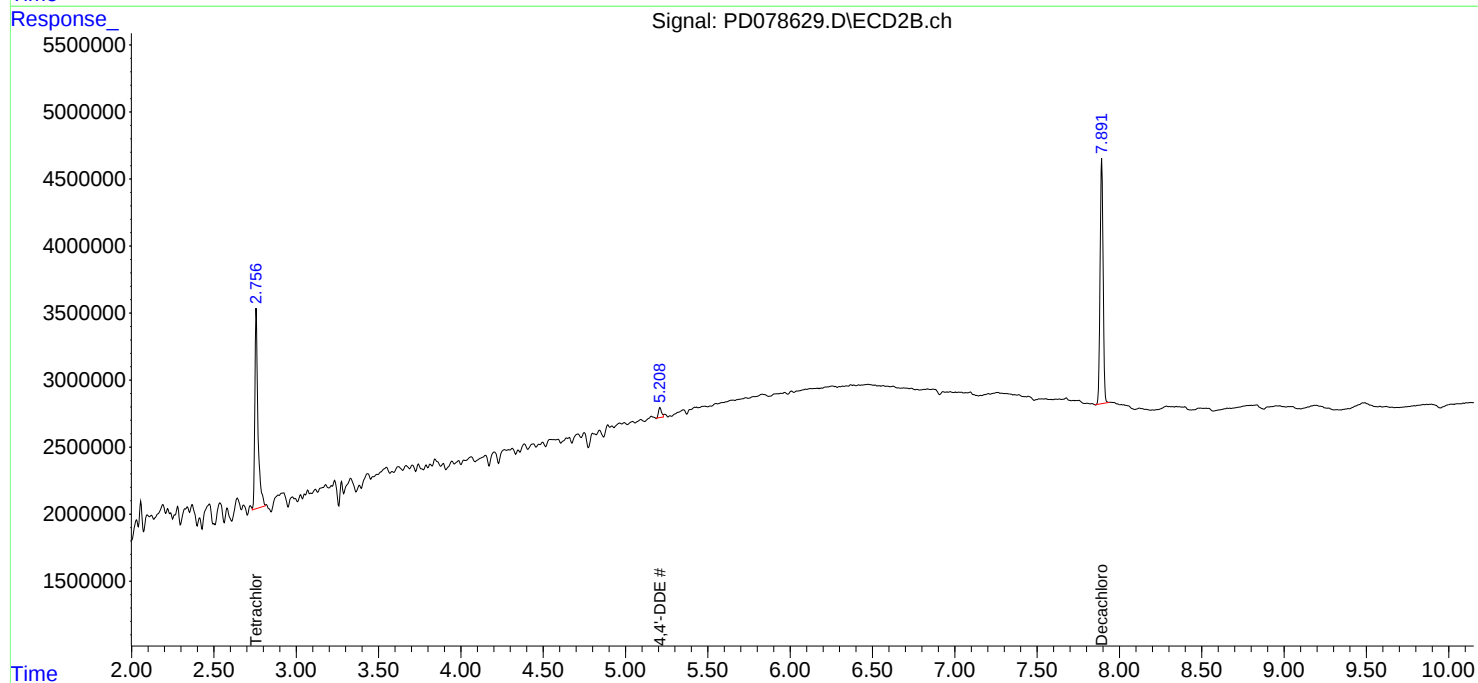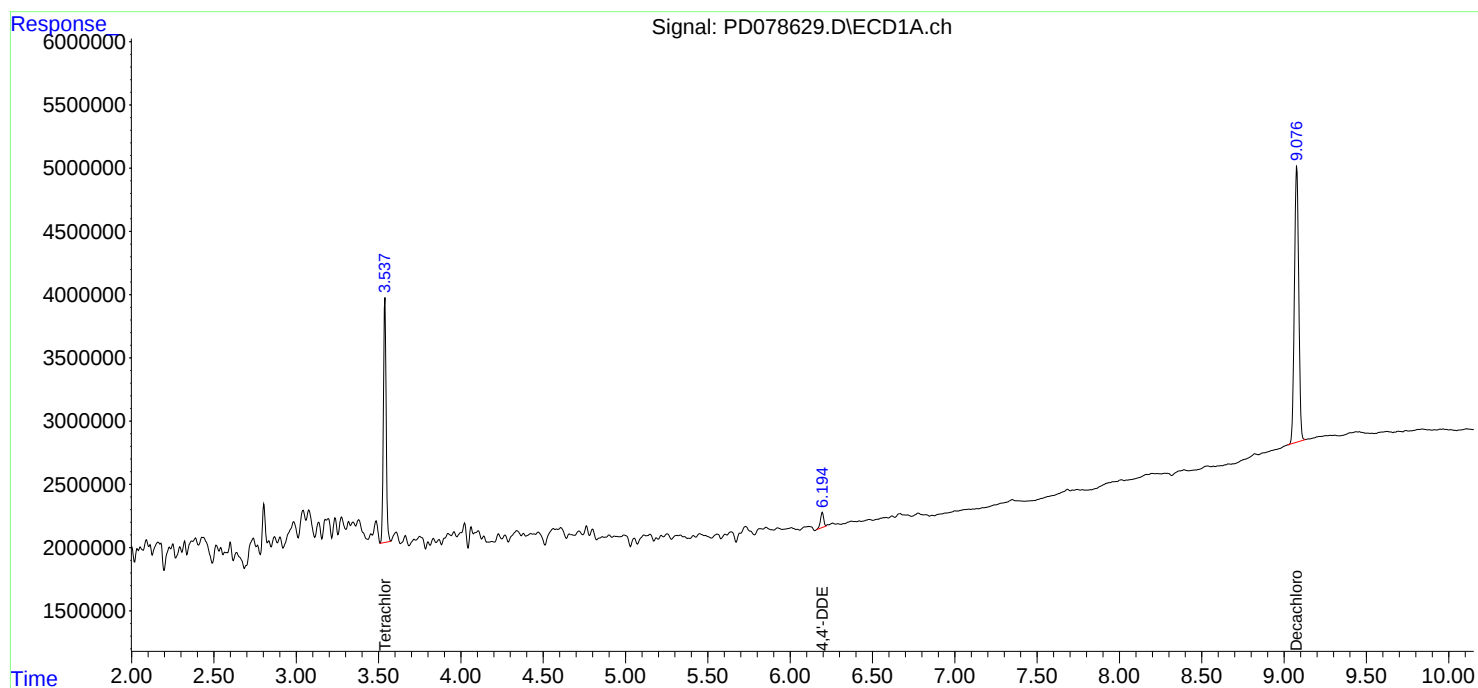

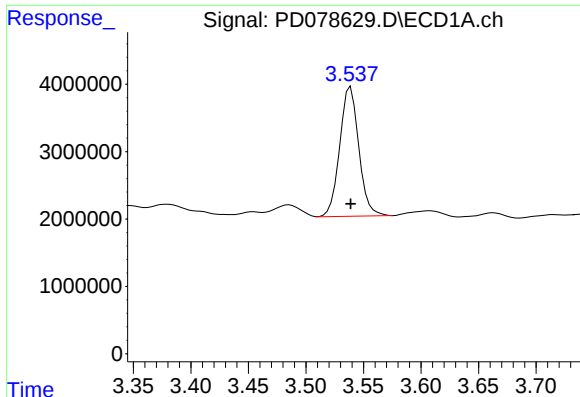


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: -0.002 min
Response: 22216593
Conc: 7.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PP-20230928-B6A-7.5-15


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/04/2023
Supervised By :Ankita Jodhani 10/04/2023

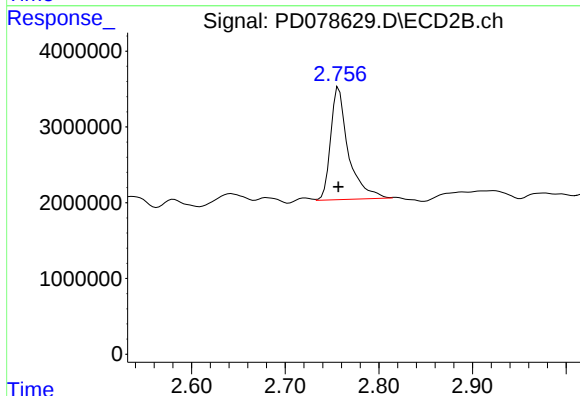


#1 Tetrachloro-m-xylene

R.T.: 2.756 min
Delta R.T.: -0.001 min
Response: 19524031
Conc: 9.56 ng/ml m

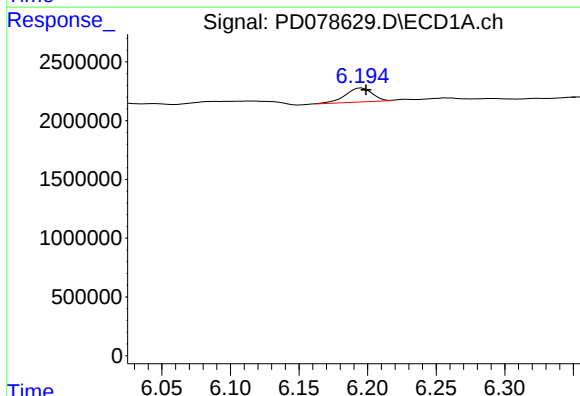


#12 4,4'-DDE

R.T.: 6.196 min
Delta R.T.: -0.003 min
Response: 1614809
Conc: 0.40 ng/ml

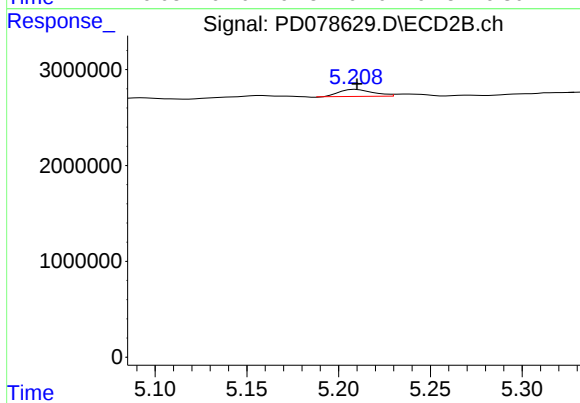

#12 4,4'-DDE

R.T.: 5.208 min
Delta R.T.: -0.002 min
Response: 967739
Conc: 0.38 ng/ml m

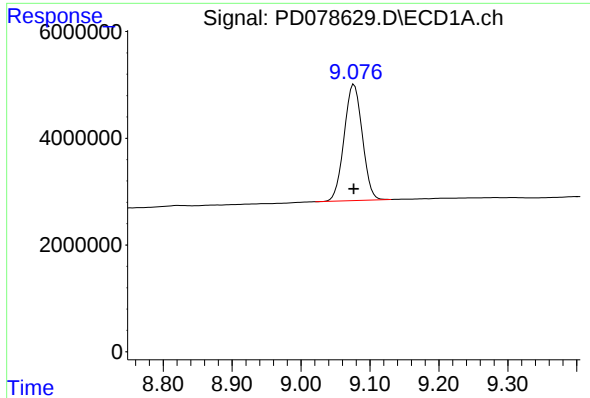


#28 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: 0.000 min
Response: 39858893
Conc: 10.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PP-20230928-B6A-7.5-15

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/04/2023
Supervised By :Ankita Jodhani 10/04/2023

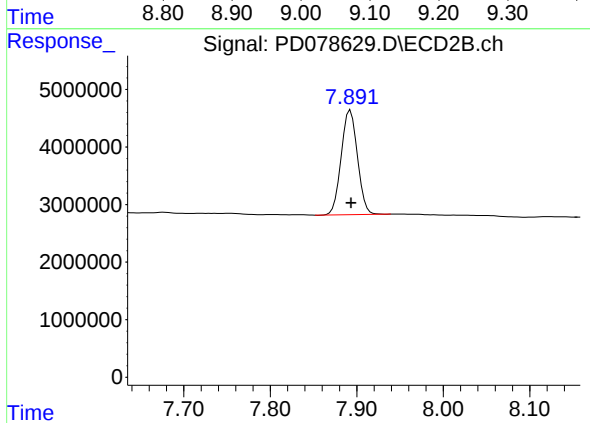

#28 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 23575683
Conc: 10.39 ng/ml