

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100423\
 Data File : PD078639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 22:23
 Operator : AR\AJ
 Sample : 04704-05
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-104-1(5-10)

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/04/2023
 Supervised By : Ankita Jodhani 10/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:16:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 01:10:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.538	2.757	18349507	13716007	6.356m	6.716m
2) SA Decachlor...	9.077	7.893	23657801	13526557	6.379	5.961

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100423\
Data File : PD078639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 22:23
Operator : AR\AJ
Sample : 04704-05
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SB-104-1(5-10)


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/04/2023
Supervised By : Ankita Jodhani 10/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:16:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 01:10:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

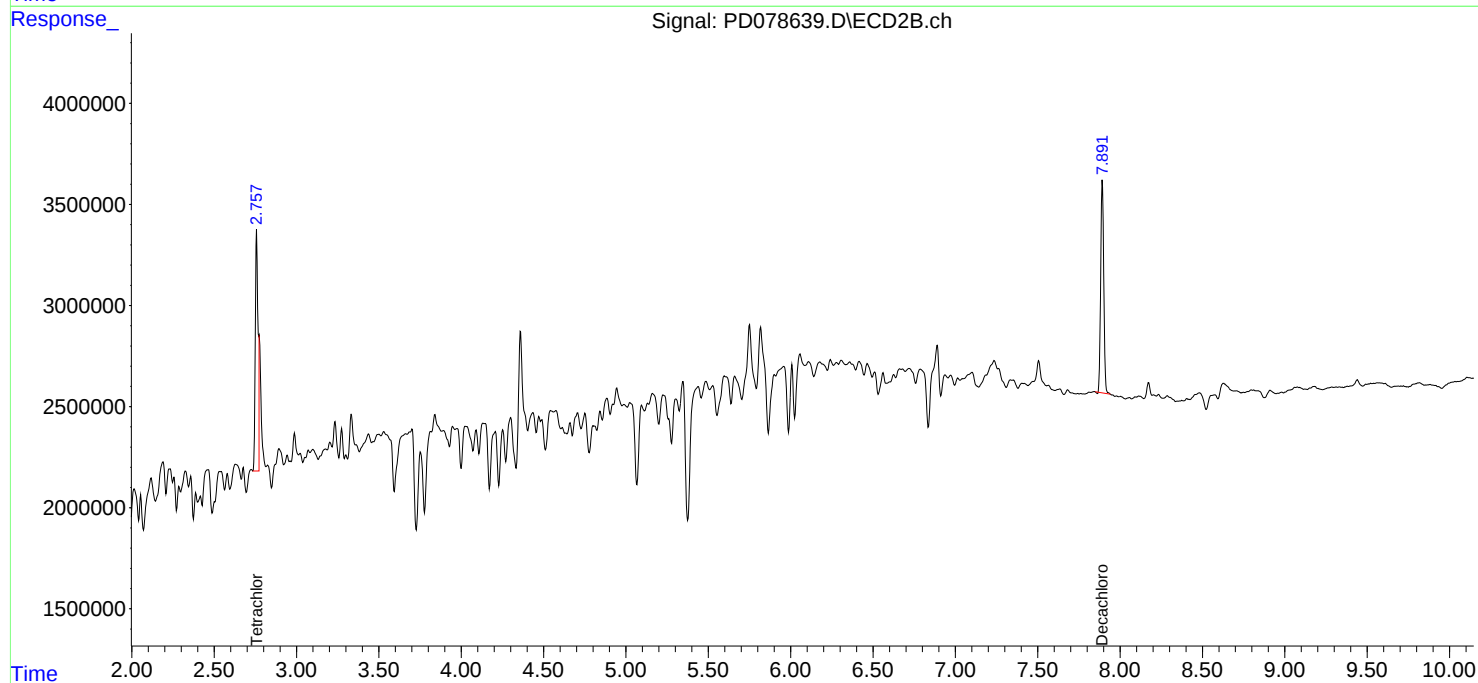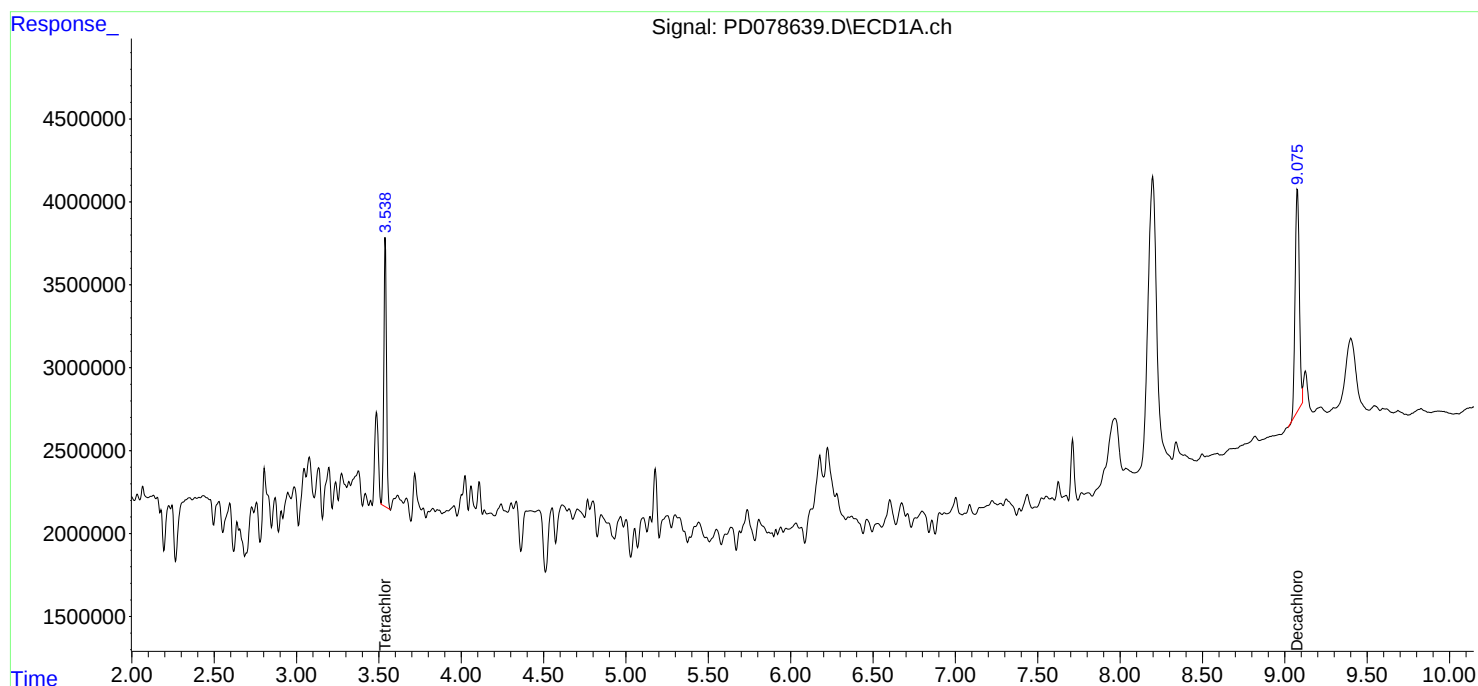

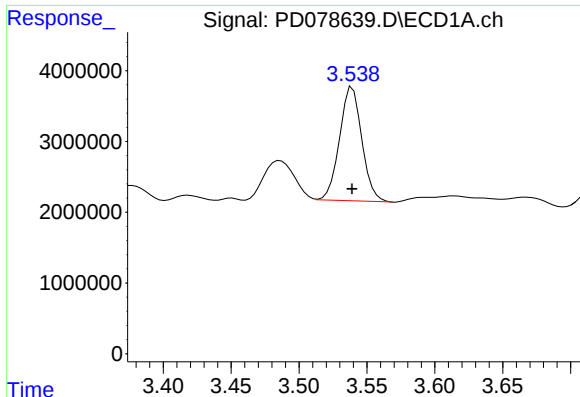

#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: -0.001 min
Response: 18349507
Conc: 6.36 ng/ml

Instrument :

ECD_D

ClientSampleId :


SB-104-1(5-10)

Manual Integrations

APPROVED


Reviewed By :Abdul Mirza 10/04/2023

Supervised By :Ankita Jodhani 10/04/2023

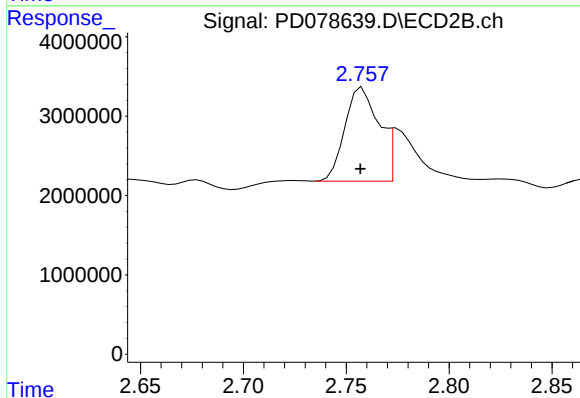


#1 Tetrachloro-m-xylene

R.T.: 2.757 min
Delta R.T.: 0.000 min
Response: 13716007
Conc: 6.72 ng/ml m

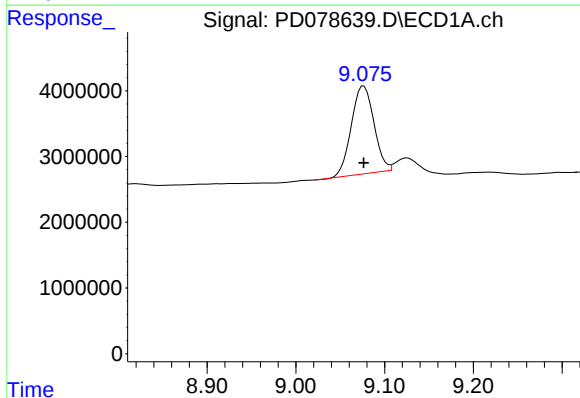

#28 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: 0.000 min
Response: 23657801
Conc: 6.38 ng/ml

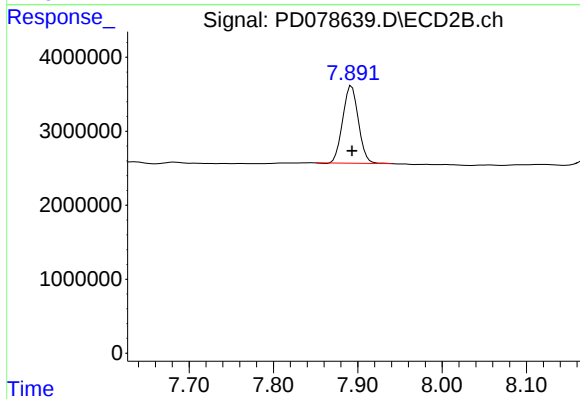

#28 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 13526557
Conc: 5.96 ng/ml