

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100423\
 Data File : PD078643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 23:30
 Operator : AR\AJ
 Sample : 04693-01DL 20X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 F-1(0-5)

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/12/2023
 Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:17:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 01:10:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.537	2.757	1693723	1517512	0.587m	0.743 #
28) SA Decachlor...	9.078	7.893	2648415	1711735	0.714	0.754

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100423\
Data File : PD078643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 23:30
Operator : AR\AJ
Sample : 04693-01DL 20X
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
F-1(0-5)


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/12/2023
Supervised By : Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:17:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 01:10:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

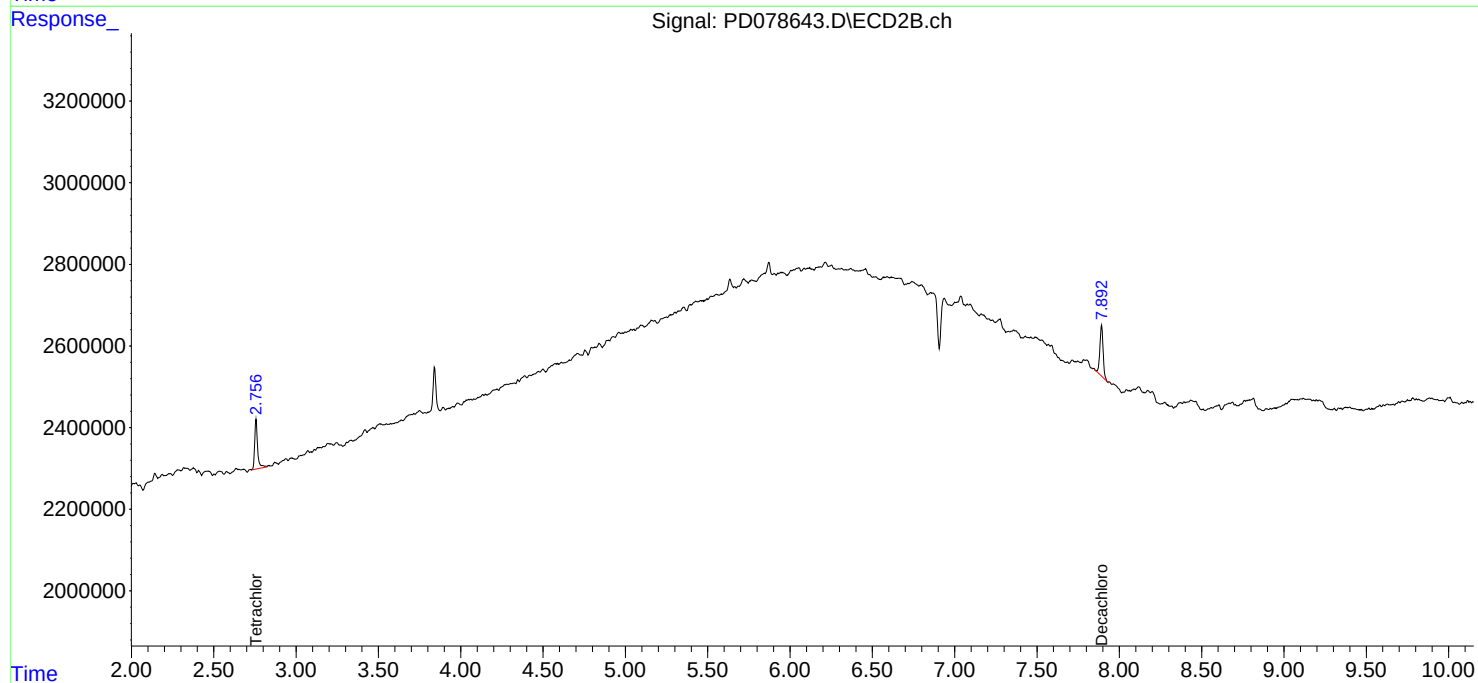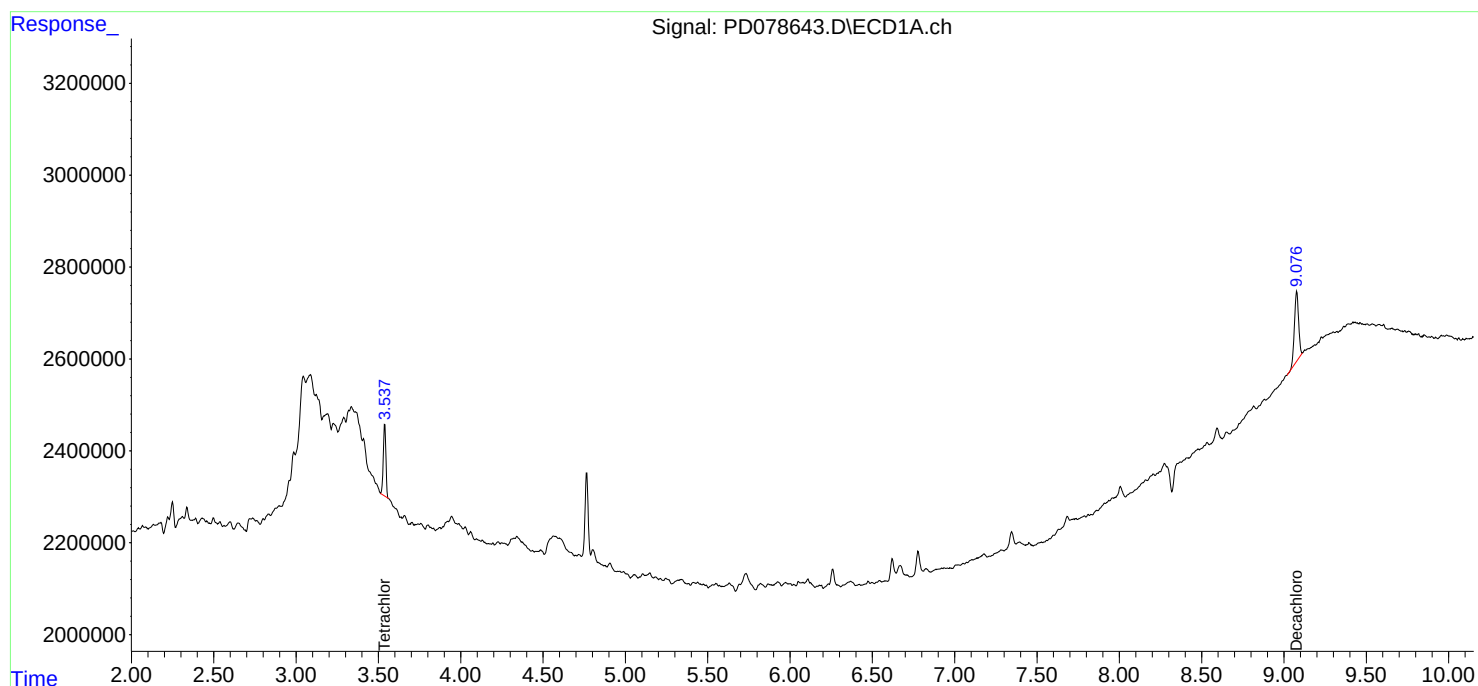

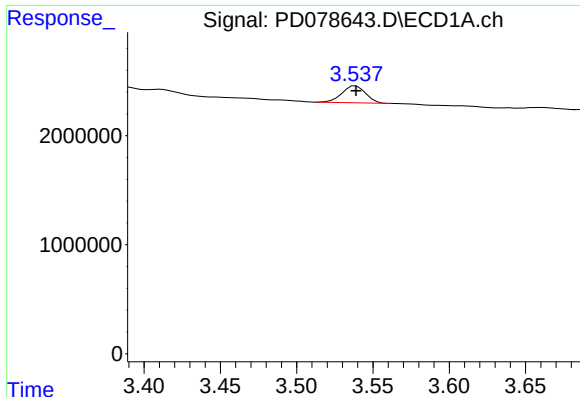


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: -0.002 min
Response: 1693723
Conc: 0.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
F-1(0-5)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/12/2023
Supervised By :Ankita Jodhani 10/12/2023

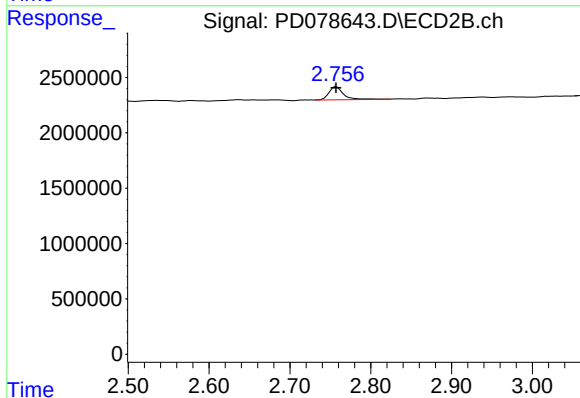


#1 Tetrachloro-m-xylene

R.T.: 2.757 min
Delta R.T.: 0.000 min
Response: 1517512
Conc: 0.74 ng/ml

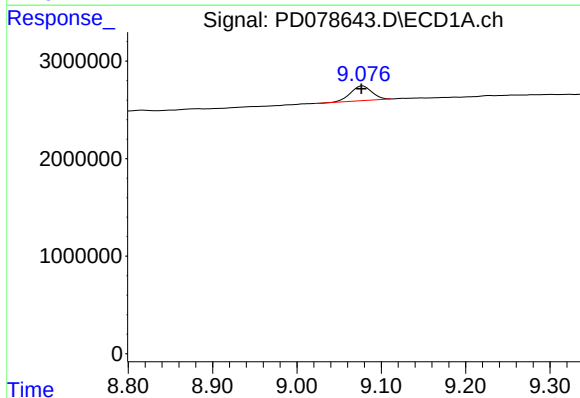

#28 Decachlorobiphenyl

R.T.: 9.078 min
Delta R.T.: 0.001 min
Response: 2648415
Conc: 0.71 ng/ml

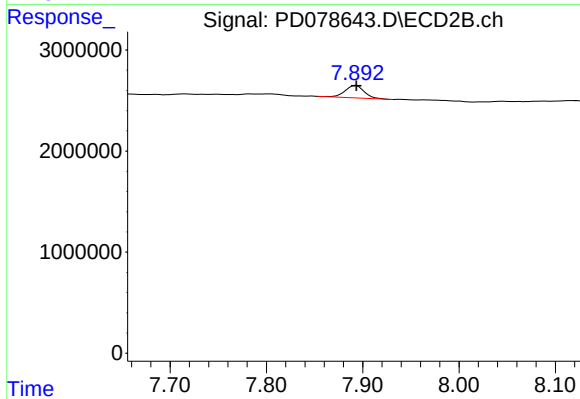

#28 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 1711735
Conc: 0.75 ng/ml