

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100423\
 Data File : PD078644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 23:43
 Operator : AR\AJ
 Sample : 04702-01DL 10X
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OK-02-100223

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/12/2023
 Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:18:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 01:10:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.537	2.757	3434647	2846993	1.190m	1.394
2) SA Decachlor...	9.077	7.892	3843273	2001788	1.036	0.882

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100423\
Data File : PD078644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 23:43
Operator : AR\AJ
Sample : 04702-01DL 10X
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
OK-02-100223


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/12/2023
Supervised By : Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:18:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 01:10:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

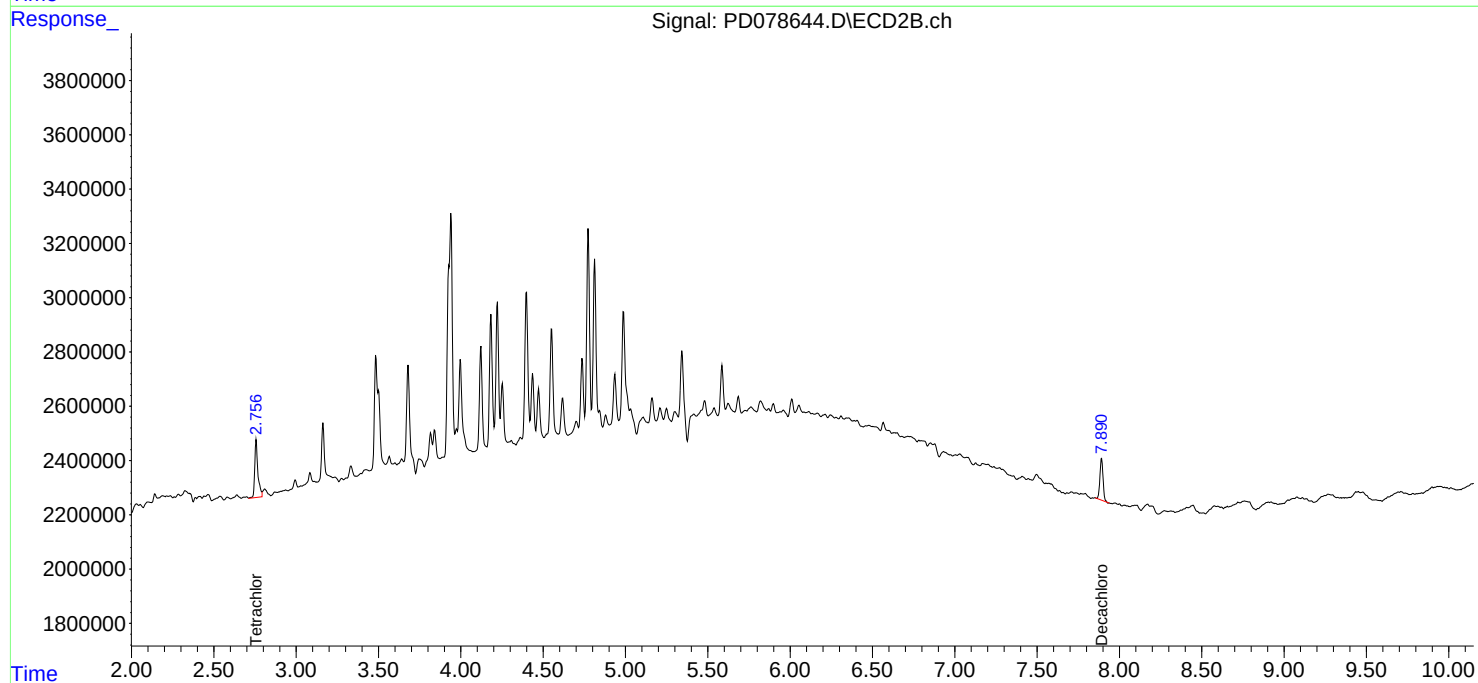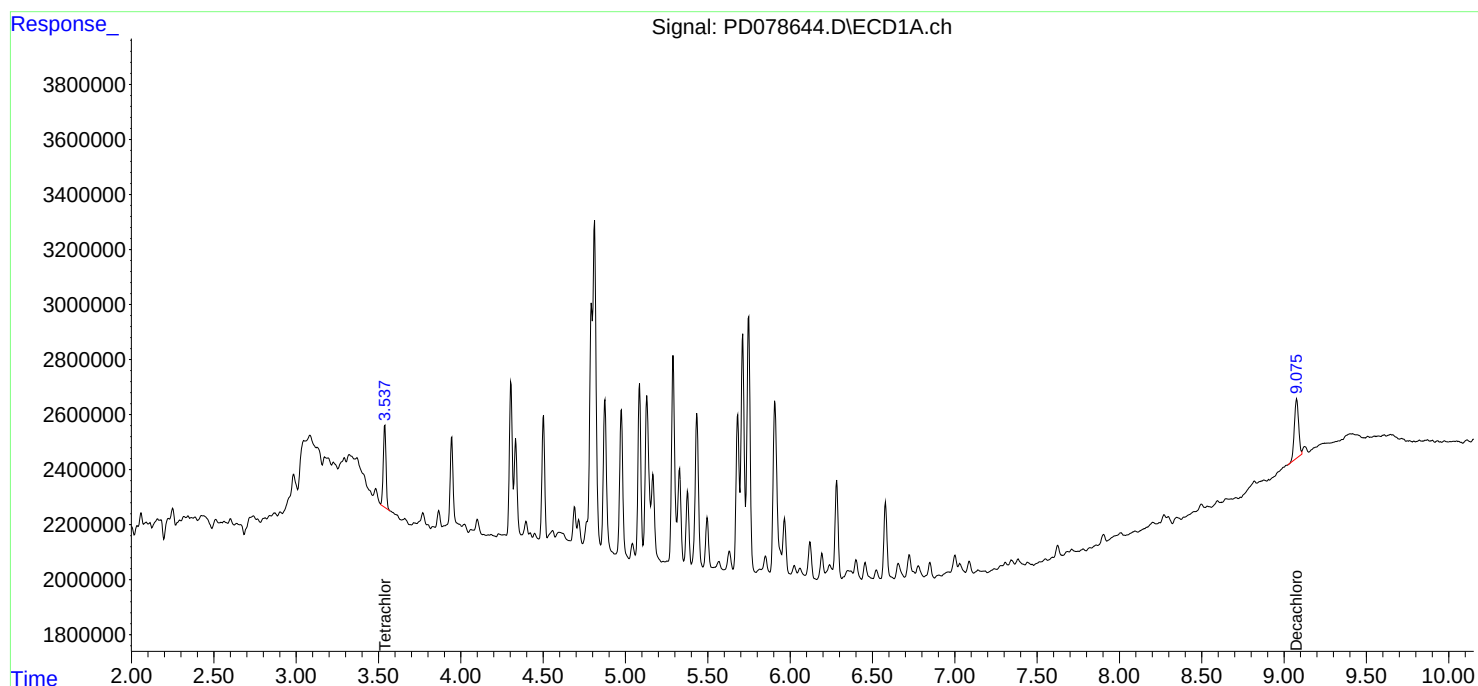

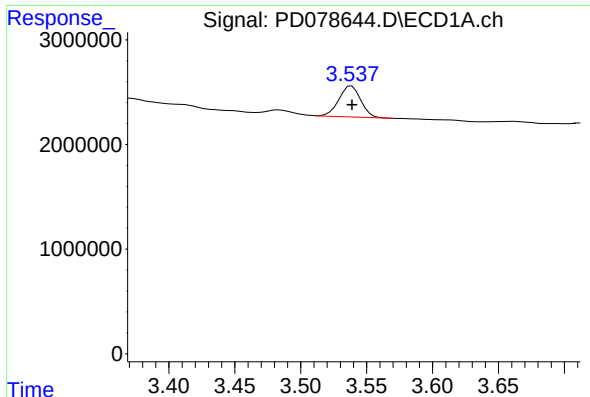

#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: -0.002 min
Response: 3434647
Conc: 1.19 ng/ml

Instrument :


ECD_D

ClientSampleId :

OK-02-100223


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/12/2023
Supervised By :Ankita Jodhani 10/12/2023

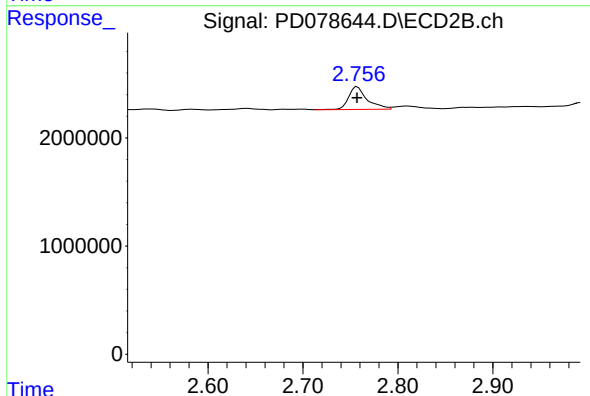


#1 Tetrachloro-m-xylene

R.T.: 2.757 min
Delta R.T.: 0.000 min
Response: 2846993
Conc: 1.39 ng/ml

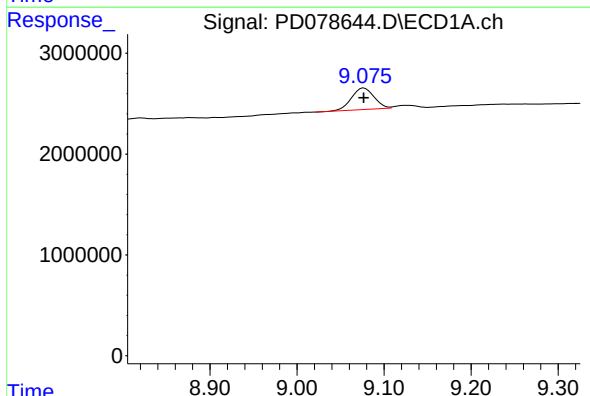

#28 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: 0.000 min
Response: 3843273
Conc: 1.04 ng/ml

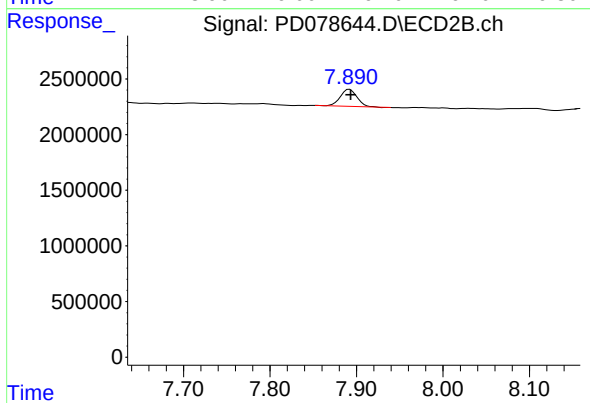

#28 Decachlorobiphenyl

R.T.: 7.892 min
Delta R.T.: -0.001 min
Response: 2001788
Conc: 0.88 ng/ml