

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100424\
 Data File : PD085910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 12:09
 Operator : AR\AJ
 Sample : P4022-06DL 4X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCD6DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/04/2024
 Supervised By :Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 02:24:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 08:04:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.443	2.884	7414819	1002.0E6	6.481m	236.293m#
2) SA Decachlor...	8.886	8.056	9124636	20358260	5.017	5.538m
Target Compounds						
2) A alpha-BHC	3.879	3.381	141.6E6	320.2E6	67.996m	50.749m#
5) MB Aldrin	5.146	4.347	10317505	24874033	4.915m	4.233m
7) B delta-BHC	4.639	4.247	182.9E6	292.0E6	95.198	49.201 #
19) B Endosulfa...	7.018	6.452	4536521	2772863	2.881m	0.649m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100424\
Data File : PD085910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 12:09
Operator : AR\AJ
Sample : P4022-06DL 4X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 02:24:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

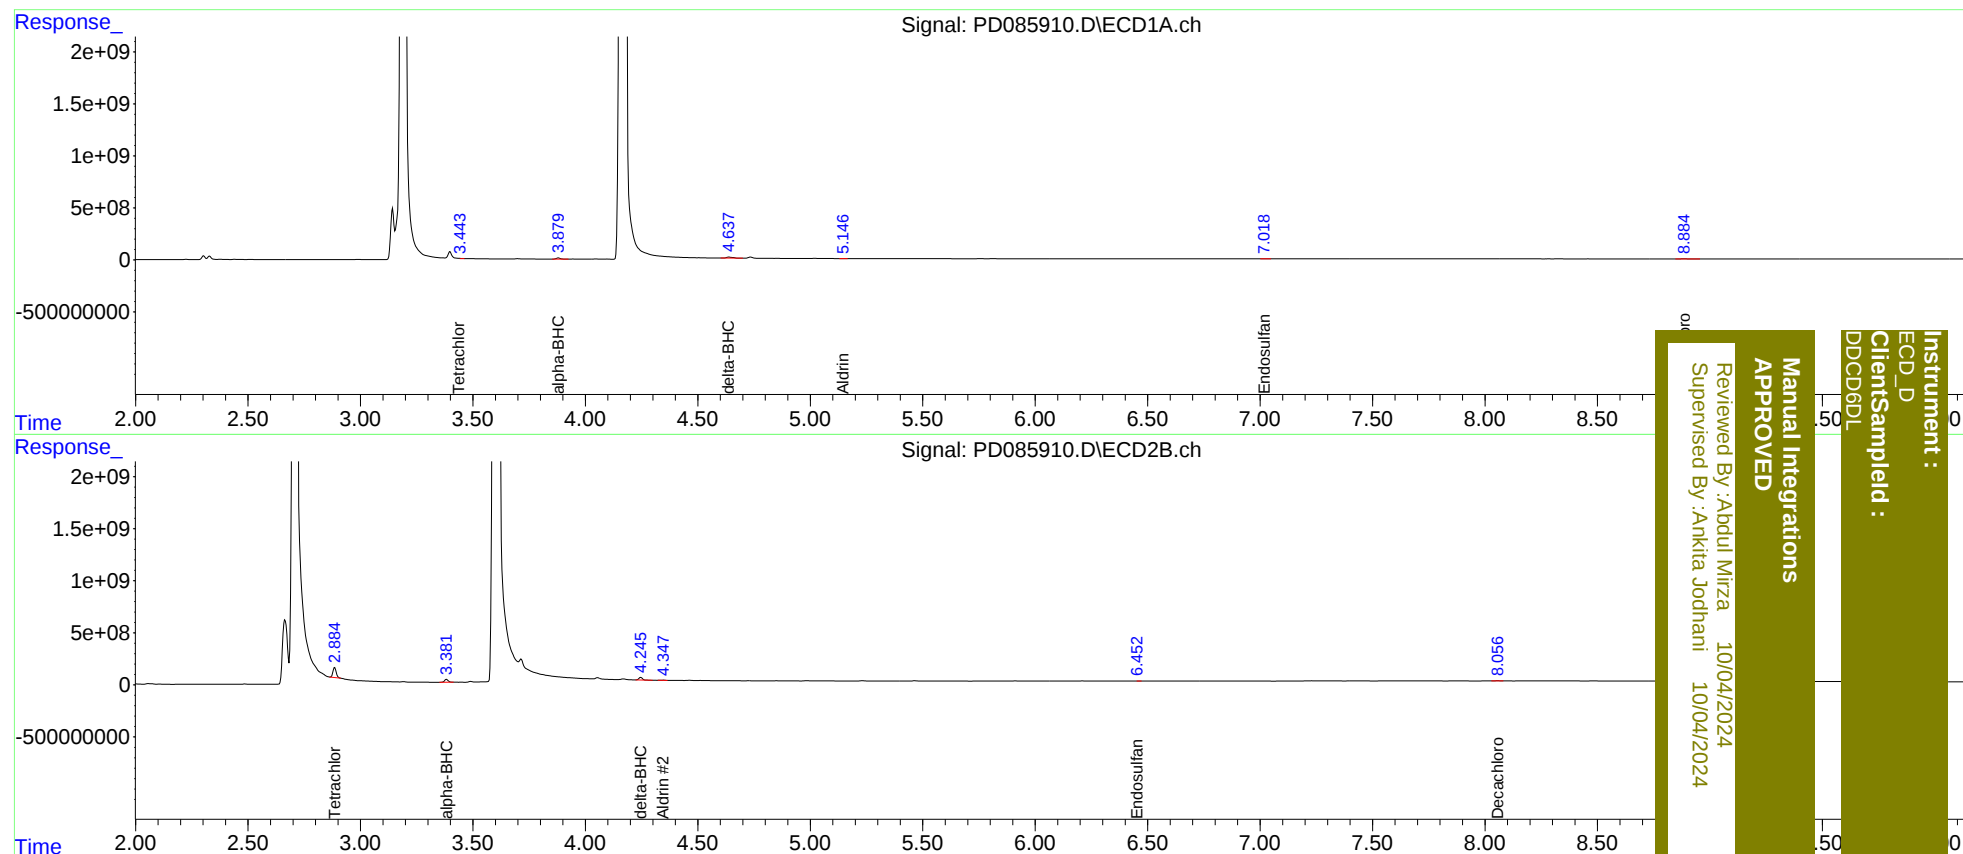

Reviewed By: Abdul Mirza 10/04/2024
Supervised By: Ankita Jodhani 10/04/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDCD6DL