

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100425\
 Data File : PD090512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2025 16:00
 Operator : AR\AJ
 Sample : Q3263-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 266380

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/06/2025
 Supervised By :mohammad ahmed 10/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:29:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:52:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.875	49897786	424.9E6	15.351m	15.480
2) SA Decachlor...	9.063	8.060	82010632	519.3E6	16.997	16.020
Target Compounds						
13) MA Dieldrin	6.340	5.503	2846559	22927305	0.494	0.589

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100425\
Data File : PD090512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2025 16:00
Operator : AR\AJ
Sample : Q3263-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
266380


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2025
Supervised By :mohammad ahmed 10/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:29:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:52:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

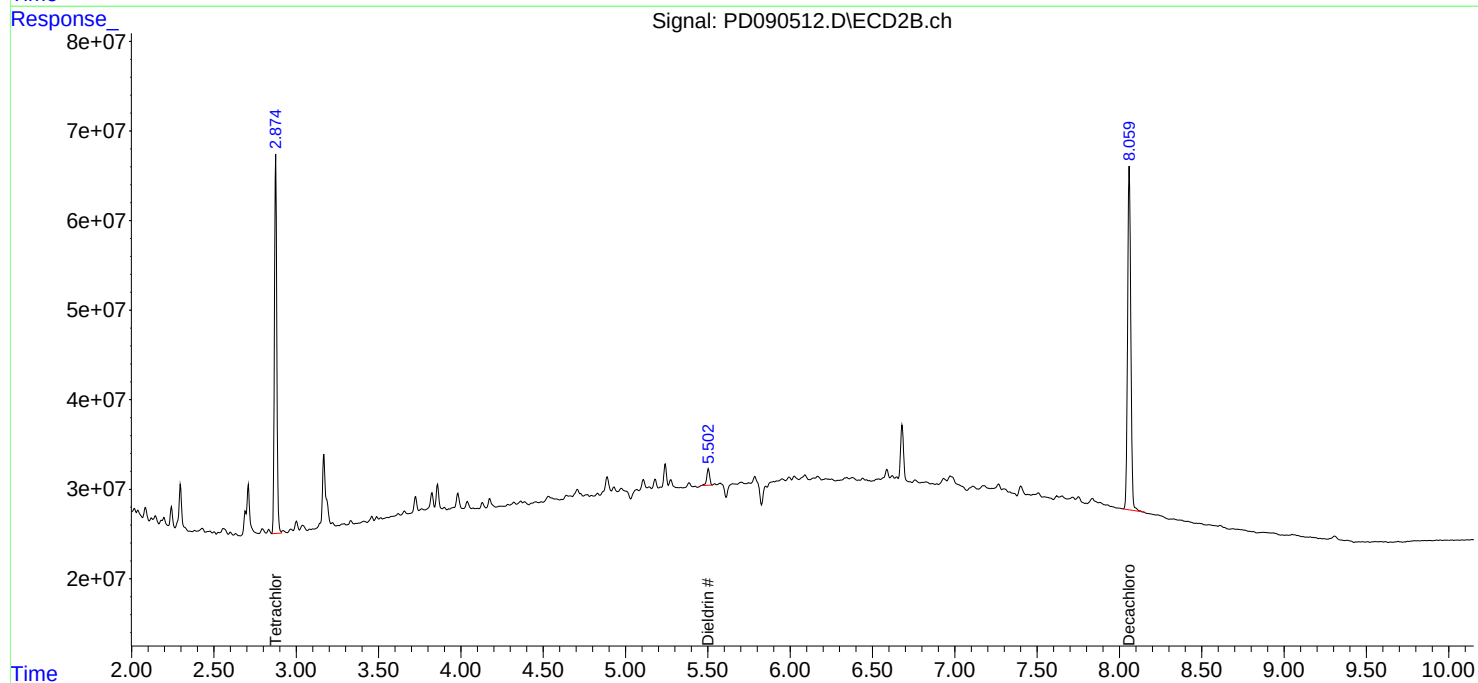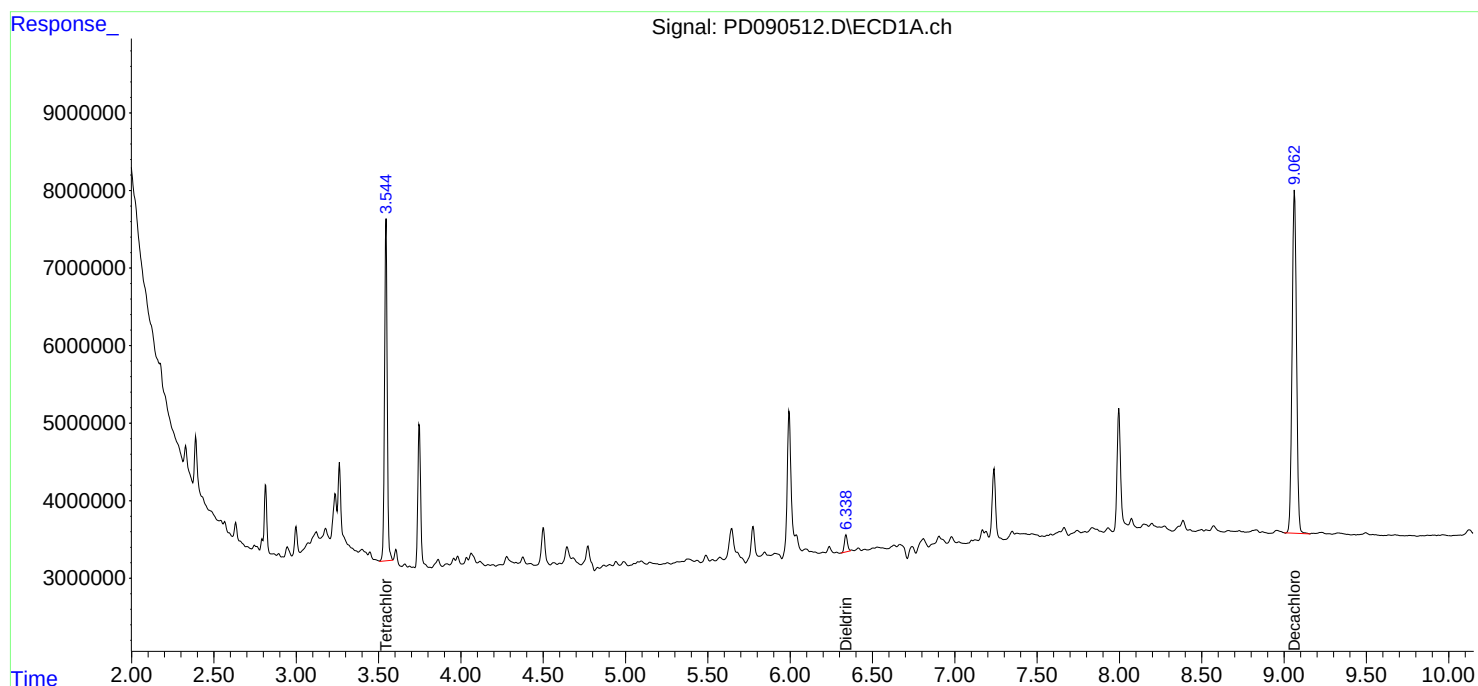

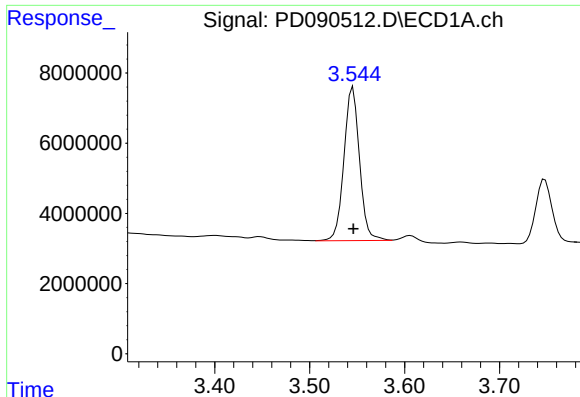


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.002 min
Response: 49897786
Conc: 15.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
266380


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2025
Supervised By :mohammad ahmed 10/06/2025

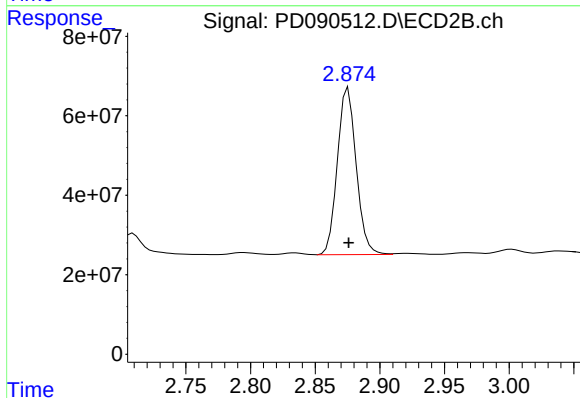


#1 Tetrachloro-m-xylene

R.T.: 2.875 min
Delta R.T.: 0.000 min
Response: 424916968
Conc: 15.48 ng/ml

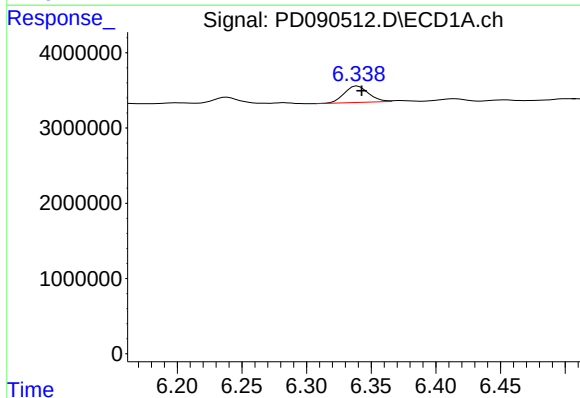


#13 Dieldrin

R.T.: 6.340 min
Delta R.T.: -0.003 min
Response: 2846559
Conc: 0.49 ng/ml

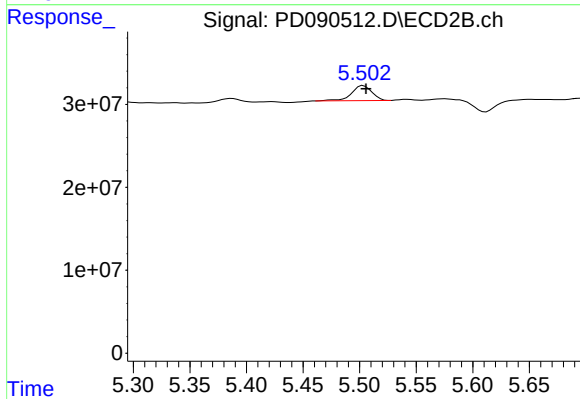

#13 Dieldrin

R.T.: 5.503 min
Delta R.T.: -0.002 min
Response: 22927305
Conc: 0.59 ng/ml

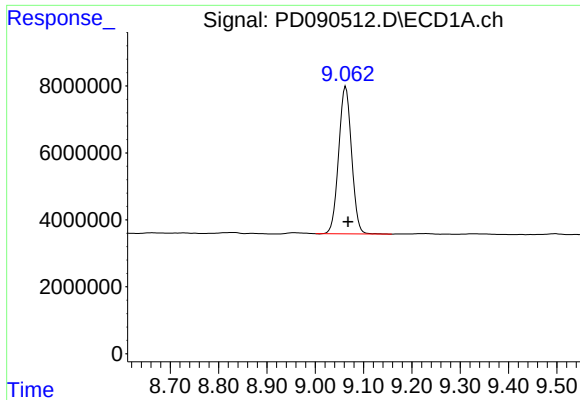

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: -0.005 min
Response: 82010632
Conc: 17.00 ng/ml


Instrument :

ECD_D

ClientSampleId :
266380

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2025
Supervised By :mohammad ahmed 10/06/2025

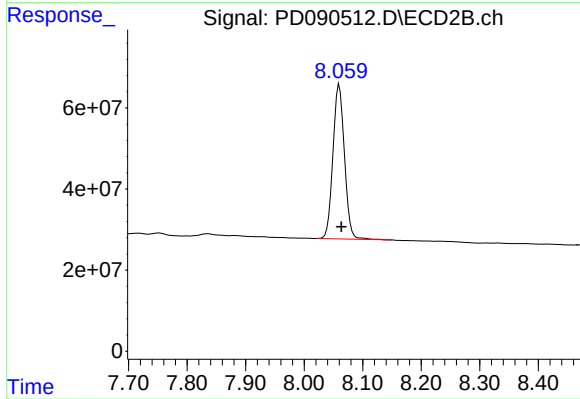

#28 Decachlorobiphenyl

R.T.: 8.060 min
Delta R.T.: -0.004 min
Response: 519293931
Conc: 16.02 ng/ml