

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100518\
 Data File : PD049614.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2018 15:13
 Operator : AJ\SJ
 Sample : J5177-21
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 23:58:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100518CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 05 23:35:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	0.000	9.065f	0	540327	N.D.	<MDL
Target Compounds							
6)	B beta-BHC	0.000	4.925f	0	5497173	N.D.	1.129
8)	B Heptachlo...	0.000	5.910	0	3793185	N.D.	0.404
10)	B trans-Chl...	0.000	6.095f	0	322710	N.D.	<MDL
14)	MA Endrin	0.000	6.790f	0	557488	N.D.	<MDL
16)	A 4,4'-DDD	0.000	6.889	0	671333	N.D.	<MDL
20)	A Methoxychlor	0.000	7.572f	0	1428914	N.D.	0.472
23)	Toxaphene-2	5.545	6.790	1395354	557488	162.242	10.757 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100518\
Data File : PD049614.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2018 15:13
Operator : AJ\SJ
Sample : J5177-21
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 23:58:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100518CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 05 23:35:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

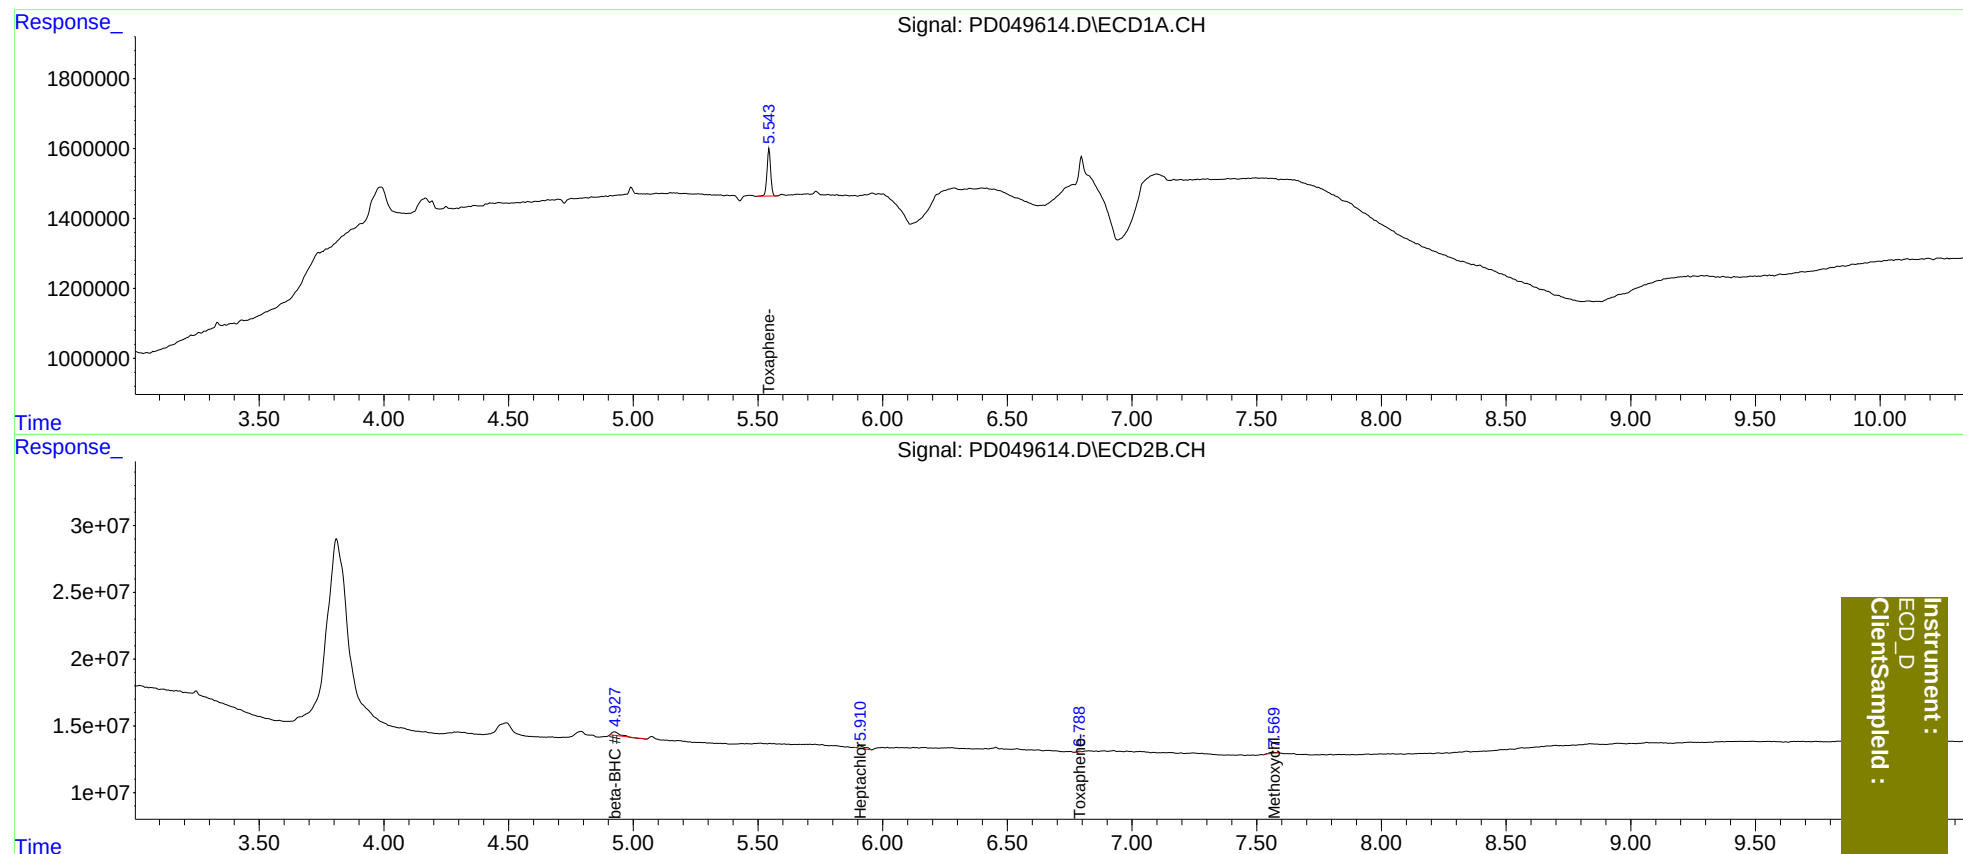

Instrument :
ECD_D
ClientSampled :