

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100518\
 Data File : PD049641.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Oct 2018 00:03
 Operator : AJ\SJ
 Sample : J5230-11
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A3Z07

Manual Integrations
 APPROVED

Sohil
 10/8/2018 10:44:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 00:51:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100518CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 05 23:35:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.284	4.036	20187849	148.1E6	16.680	16.879
2) SA Decachlor...	7.878	9.127	42587784	277.3E6	38.310	38.749m
Target Compounds						
12) B 4,4'-DDE	5.355	6.378	5970726	38011485	4.303	4.247m
16) A 4,4'-DDD	5.848	6.869	12602480	141.3E6	11.244	20.054 #
17) MA 4,4'-DDT	6.082	7.174	5167726	48652022	4.450	7.565 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100518\
Data File : PD049641.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Oct 2018 00:03
Operator : AJ\SJ
Sample : J5230-11
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 00:51:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100518CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 05 23:35:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

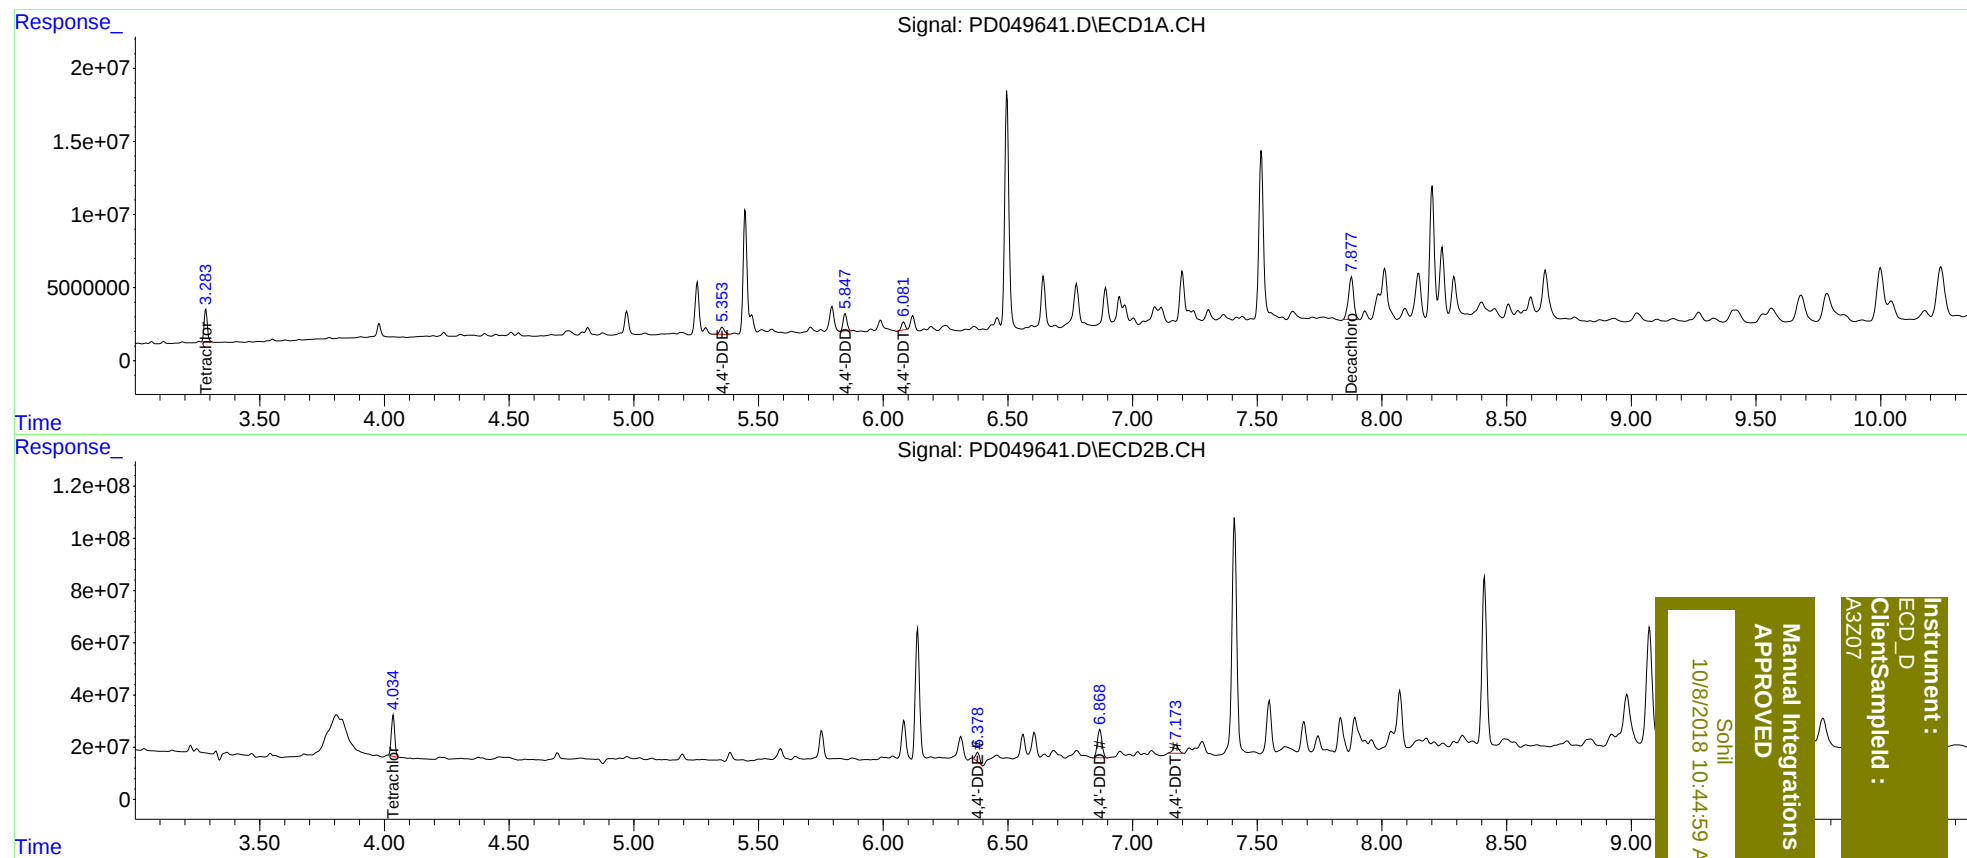

Instrument :
ECD_D
Client Sampled :
A3207

Manual Integrations
APPROVED

Sohil
10/8/2018 10:44:59 AM