

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100518\
 Data File : PD049637.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2018 22:13
 Operator : AJ\SJ
 Sample : J5230-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A3YZ2

Manual Integrations
 APPROVED

Sohil
 10/8/2018 10:44:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 00:50:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100518CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 05 23:35:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	4.036	15642158	109.8E6	12.924	12.507
27)	SA Decachlor...	7.876	9.127	34774643	193.4E6	31.281m	27.021m
Target Compounds							
12)	B 4,4'-DDE	5.357	6.379	4305509	32921969	3.103	3.678m
16)	A 4,4'-DDD	5.848	6.869	13391654	169.9E6	11.948	24.107 #
17)	MA 4,4'-DDT	6.083	7.172	10050486	89372191	8.654	13.897 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100518\
Data File : PD049637.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2018 22:13
Operator : AJ\SJ
Sample : J5230-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 00:50:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100518CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 05 23:35:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

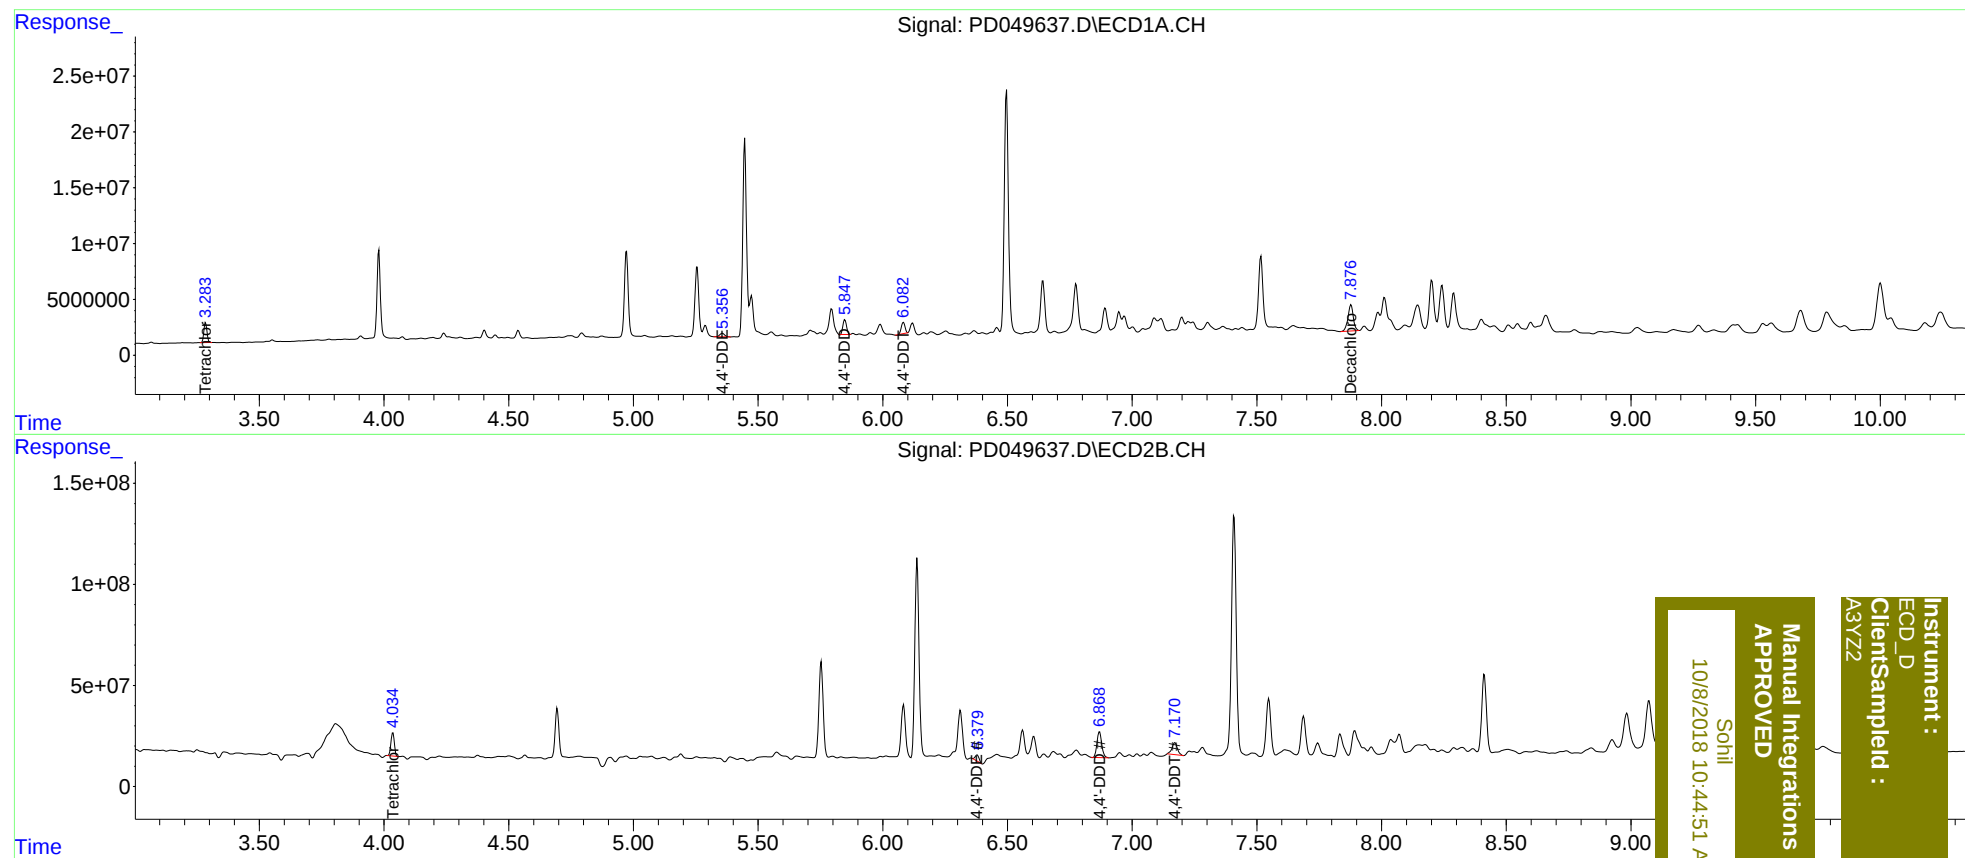

10/8/2018 10:44:51 AM

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
A3YZ2