

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100522\
 Data File : PD072214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2022 11:17
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 12:30:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 12:29:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.743	3.497	305.2E6	3366.1E6	100.295	95.335
28)	SA Decachlor...	7.919	8.984	240.1E6	911.2E6	95.050	91.501
Target Compounds							
23)	Chlordane-1	3.748	4.653	97926505	1047.9E6	989.986	911.384
24)	Chlordane-2	4.328	5.185	106.2E6	783.7E6	939.282	871.418
25)	Chlordane-3	4.963	5.894	324.6E6	2326.9E6	1011.774	943.448
26)	Chlordane-4	5.027	5.973	313.9E6	2629.6E6	1017.598	941.895
27)	Chlordane-5	5.926	6.831	104.2E6	508.3E6	984.305	939.904



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100522\
Data File : PD072214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2022 11:17
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 12:30:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 12:29:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

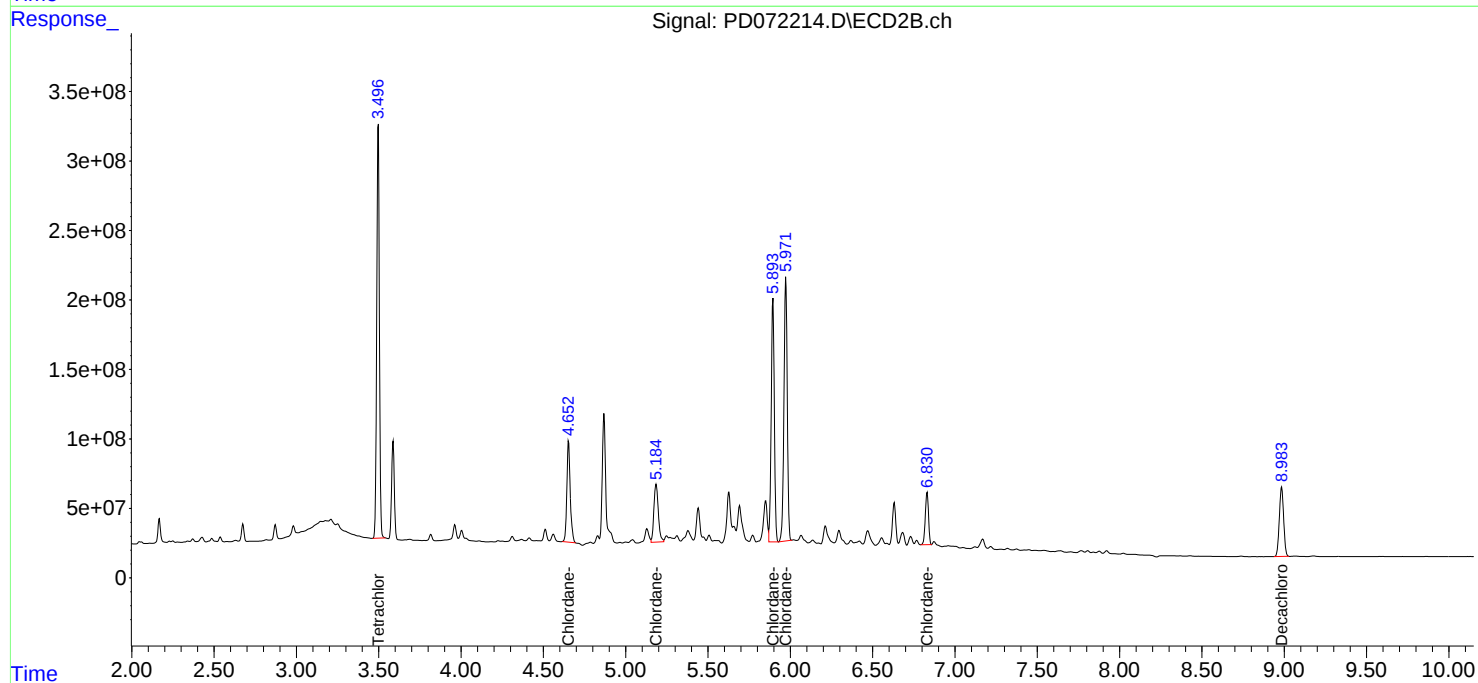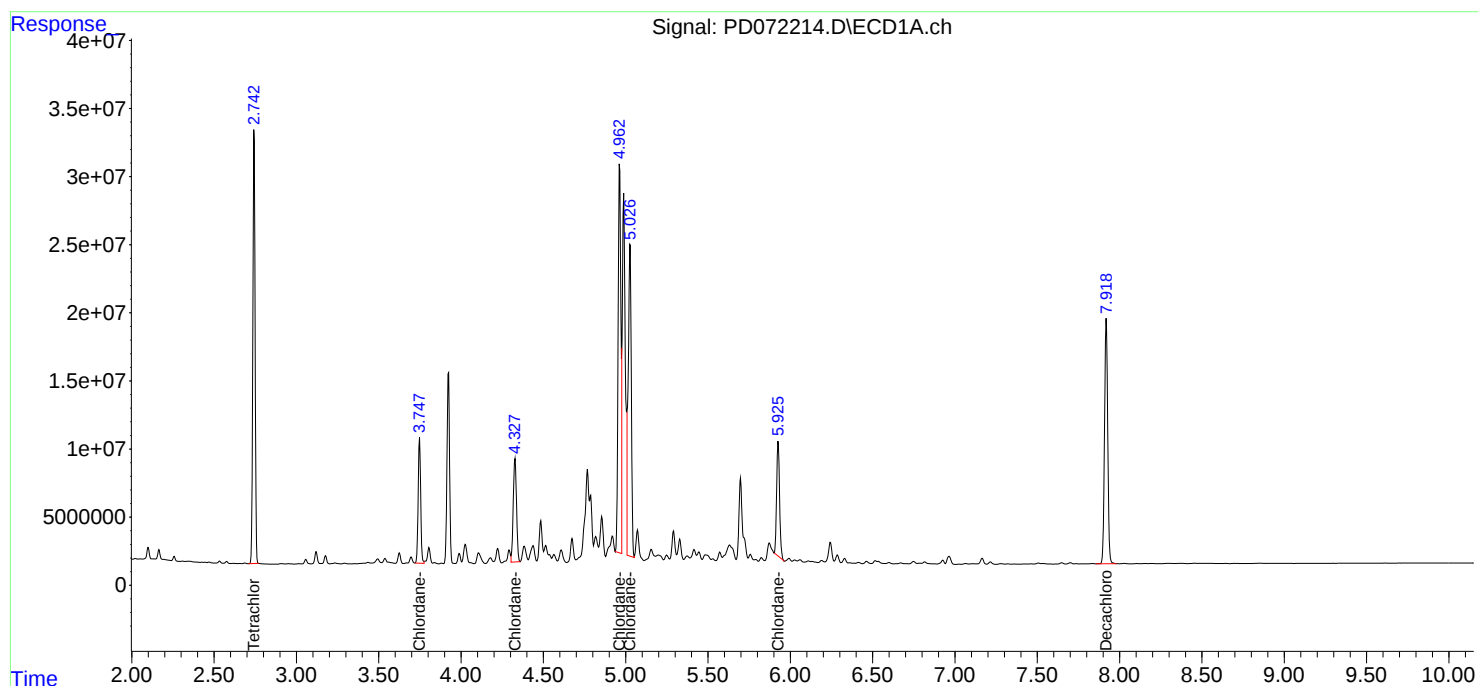


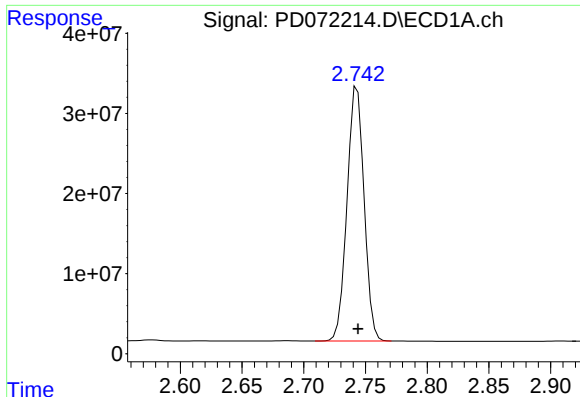

#1 Tetrachloro-m-xylene


R.T.: 2.743 min
Delta R.T.: 0.000 min
Response: 305205978
Conc: 100.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

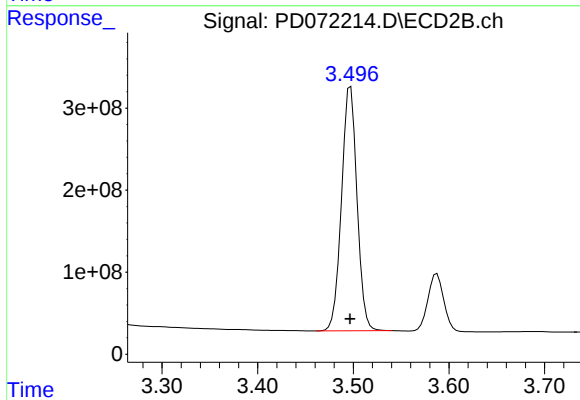


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 3366092463
Conc: 95.33 ng/ml

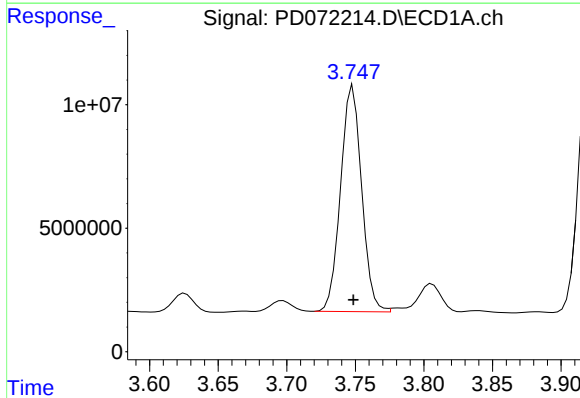


#23 Chlordane-1

R.T.: 3.748 min
Delta R.T.: 0.000 min
Response: 97926505
Conc: 989.99 ng/ml

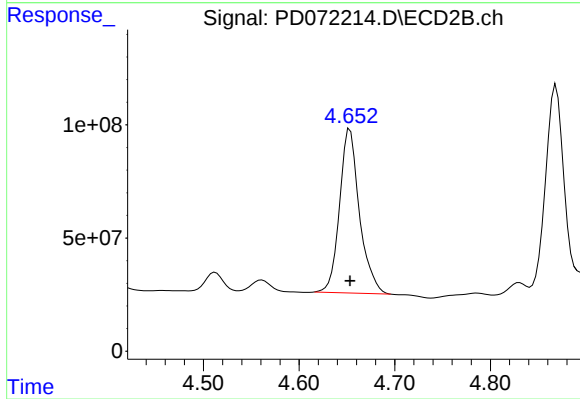

#23 Chlordane-1


R.T.: 4.653 min
Delta R.T.: 0.000 min
Response: 1047913247
Conc: 911.38 ng/ml

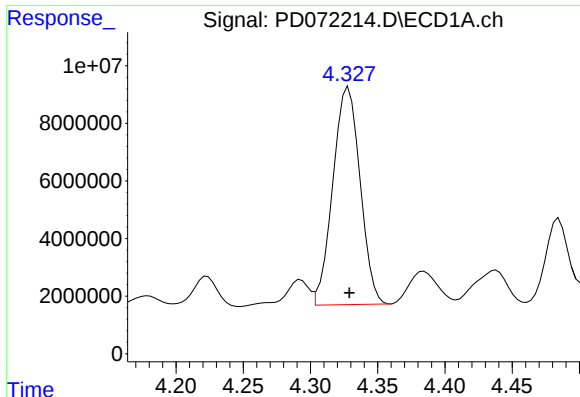

#24 Chlordane-2


R.T.: 4.328 min
Delta R.T.: 0.000 min
Response: 106203513
Conc: 939.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

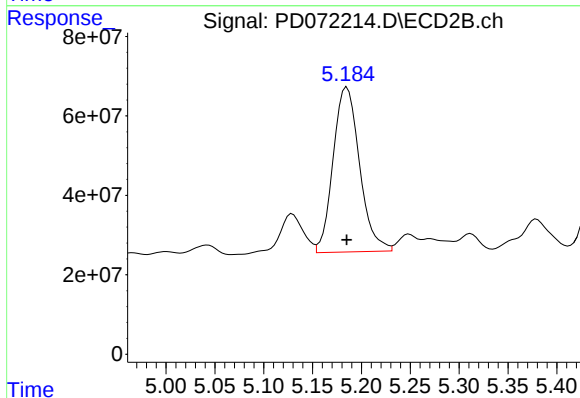


#24 Chlordane-2

R.T.: 5.185 min
Delta R.T.: 0.000 min
Response: 783675001
Conc: 871.42 ng/ml

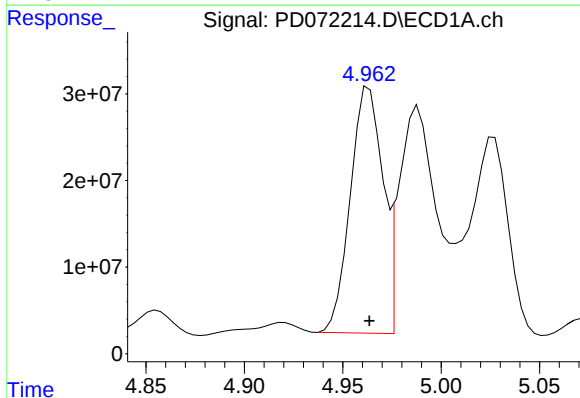


#25 Chlordane-3

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 324628144
Conc: 1011.77 ng/ml

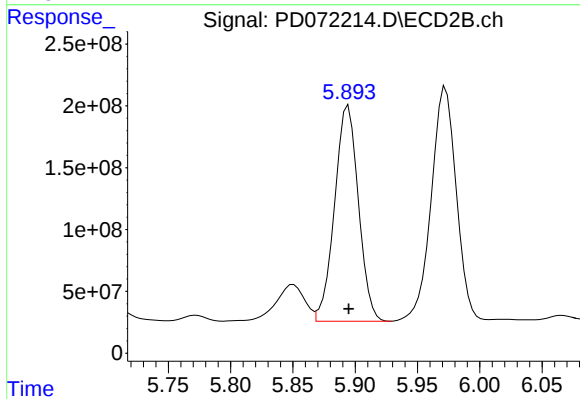

#25 Chlordane-3


R.T.: 5.894 min
Delta R.T.: 0.000 min
Response: 2326907457
Conc: 943.45 ng/ml

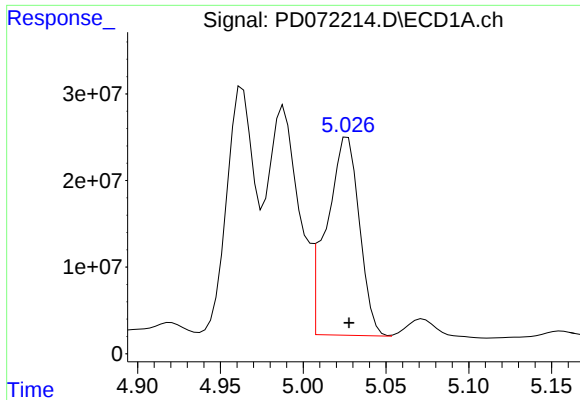

#26 Chlordane-4


R.T.: 5.027 min
Delta R.T.: 0.000 min
Response: 313888038
Conc: 1017.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

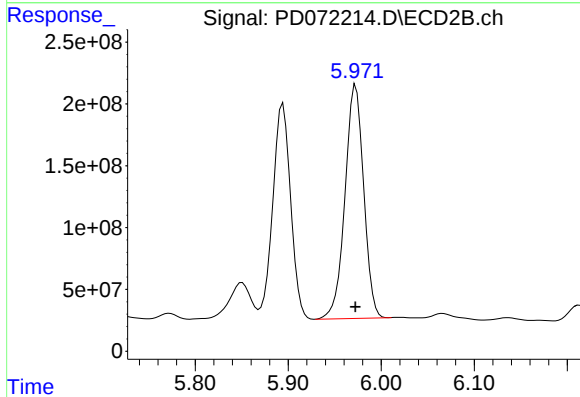


#26 Chlordane-4

R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 2629608381
Conc: 941.89 ng/ml

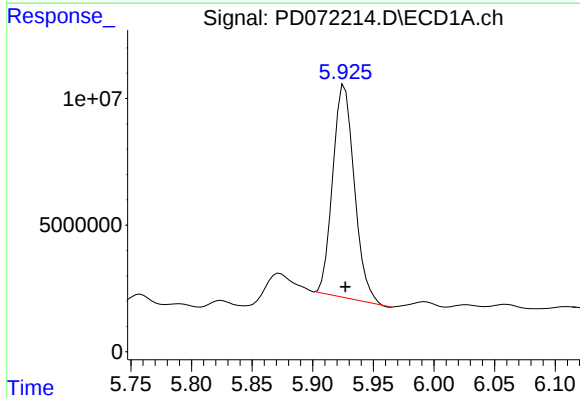


#27 Chlordane-5

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 104221374
Conc: 984.30 ng/ml

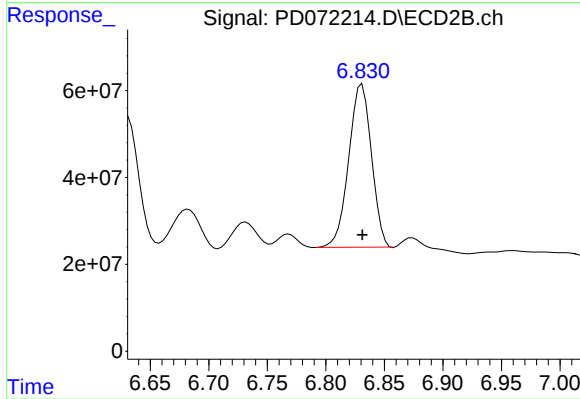

#27 Chlordane-5


R.T.: 6.831 min
Delta R.T.: 0.000 min
Response: 508259368
Conc: 939.90 ng/ml

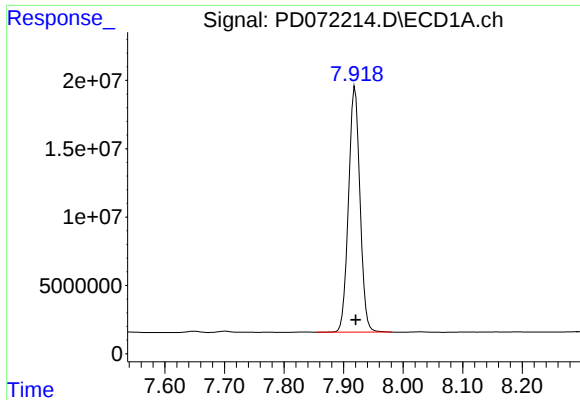

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: -0.001 min
Response: 240073390
Conc: 95.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

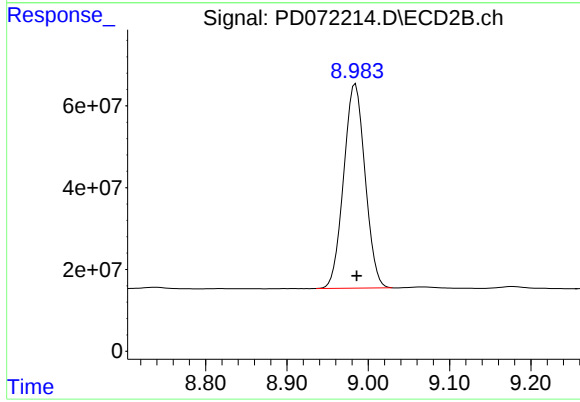

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: -0.001 min
Response: 911168203
Conc: 91.50 ng/ml