

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100522\
 Data File : PD072215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2022 11:30
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 12:30:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 12:29:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.743	3.497	225.6E6	2512.0E6	74.140	71.146
28)	SA Decachlor...	7.919	8.984	183.1E6	698.1E6	72.505	70.100
Target Compounds							
23)	Chlordane-1	3.748	4.653	72577457	799.0E6	733.720	694.932
24)	Chlordane-2	4.328	5.185	80414178	607.2E6	711.197	675.134
25)	Chlordane-3	4.963	5.894	242.5E6	1744.4E6	755.724	707.261
26)	Chlordane-4	5.026	5.972	235.8E6	1966.1E6	764.588	704.242
27)	Chlordane-5	5.926	6.830	78015877	384.5E6	736.811	711.034



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100522\
Data File : PD072215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2022 11:30
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 12:30:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 12:29:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

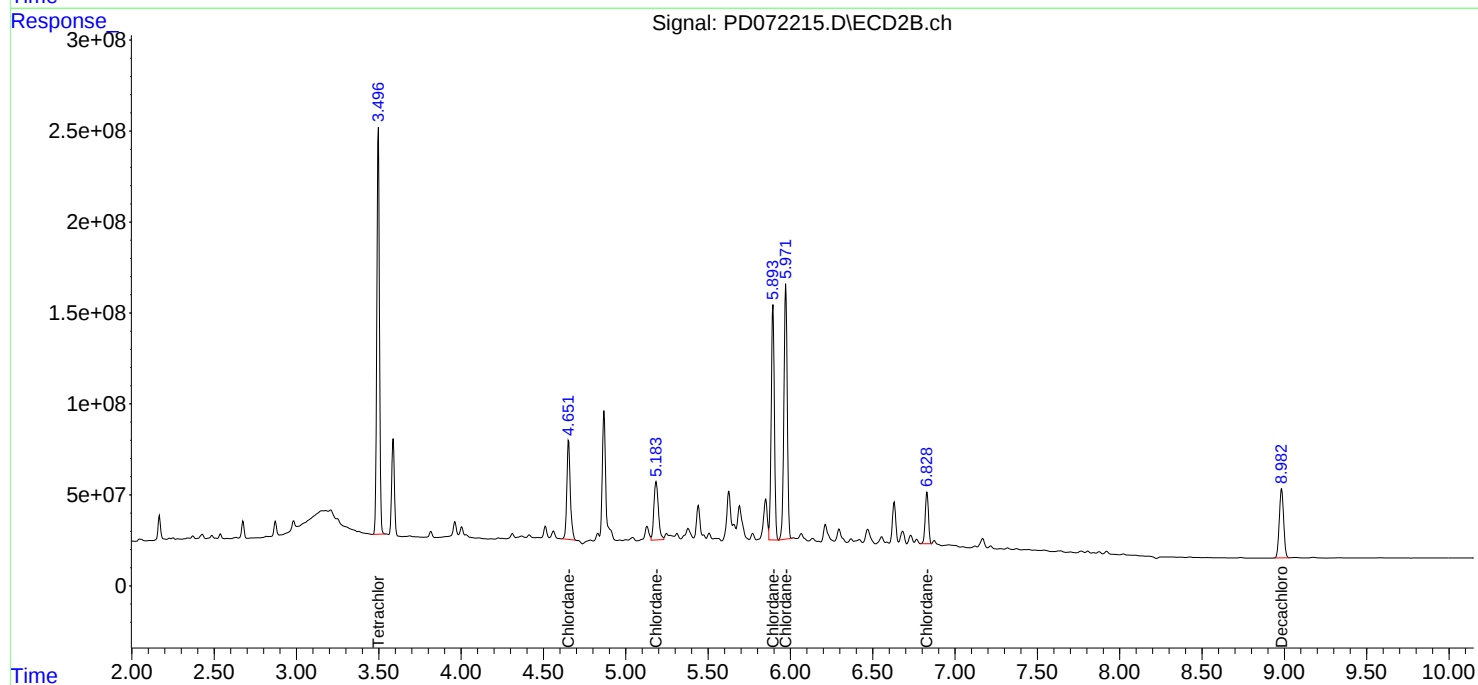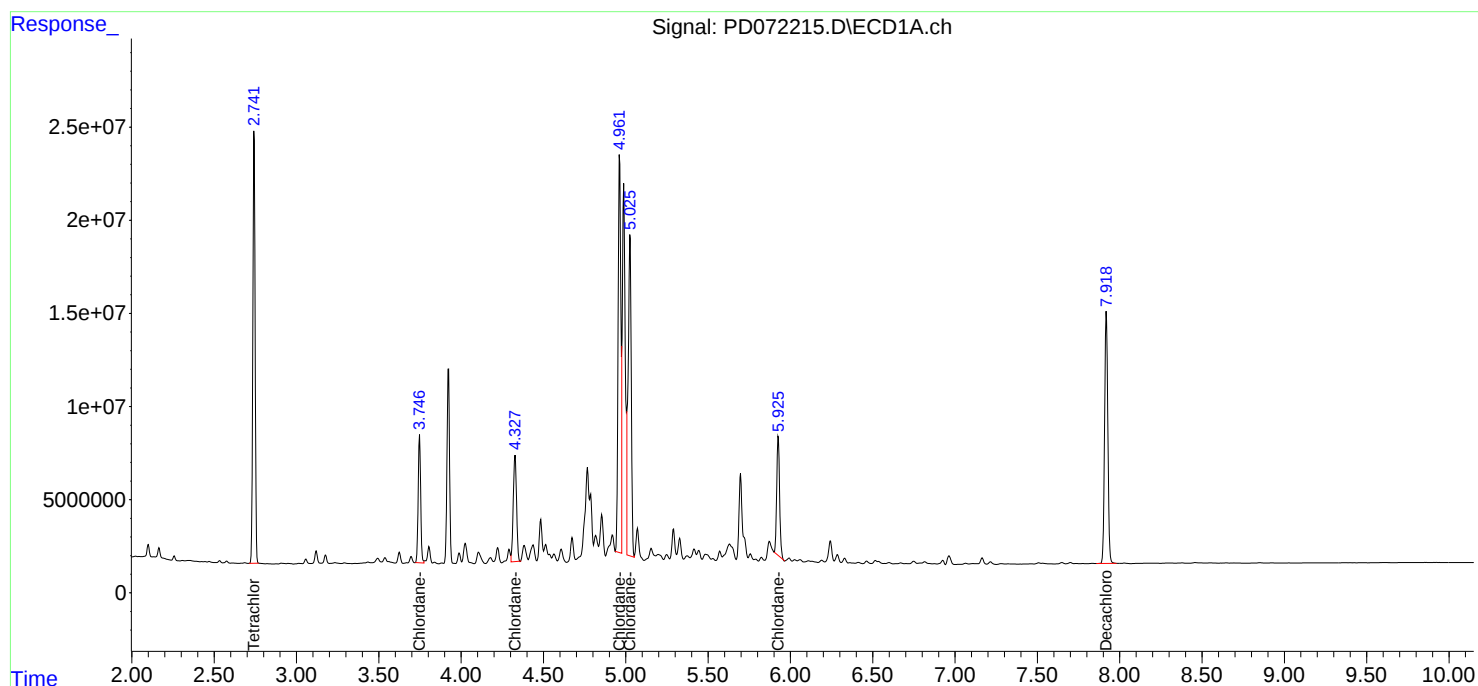


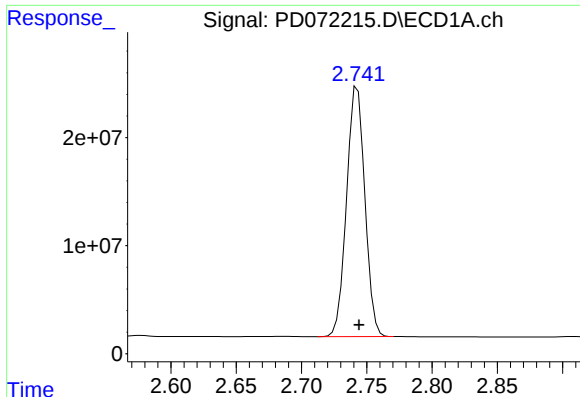

#1 Tetrachloro-m-xylene


R.T.: 2.743 min
Delta R.T.: -0.001 min
Response: 225614357
Conc: 74.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

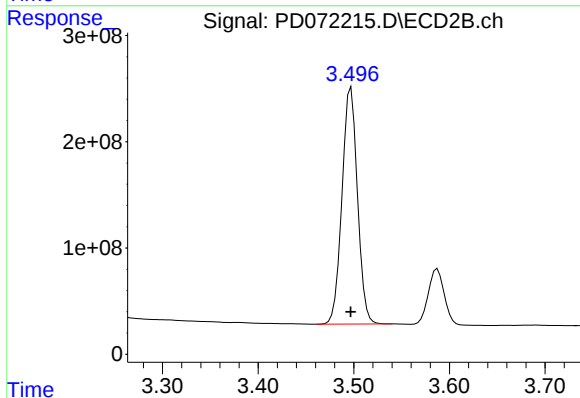


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 2512038294
Conc: 71.15 ng/ml

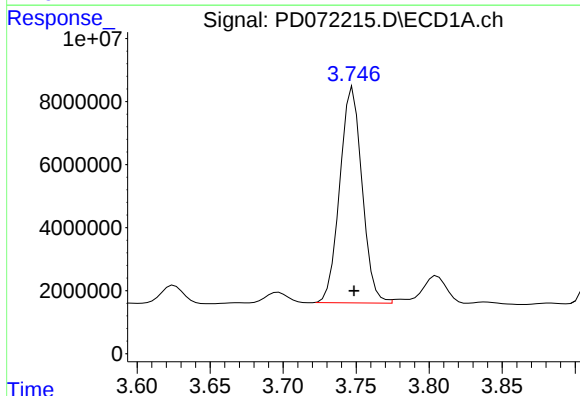


#23 Chlordane-1

R.T.: 3.748 min
Delta R.T.: 0.000 min
Response: 72577457
Conc: 733.72 ng/ml

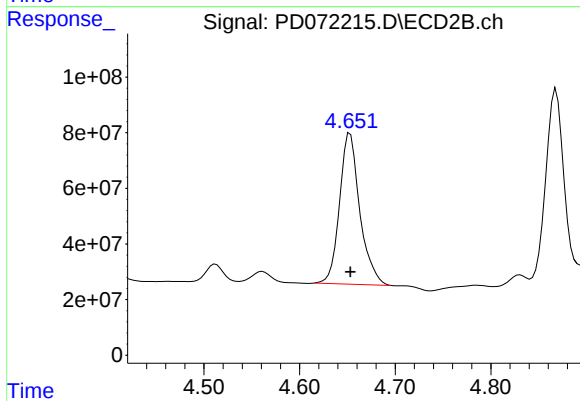

#23 Chlordane-1


R.T.: 4.653 min
Delta R.T.: 0.000 min
Response: 799036034
Conc: 694.93 ng/ml

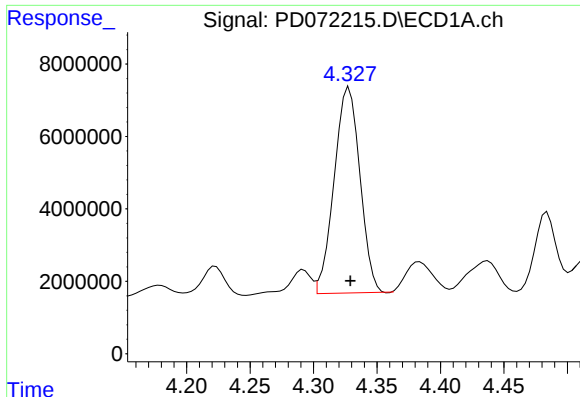

#24 Chlordane-2


R.T.: 4.328 min
Delta R.T.: -0.001 min
Response: 80414178
Conc: 711.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

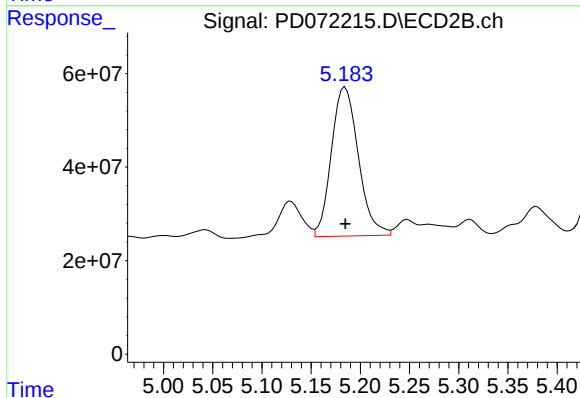


#24 Chlordane-2

R.T.: 5.185 min
Delta R.T.: 0.000 min
Response: 607154913
Conc: 675.13 ng/ml

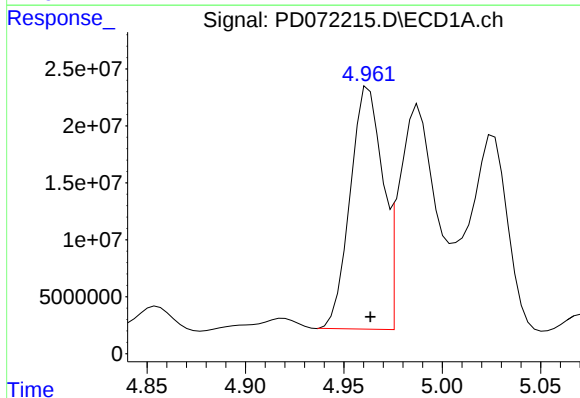


#25 Chlordane-3

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 242474248
Conc: 755.72 ng/ml

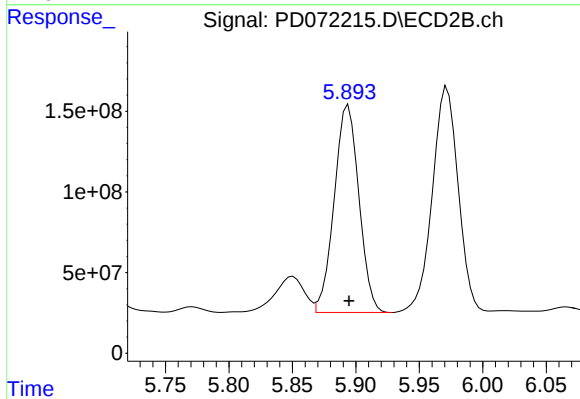

#25 Chlordane-3


R.T.: 5.894 min
Delta R.T.: 0.000 min
Response: 1744378611
Conc: 707.26 ng/ml

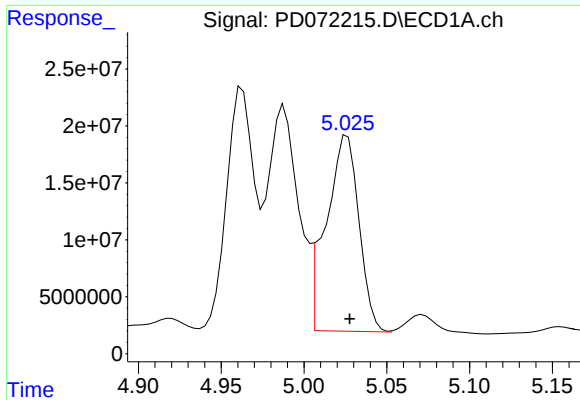

#26 Chlordane-4


R.T.: 5.026 min
Delta R.T.: -0.001 min
Response: 235844509
Conc: 764.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

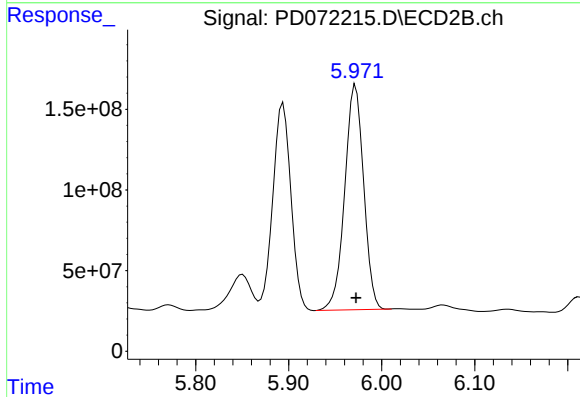


#26 Chlordane-4

R.T.: 5.972 min
Delta R.T.: 0.000 min
Response: 1966123476
Conc: 704.24 ng/ml

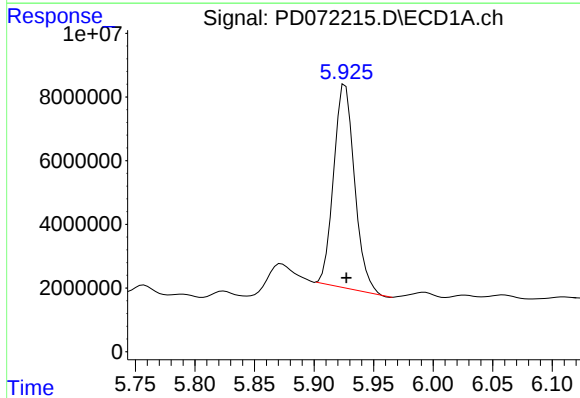


#27 Chlordane-5

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 78015877
Conc: 736.81 ng/ml

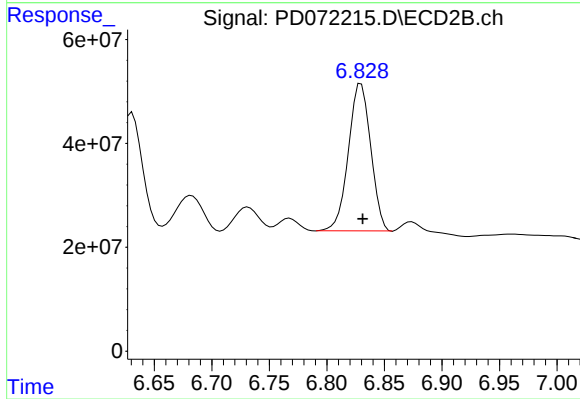

#27 Chlordane-5


R.T.: 6.830 min
Delta R.T.: -0.001 min
Response: 384496369
Conc: 711.03 ng/ml

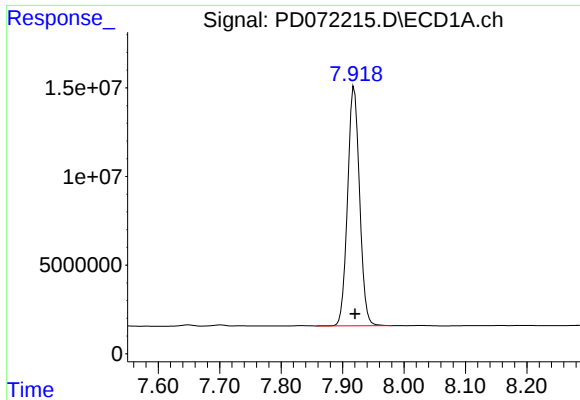

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: -0.001 min
Response: 183131050
Conc: 72.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

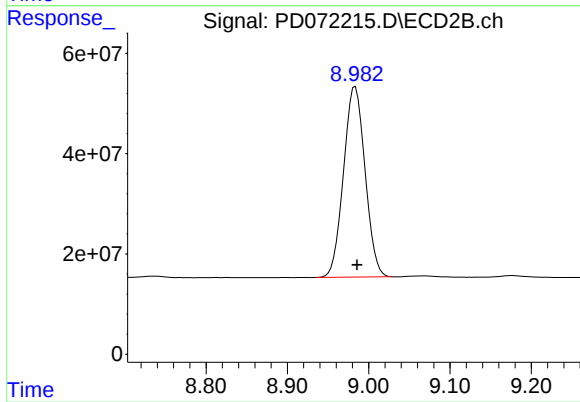

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: -0.002 min
Response: 698051649
Conc: 70.10 ng/ml