

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100522\
 Data File : PD072225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2022 14:46
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD100522

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 15:16:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 15:13:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.744	3.497	153.0E6	1770.0E6	51.187	49.029
28)	SA Decachlor...	7.921	8.986	128.4E6	498.4E6	49.669	49.404
Target Compounds							
23)	Chlordane-1	3.749	4.653	49827977	579.1E6	494.346	496.143
24)	Chlordane-2	4.329	5.185	57031693	446.7E6	495.009	514.301
25)	Chlordane-3	4.964	5.894	162.1E6	1251.2E6	511.405	495.805
26)	Chlordane-4	5.028	5.972	157.1E6	1439.8E6	505.572	503.645
27)	Chlordane-5	5.928	6.831	53462500	273.2E6	516.338	509.586



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100522\
Data File : PD072225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2022 14:46
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD100522

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 15:16:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 15:13:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

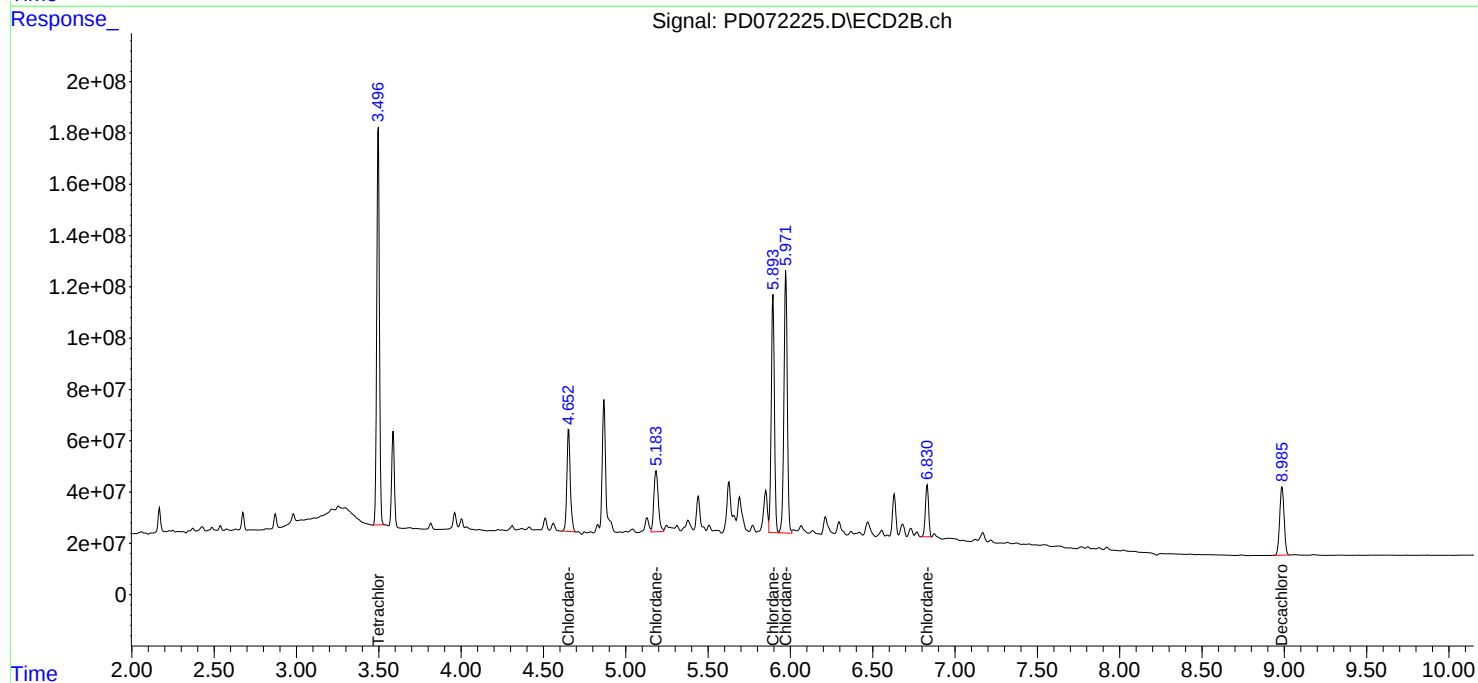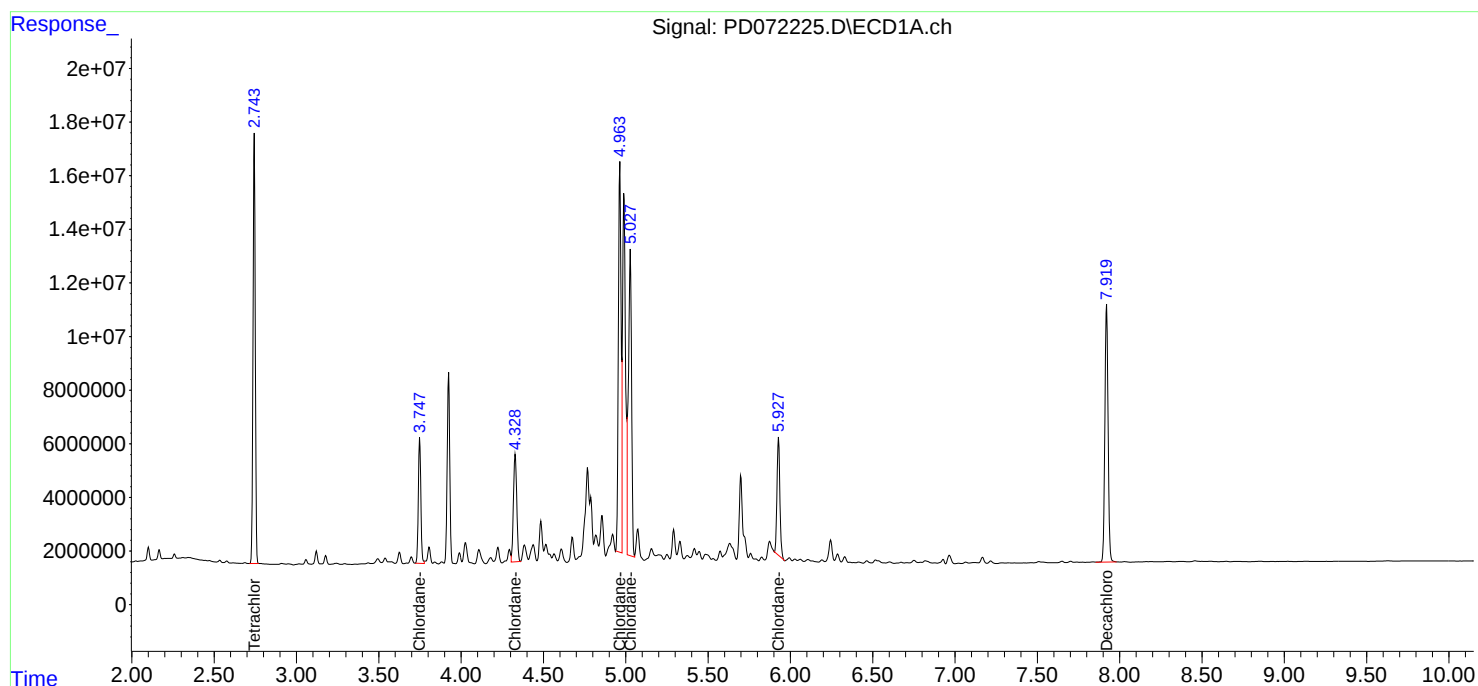


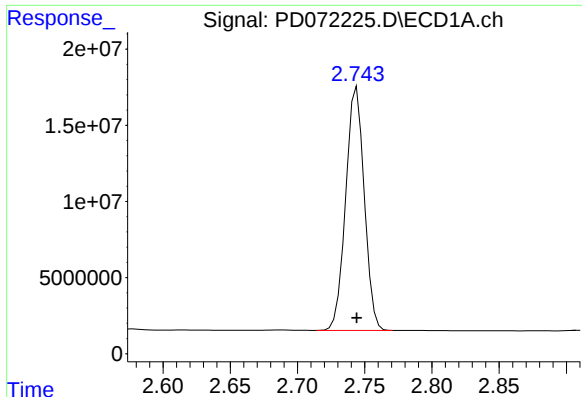

#1 Tetrachloro-m-xylene


R.T.: 2.744 min
Delta R.T.: 0.000 min
Response: 152974915
Conc: 51.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD100522

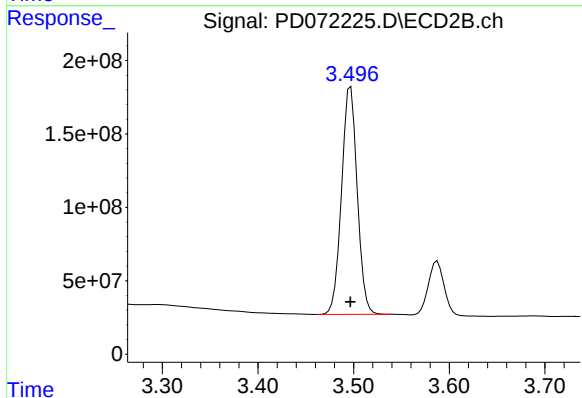


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 1770033999
Conc: 49.03 ng/ml

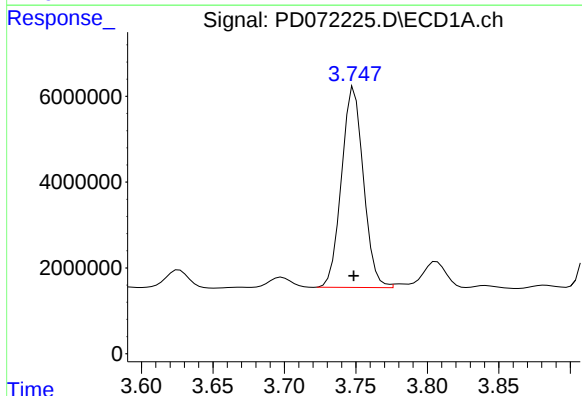


#23 Chlordane-1

R.T.: 3.749 min
Delta R.T.: 0.000 min
Response: 49827977
Conc: 494.35 ng/ml

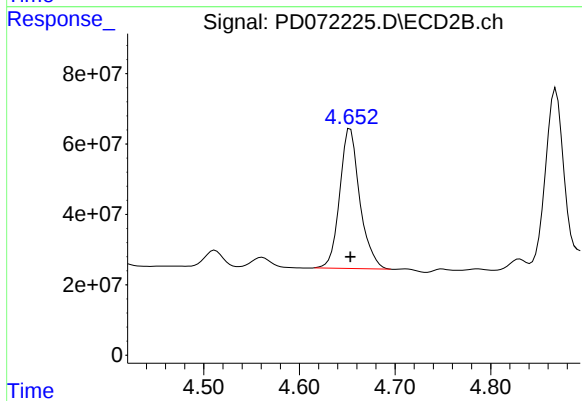

#23 Chlordane-1


R.T.: 4.653 min
Delta R.T.: 0.000 min
Response: 579134593
Conc: 496.14 ng/ml

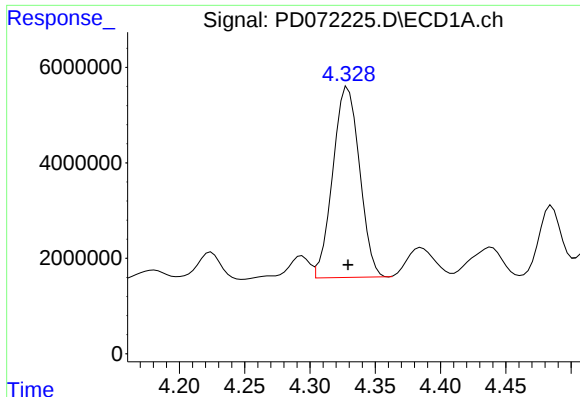

#24 Chlordane-2


R.T.: 4.329 min
Delta R.T.: 0.000 min
Response: 57031693
Conc: 495.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD100522

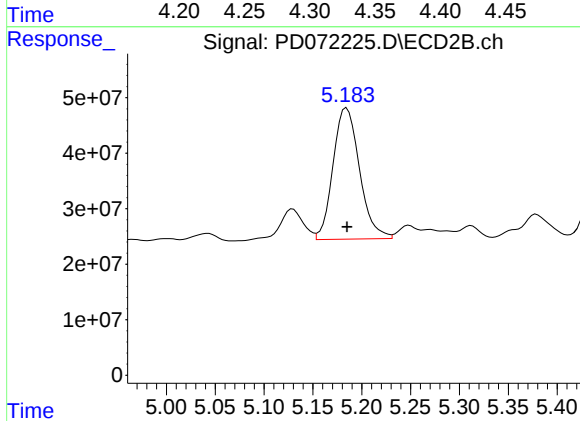


#24 Chlordane-2

R.T.: 5.185 min
Delta R.T.: 0.000 min
Response: 446749381
Conc: 514.30 ng/ml

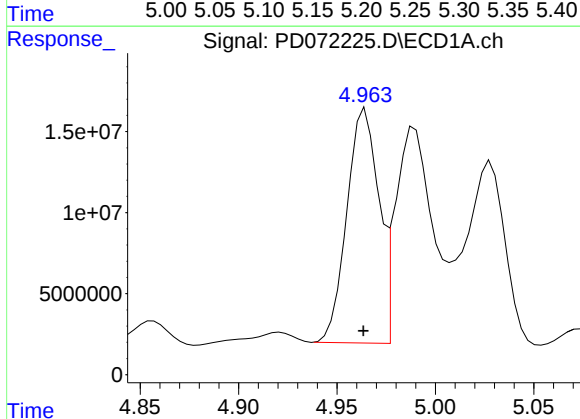


#25 Chlordane-3

R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 162070056
Conc: 511.41 ng/ml

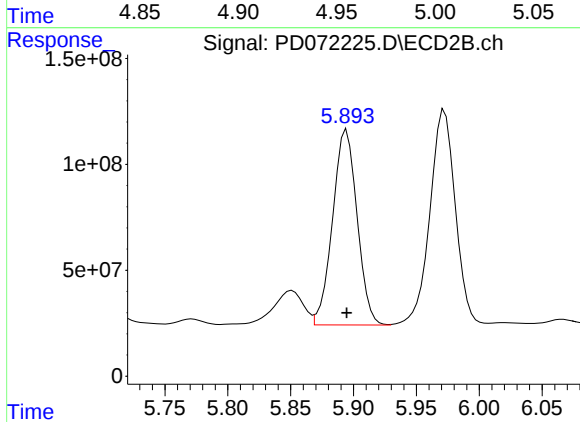

#25 Chlordane-3


R.T.: 5.894 min
Delta R.T.: 0.000 min
Response: 1251152325
Conc: 495.80 ng/ml

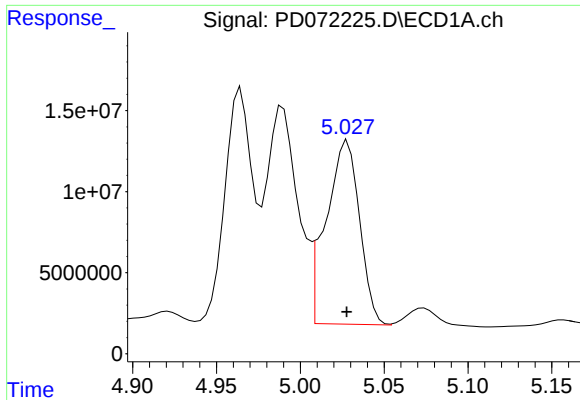

#26 Chlordane-4


R.T.: 5.028 min
Delta R.T.: 0.000 min
Response: 157116754
Conc: 505.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD100522

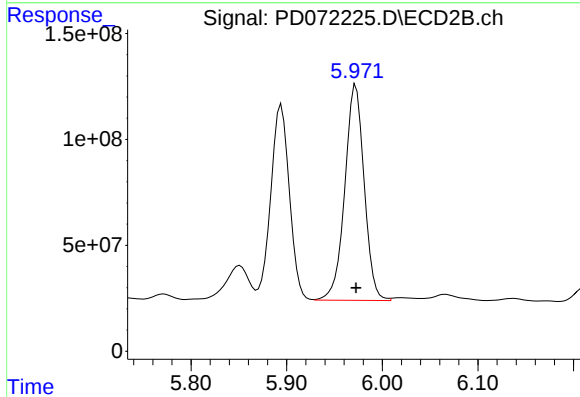


#26 Chlordane-4

R.T.: 5.972 min
Delta R.T.: 0.000 min
Response: 1439772858
Conc: 503.65 ng/ml

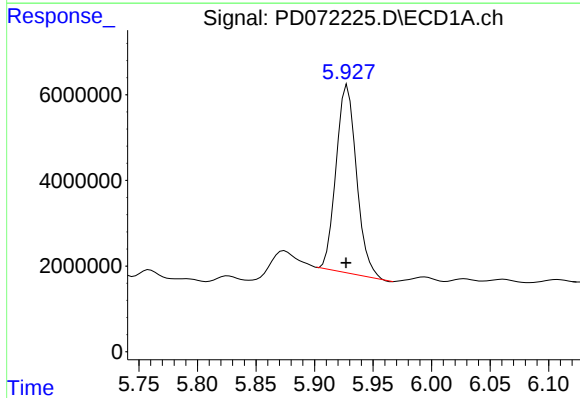


#27 Chlordane-5

R.T.: 5.928 min
Delta R.T.: 0.001 min
Response: 53462500
Conc: 516.34 ng/ml

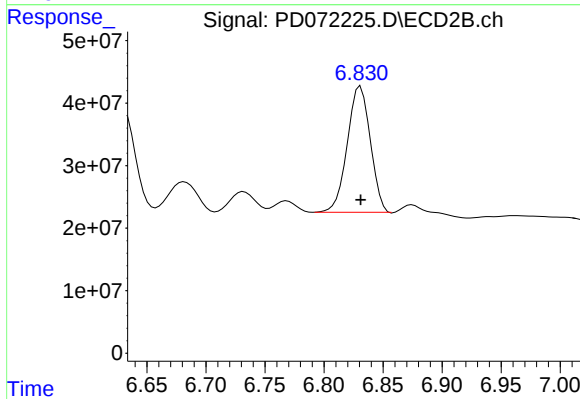

#27 Chlordane-5


R.T.: 6.831 min
Delta R.T.: 0.000 min
Response: 273232317
Conc: 509.59 ng/ml

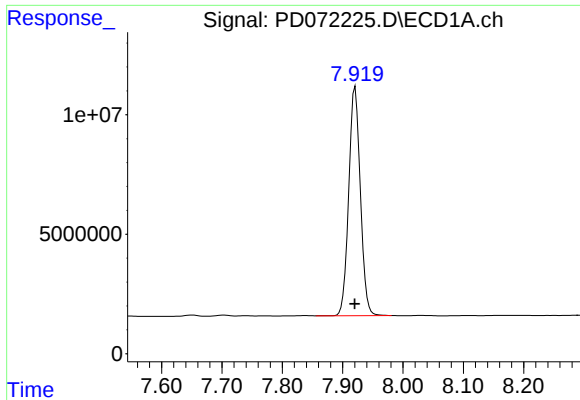

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: 0.000 min
Response: 128361230
Conc: 49.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD100522

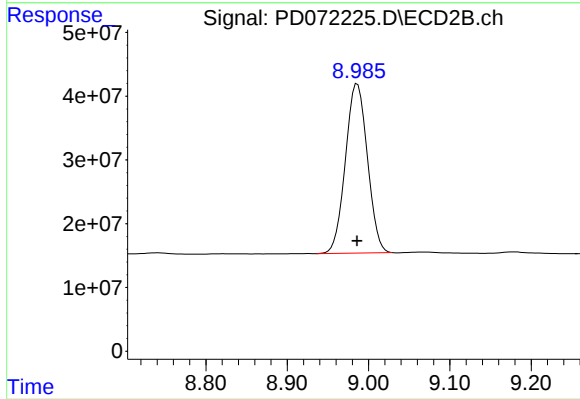

#28 Decachlorobiphenyl

R.T.: 8.986 min
Delta R.T.: 0.000 min
Response: 498384341
Conc: 49.40 ng/ml