

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100523\
 Data File : PD078651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 09:36
 Operator : AR\AJ
 Sample : PB156000BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS000

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/05/2023
 Supervised By :Ankita Jodhani 10/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 21:18:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 28 13:47:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.758	47733864	32082615	19.440	19.420
27)	SA Decachlor...	9.086	7.896	105.3E6	64846794	32.576	35.028
Target Compounds							
2)	A alpha-BHC	4.003	3.259	19622583	11965861	4.733	4.694
3)	MA gamma-BHC...	4.336	3.589	18478308	11515720	4.658	4.822
4)	MA Heptachlor	4.926	3.928	21357466	12771978	5.141	5.140
5)	MB Aldrin	5.269	4.207	21742974	13047242	5.348	5.318
6)	B beta-BHC	4.534	3.887	9239879	5931209	5.342	5.448
7)	B delta-BHC	4.780	4.116	16401018	6304867	4.115	2.565 #
8)	B Heptachlo...	5.696	4.709	18616298	12108129	5.025	5.247
9)	A Endosulfan I	6.082	5.079	18438808	11469858	5.532m	5.576
10)	B trans-Chl...	5.953	4.960	19593009	12031288	5.433	5.400
11)	B cis-Chlor...	6.032	5.024	19190930	12350094	5.173	5.377
12)	B 4,4'-DDE	6.205	5.212	38627388	23669576	10.795	10.997
13)	MA Dieldrin	6.359	5.344	38647088	24421567	10.388	10.339
14)	MA Endrin	6.589	5.620	29579342	21452727	9.840	10.254
15)	B Endosulfa...	6.809	5.915	34226113	22333902	10.944	11.001
16)	A 4,4'-DDD	6.723	5.767	27615316	18564202	10.670	11.781
17)	MA 4,4'-DDT	7.038	6.018	26292983	16878625	10.180	10.375
18)	B Endrin al...	6.939	6.094	26682776	17664175	10.981	11.394
19)	B Endosulfa...	7.175	6.317	28137643	18965467	9.853	10.189
20)	A Methoxychlor	7.515	6.593	79526432	53389774	53.892	60.191
21)	B Endrin ke...	7.661	6.823	34545809	24323890	10.864	11.323

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100523\
Data File : PD078651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 09:36
Operator : AR\AJ
Sample : PB156000BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 21:18:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 28 13:47:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

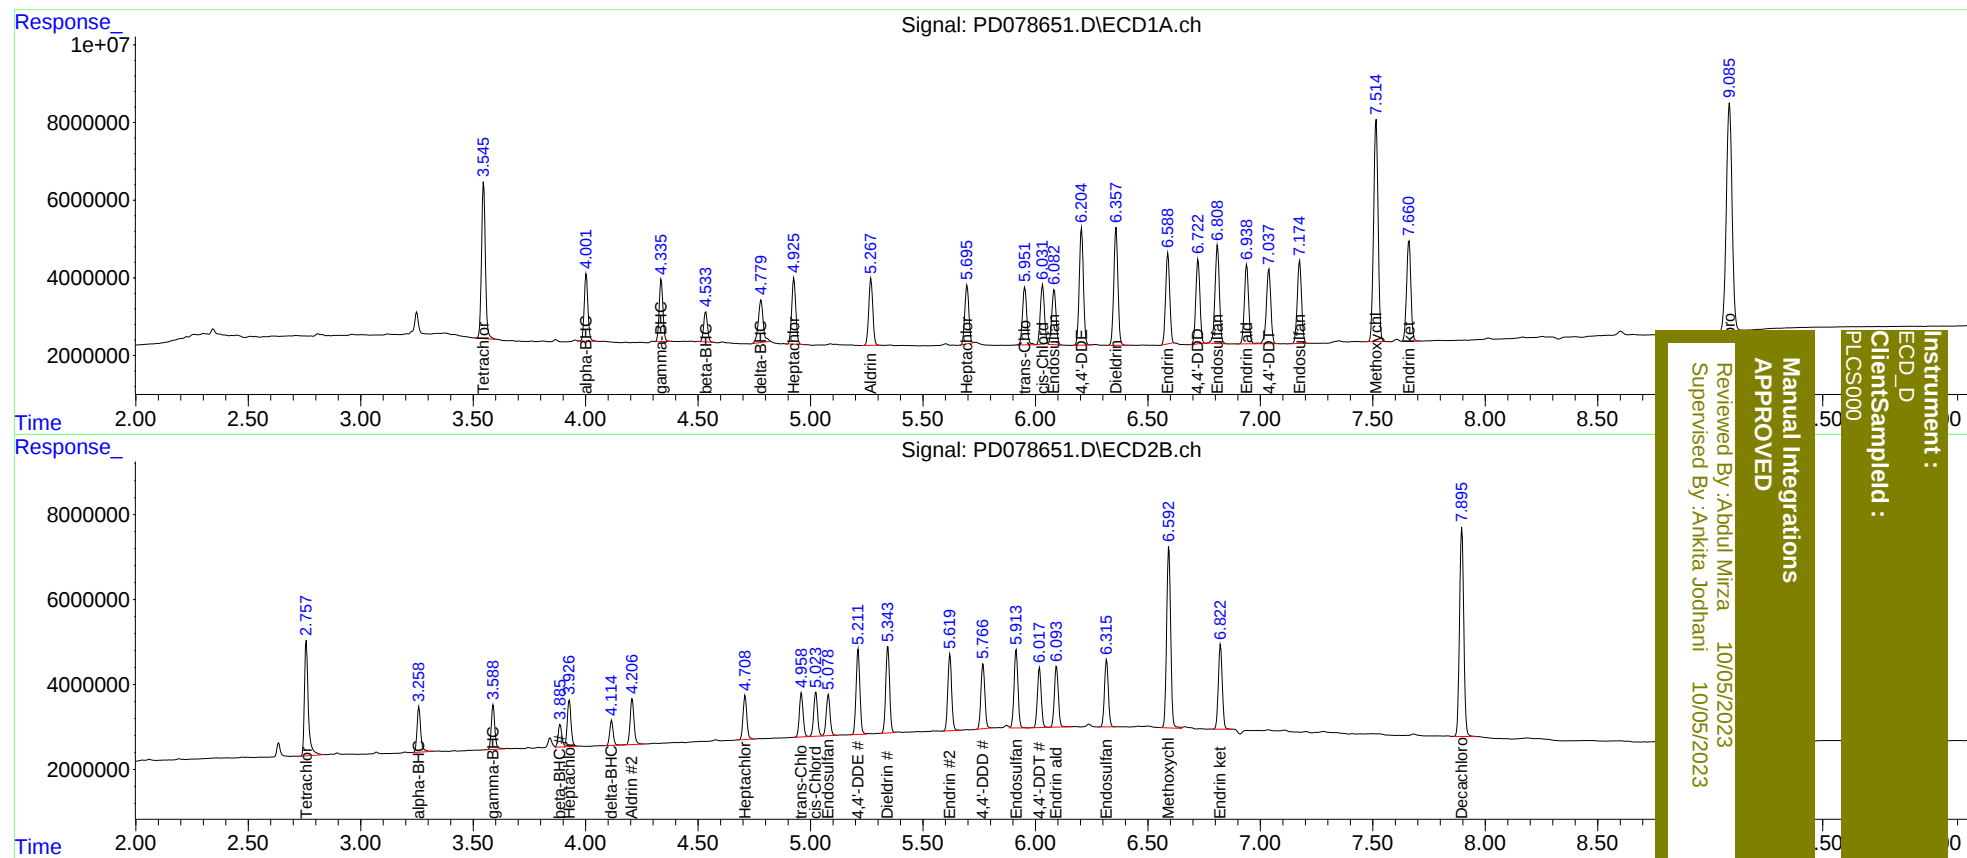

Instrument :
ECD_D
ClientSampled :
PLCS000

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 10/05/2023
Supervised By: Ankita Jodhani 10/05/2023