

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100523\
 Data File : PD078668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 13:56
 Operator : AR\AJ
 Sample : 04624-04MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BBJR1MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/05/2023
 Supervised By : Ankita Jodhani 10/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 21:24:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 28 13:47:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.758	50193215	32974043	20.441	19.960
27)	SA Decachlor...	9.078	7.893	40361011	21862006	12.486	11.809
Target Compounds							
2)	A alpha-BHC	3.997	3.257	230.6E6	146.3E6	55.619	57.384m
3)	MA gamma-BHC...	4.328	3.588	197.3E6	130.1E6	49.723m	54.485
4)	MA Heptachlor	4.920	3.926	201.7E6	132.4E6	48.543	53.270
5)	MB Aldrin	5.263	4.205	197.5E6	126.0E6	48.591	51.371
6)	B beta-BHC	4.528	3.885	83357569	54666688	48.191	50.216
7)	B delta-BHC	4.776	4.114	165.0E6	107.6E6	41.392	43.755
8)	B Heptachlo...	5.690	4.708	181.3E6	125.0E6	48.953	54.167
9)	A Endosulfan I	6.076	5.077	165.6E6	106.9E6	49.681m	51.956
10)	B trans-Chl...	5.947	4.957	170.2E6	117.5E6	47.204	52.753
11)	B cis-Chlor...	6.026	5.022	163.3E6	118.4E6	44.011	51.533
12)	B 4,4'-DDE	6.198	5.210	346.1E6	226.7E6	96.707	105.321
13)	MA Dieldrin	6.352	5.342	370.7E6	249.6E6	99.652	105.662
14)	MA Endrin	6.583	5.618	299.9E6	223.4E6	99.771	106.801
15)	B Endosulfa...	6.803	5.912	305.1E6	213.5E6	97.568	105.179
16)	A 4,4'-DDD	6.717	5.765	263.1E6	173.9E6	101.668	110.380
17)	MA 4,4'-DDT	7.032	6.016	270.7E6	185.1E6	104.800	113.774
18)	B Endrin al...	6.933	6.091	217.9E6	152.1E6	89.691	98.085
19)	B Endosulfa...	7.168	6.314	256.0E6	187.0E6	89.656	100.492
20)	A Methoxychlor	7.508	6.591	726.1E6	481.9E6	492.015	543.265
21)	B Endrin ke...	7.655	6.821	306.9E6	216.3E6	96.516	100.696

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100523\
Data File : PD078668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 13:56
Operator : AR\AJ
Sample : 04624-04MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 21:24:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 28 13:47:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

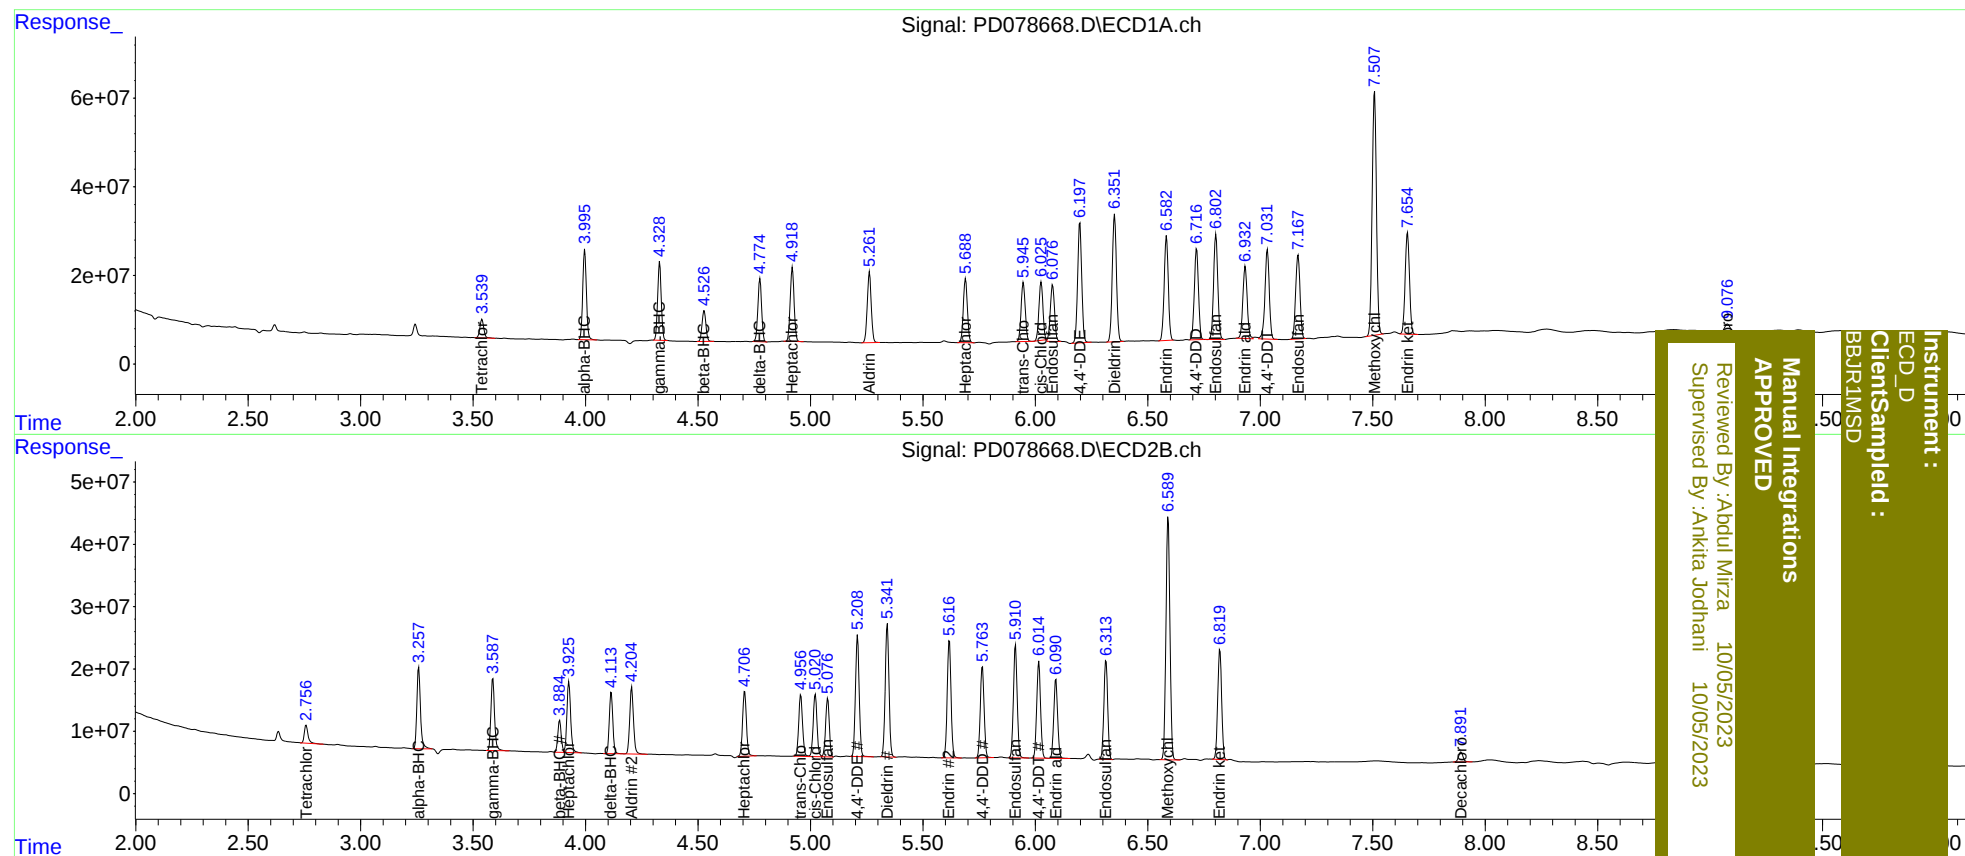

Instrument :
ECD_D
Client Sampled :
BBJRMMSD

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 10/05/2023
Supervised By: Ankita Jodhani 10/05/2023