

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100620\
 Data File : PD059523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 17:35
 Operator : DD\AJ
 Sample : L4259-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5CF4

Manual Integrations
 APPROVED

Ankita
 10/7/2020 3:34:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 02:08:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:21:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.509	4.024	36174676	43815983	25.043m	22.060m
27)	SA Decachlor...	8.316	9.111	39015993	54931684	36.413	36.921
Target Compounds							
8)	B Heptachlo...	5.246	5.906	6032980	13068640	3.727m	5.822 #
10)	B trans-Chl...	5.477	6.138	1724425	3454408	1.062	1.548m#
11)	B cis-Chlor...	5.536	6.215	3431506	5513580	2.119	2.521
13)	MA Dieldrin	5.836	6.523	29722930	40282192	18.123	18.070

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100620\
Data File : PD059523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2020 17:35
Operator : DD\AJ
Sample : L4259-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:08:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

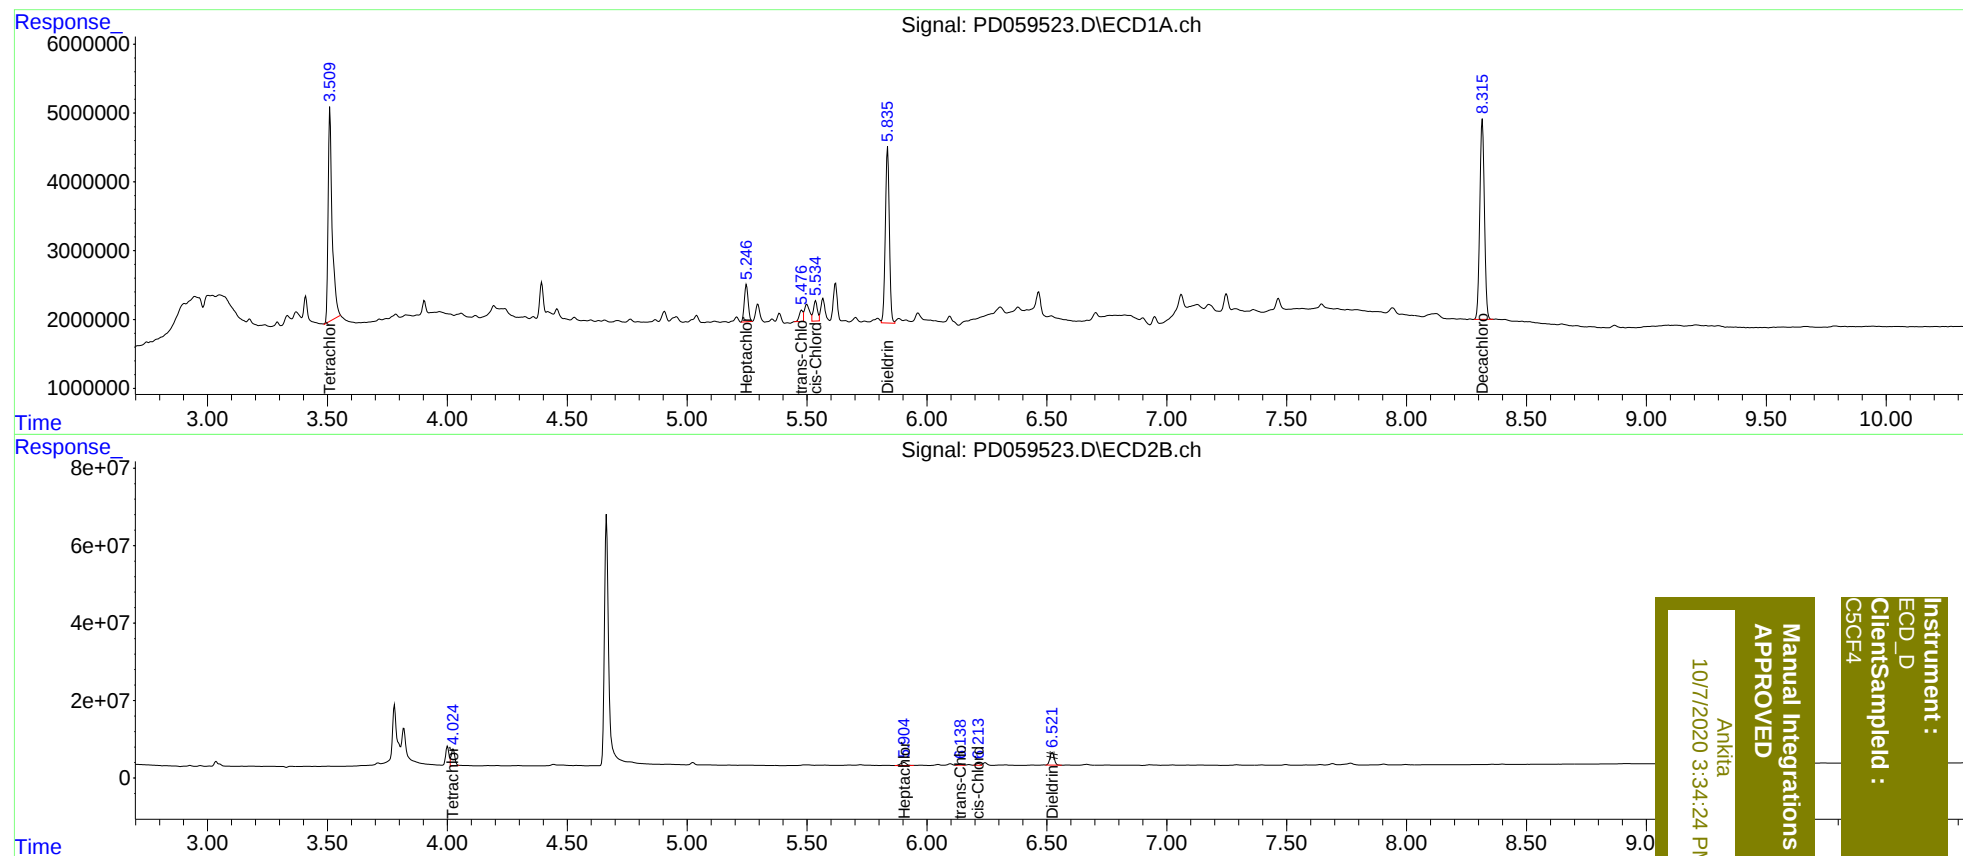

Manual Integrations
APPROVED

Ankita
10/7/2020 3:34:24 PM

Instrument :
ECD_D
ClientSampled :
C5CF4