

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100621\
 Data File : PD066043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2021 15:53
 Operator : AR\AJ
 Sample : PB139664TB
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB139664TB

Manual Integrations
 APPROVED

mohammad
 10/7/2021 9:05:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 22:25:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.498	0.000	489593	0	0.661m	N.D. #
28) SA Decachlor...	0.000	9.078	0	266343	N.D.	0.069 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100621\
Data File : PD066043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2021 15:53
Operator : AR\AJ
Sample : PB139664TB
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PB139664TB


Manual Integrations
APPROVED

mohammad
10/7/2021 9:05:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 22:25:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

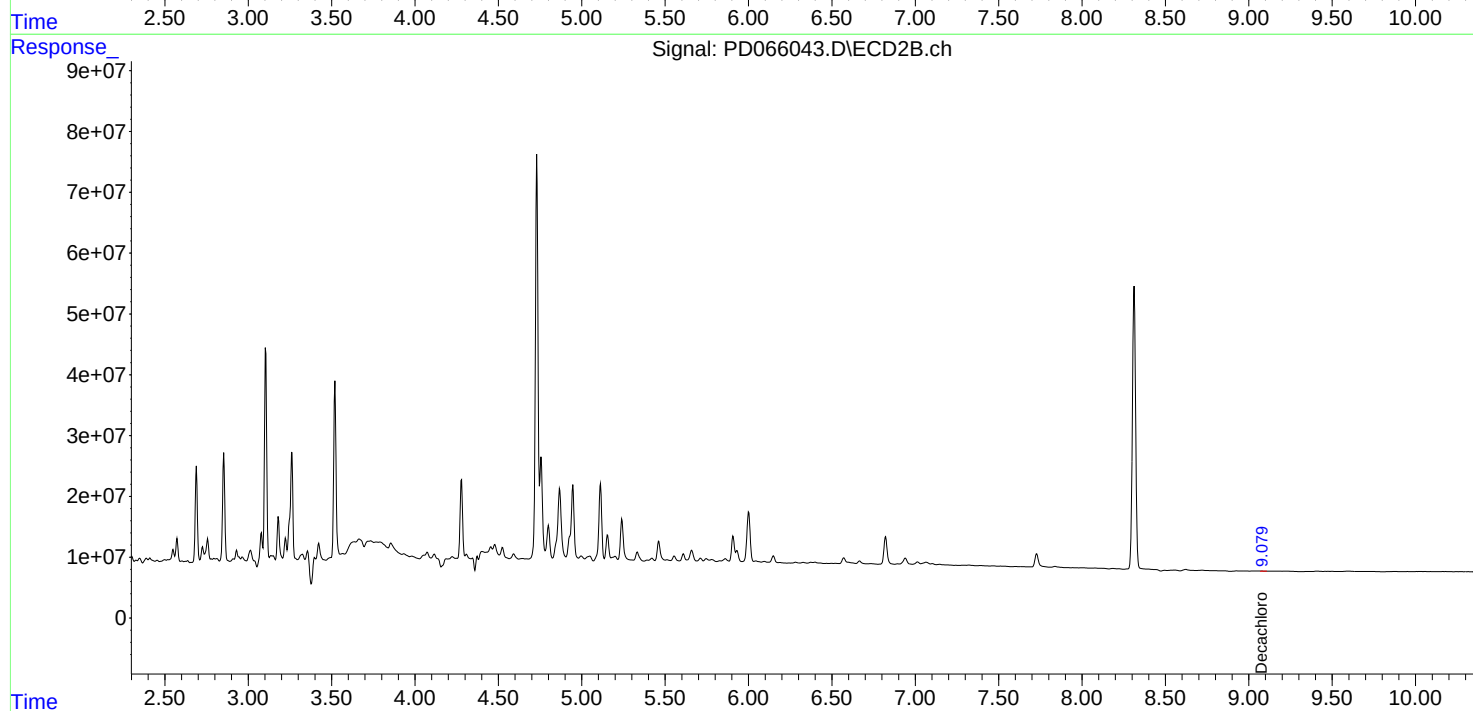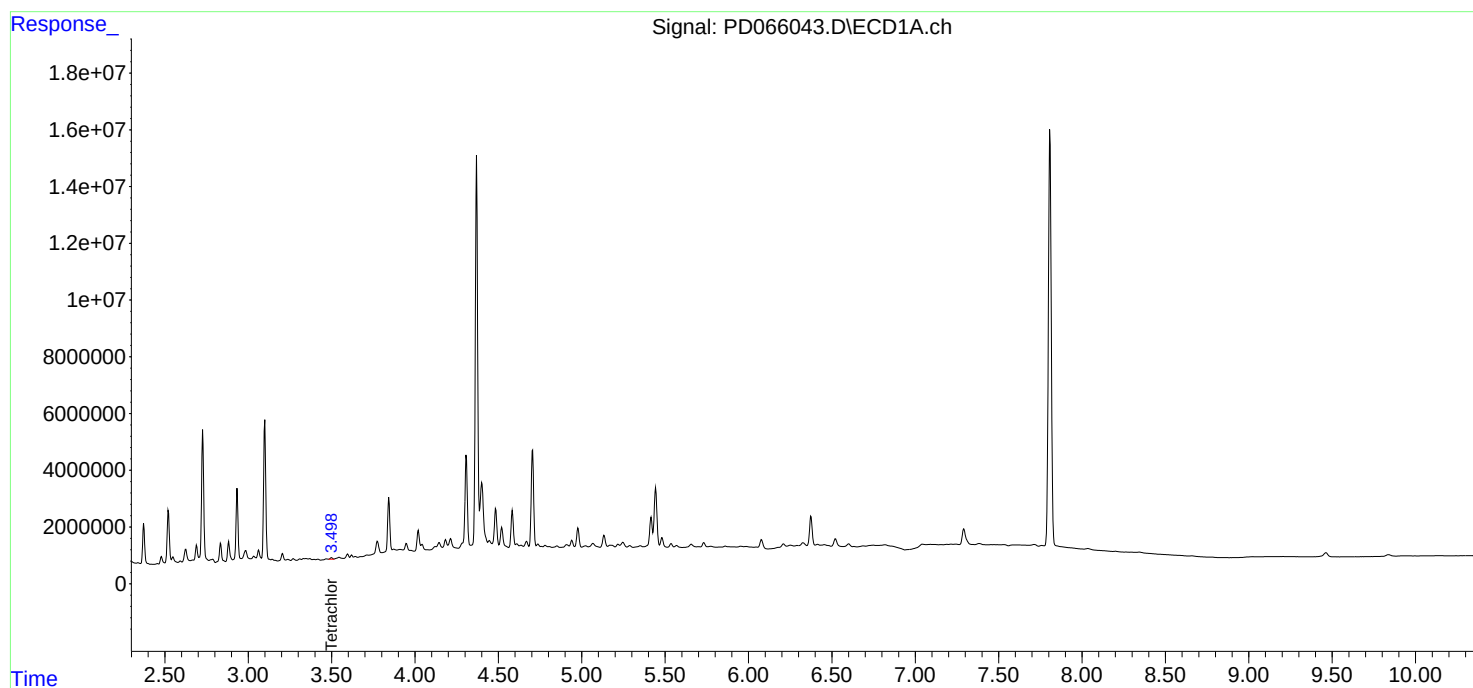

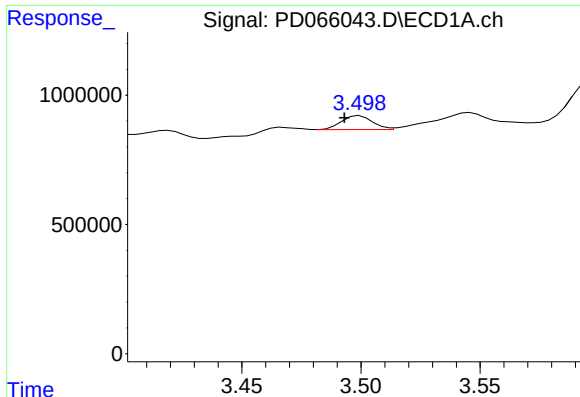


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: 0.005 min
Response: 489593
Conc: 0.66 ng/ml m

Instrument :
ECD_D
ClientSampleId :
PB139664TB


Manual Integrations
APPROVED

mohammad
10/7/2021 9:05:26 AM

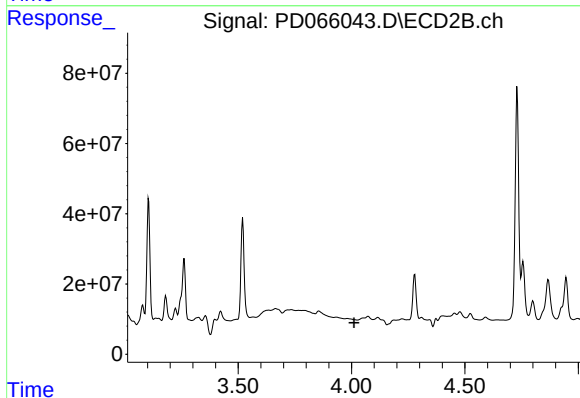


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.012 min
Response: 0
Conc: N.D.

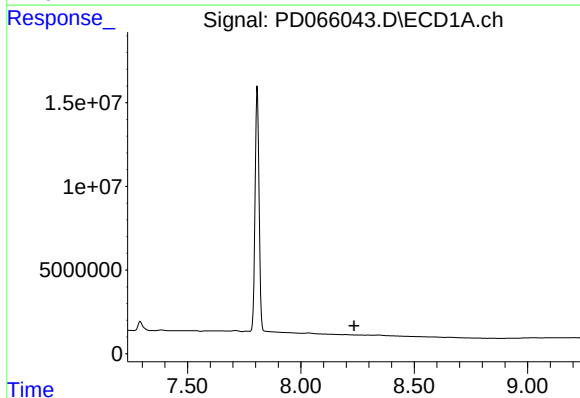

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.235 min
Response: 0
Conc: N.D.

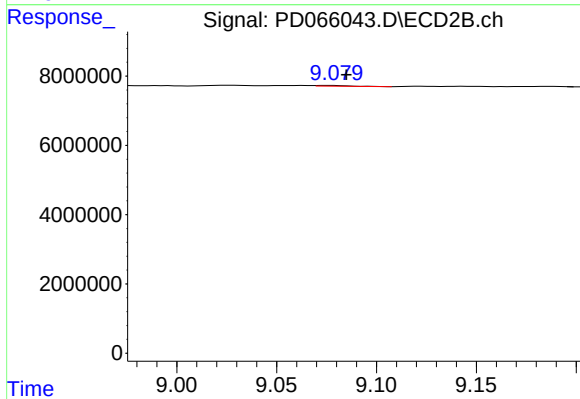

#28 Decachlorobiphenyl

R.T.: 9.078 min
Delta R.T.: -0.007 min
Response: 266343
Conc: 0.07 ng/ml