

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100621\
 Data File : PD066051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2021 17:50
 Operator : AR\AJ
 Sample : M4057-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SHAFT-17B-SP

Manual Integrations
 APPROVED

mohammad
 10/7/2021 9:05:31 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 22:28:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.512f	3.997f	115.1E6	100.1E6	155.460m	17.436m#
28)	SA Decachlor...	8.259f	9.074	4108945	6280085	3.008	1.623 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100621\
Data File : PD066051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2021 17:50
Operator : AR\AJ
Sample : M4057-02
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SHAFT-17B-SP


Manual Integrations
APPROVED

mohammad
10/7/2021 9:05:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 22:28:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

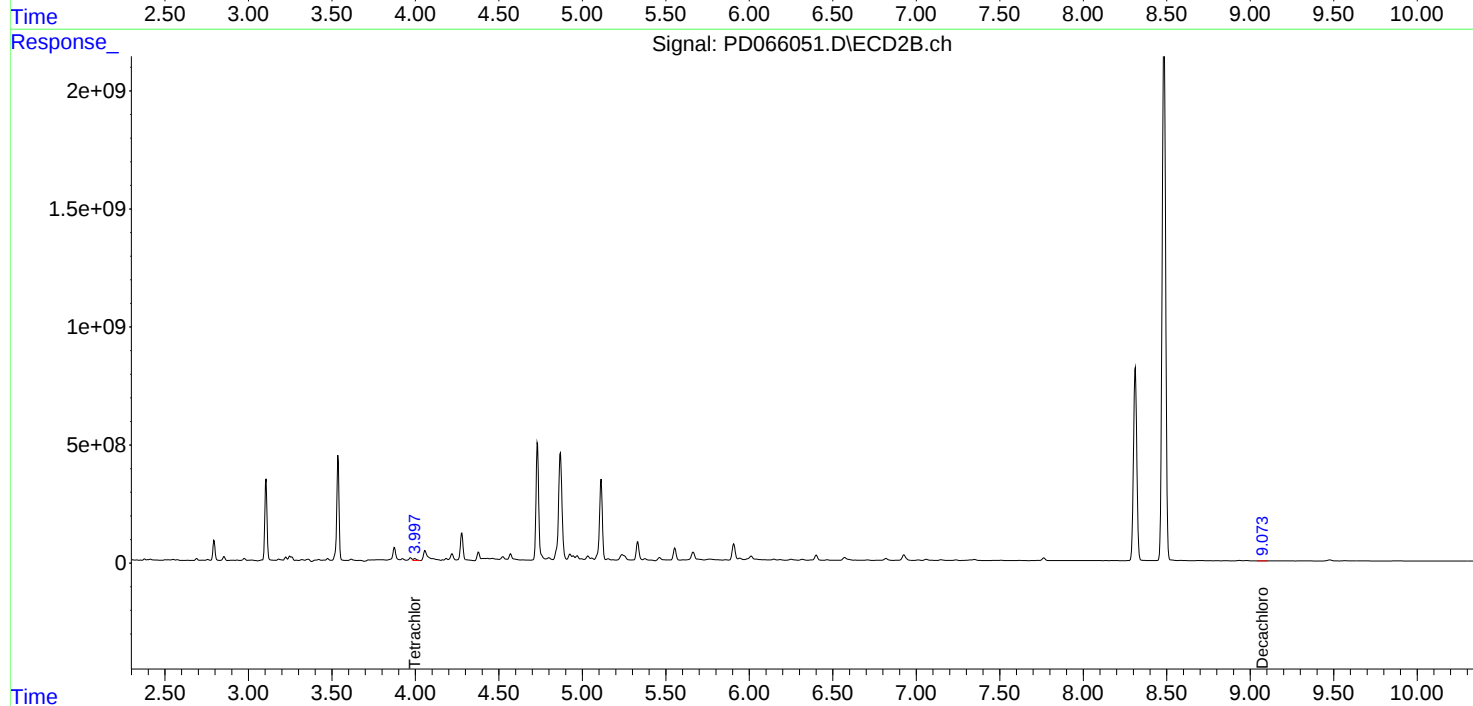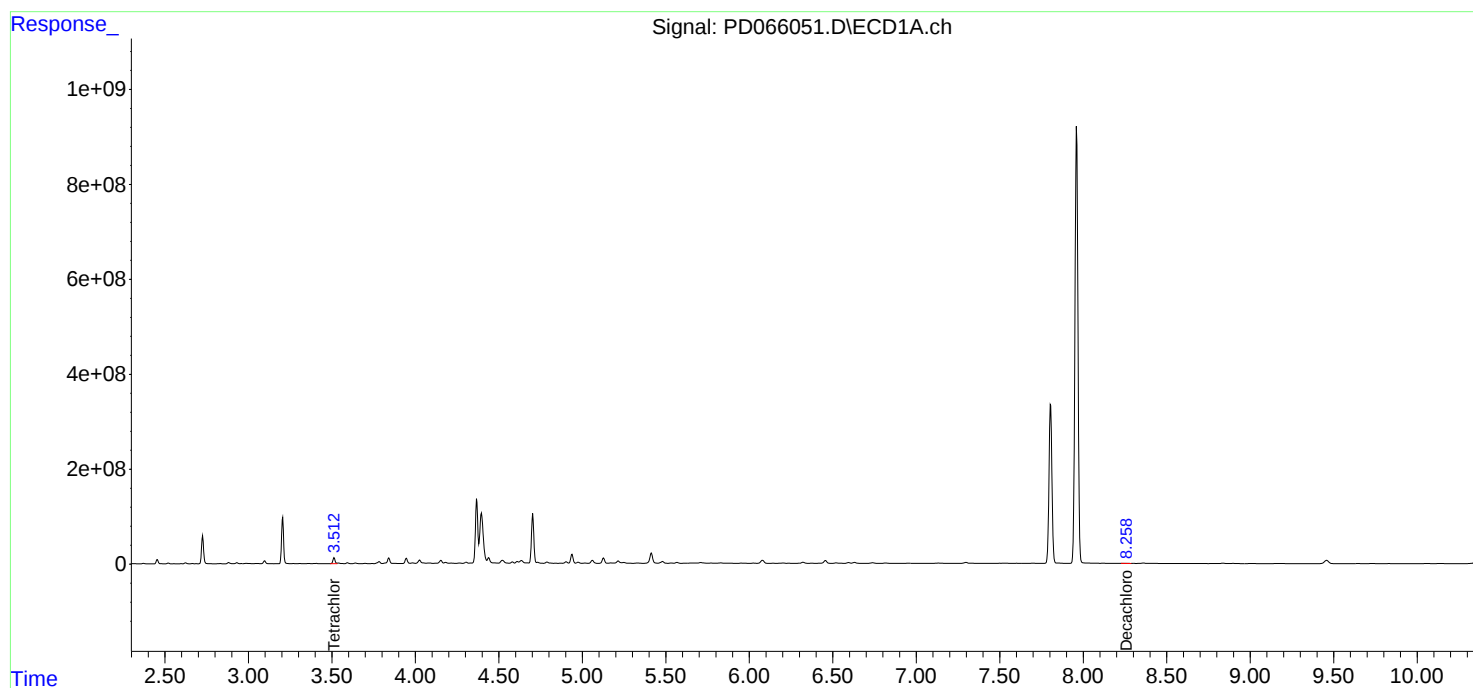

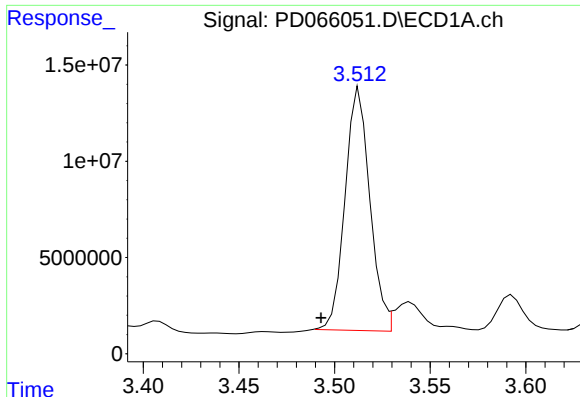

#1 Tetrachloro-m-xylene

R.T.: 3.512 min

Delta R.T.: 0.019 min


Response: 115126798

Conc: 155.46 ng/ml m

Instrument :
ECD_D
ClientSampleId :
SHAFT-17B-SP

Manual Integrations
APPROVED

mohammad
10/7/2021 9:05:31 AM

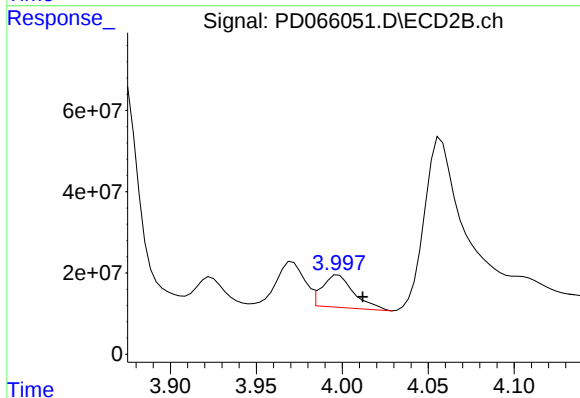


#1 Tetrachloro-m-xylene

R.T.: 3.997 min

Delta R.T.: -0.015 min

Response: 100121246

Conc: 17.44 ng/ml m

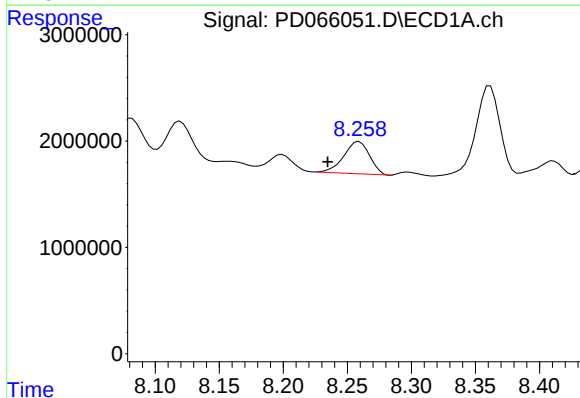


#28 Decachlorobiphenyl

R.T.: 8.259 min

Delta R.T.: 0.024 min

Response: 4108945

Conc: 3.01 ng/ml

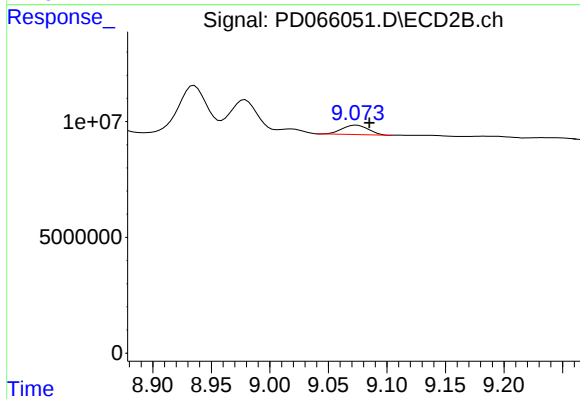

#28 Decachlorobiphenyl

R.T.: 9.074 min

Delta R.T.: -0.011 min

Response: 6280085

Conc: 1.62 ng/ml