

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100622\
 Data File : PD072242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2022 12:07
 Operator : AR\AJ
 Sample : N4988-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 AU-5-100422

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 00:26:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 15:15:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.744	3.497	25934707	396.5E6	10.334	10.936
28)	SA Decachlor...	7.919	8.985	32156773	134.4E6	12.615	13.381
Target Compounds							
12)	B 4,4'-DDE	5.219	6.143	1057343	5807720	0.347	0.326m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100622\
Data File : PD072242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2022 12:07
Operator : AR\AJ
Sample : N4988-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
AU-5-100422

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 00:26:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 15:15:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

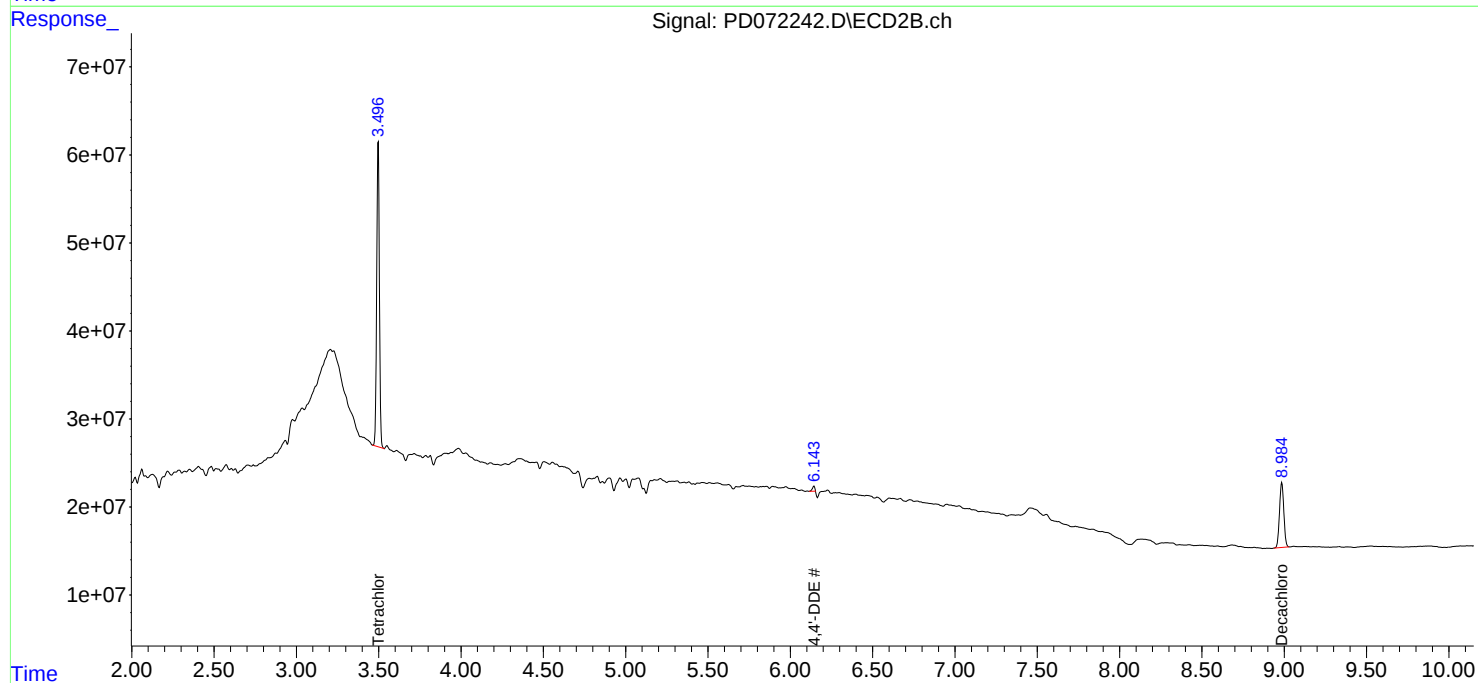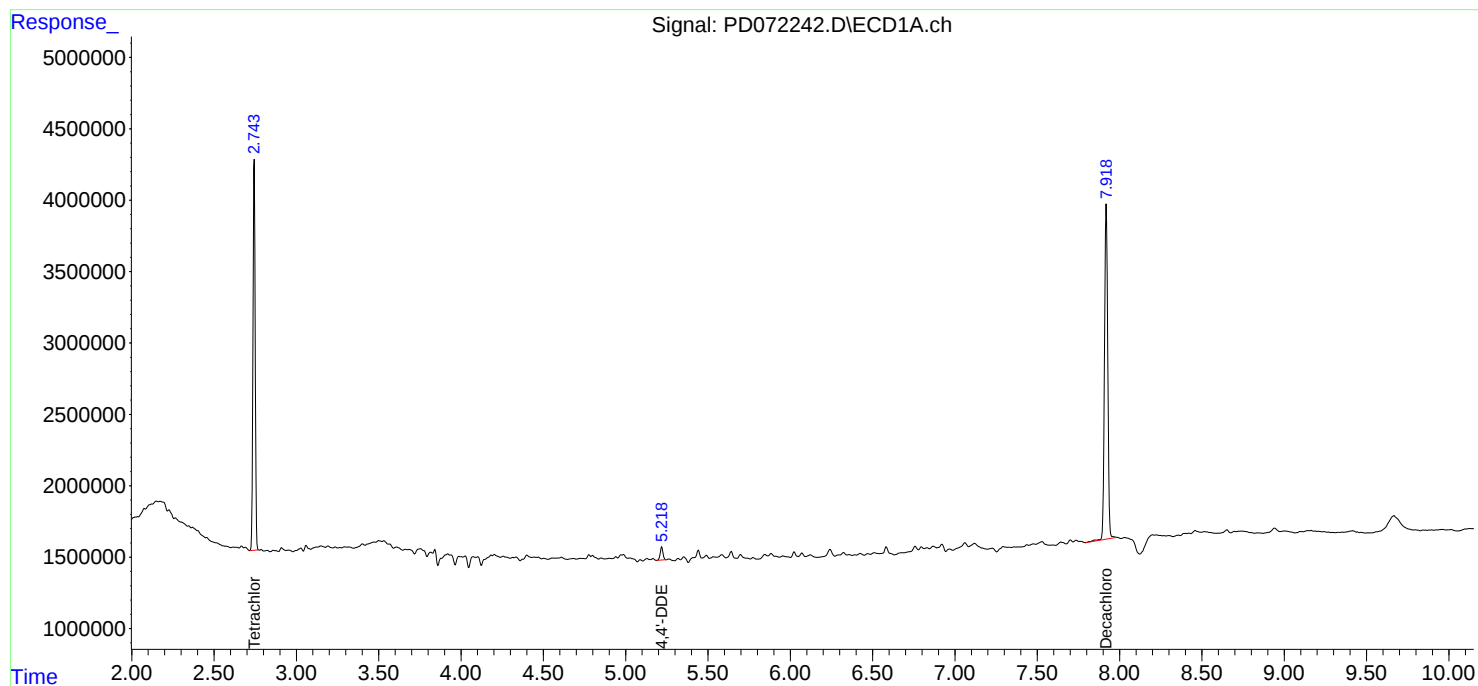


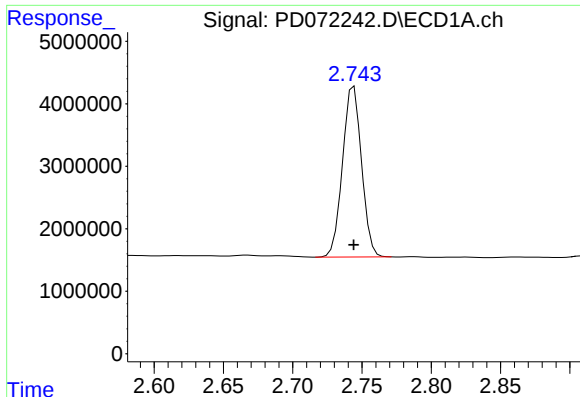

#1 Tetrachloro-m-xylene


R.T.: 2.744 min
Delta R.T.: 0.000 min
Response: 25934707
Conc: 10.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
AU-5-100422

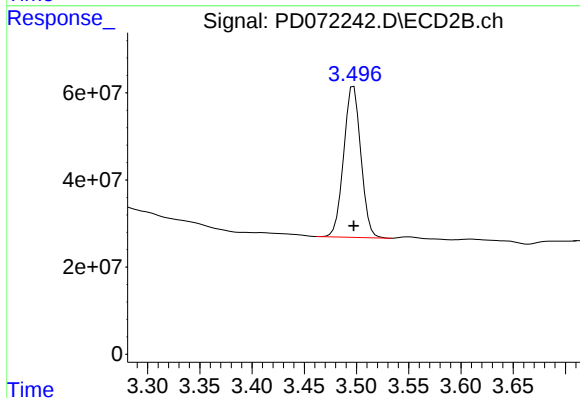


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 396451340
Conc: 10.94 ng/ml

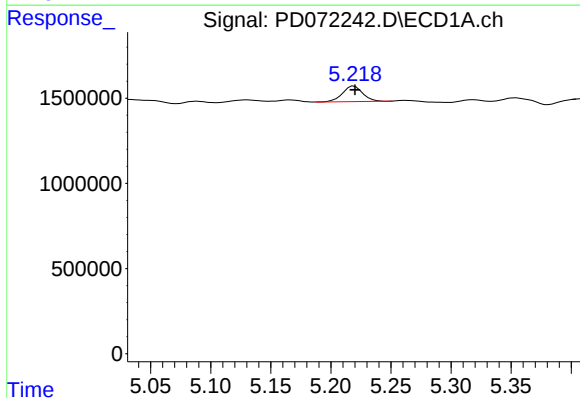


#12 4,4'-DDE

R.T.: 5.219 min
Delta R.T.: 0.000 min
Response: 1057343
Conc: 0.35 ng/ml

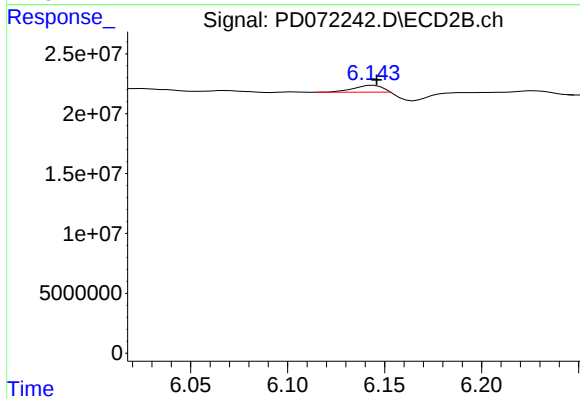

#12 4,4'-DDE


R.T.: 6.143 min
Delta R.T.: -0.003 min
Response: 5807720
Conc: 0.33 ng/ml m

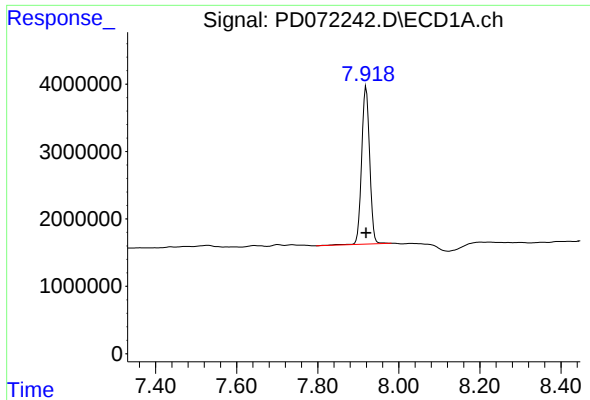

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: 0.000 min
Response: 32156773
Conc: 12.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
AU-5-100422

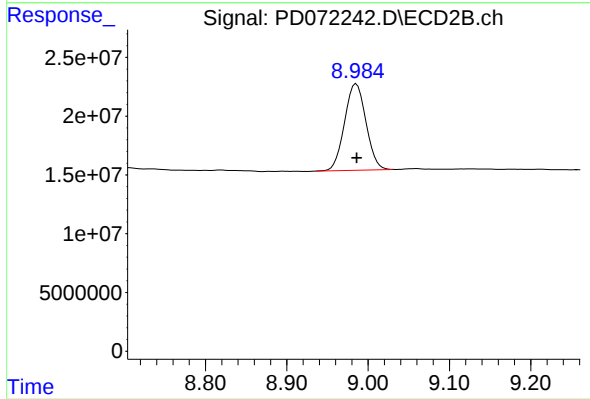

#28 Decachlorobiphenyl

R.T.: 8.985 min
Delta R.T.: 0.000 min
Response: 134442762
Conc: 13.38 ng/ml