

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100622\
 Data File : PD072259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2022 19:08
 Operator : AR\AJ
 Sample : N5014-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-09-2.0-3.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 00:40:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 15:15:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.744	3.498	48790251	699.2E6	19.442	19.288
28)	SA Decachlor...	7.919	8.986	43478279	203.8E6	17.056	20.288
Target Compounds							
12)	B 4,4'-DDE	5.218	6.146	2020736	16340971	0.664m	0.919 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100622\
Data File : PD072259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2022 19:08
Operator : AR\AJ
Sample : N5014-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SB-09-2.0-3.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 00:40:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 15:15:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

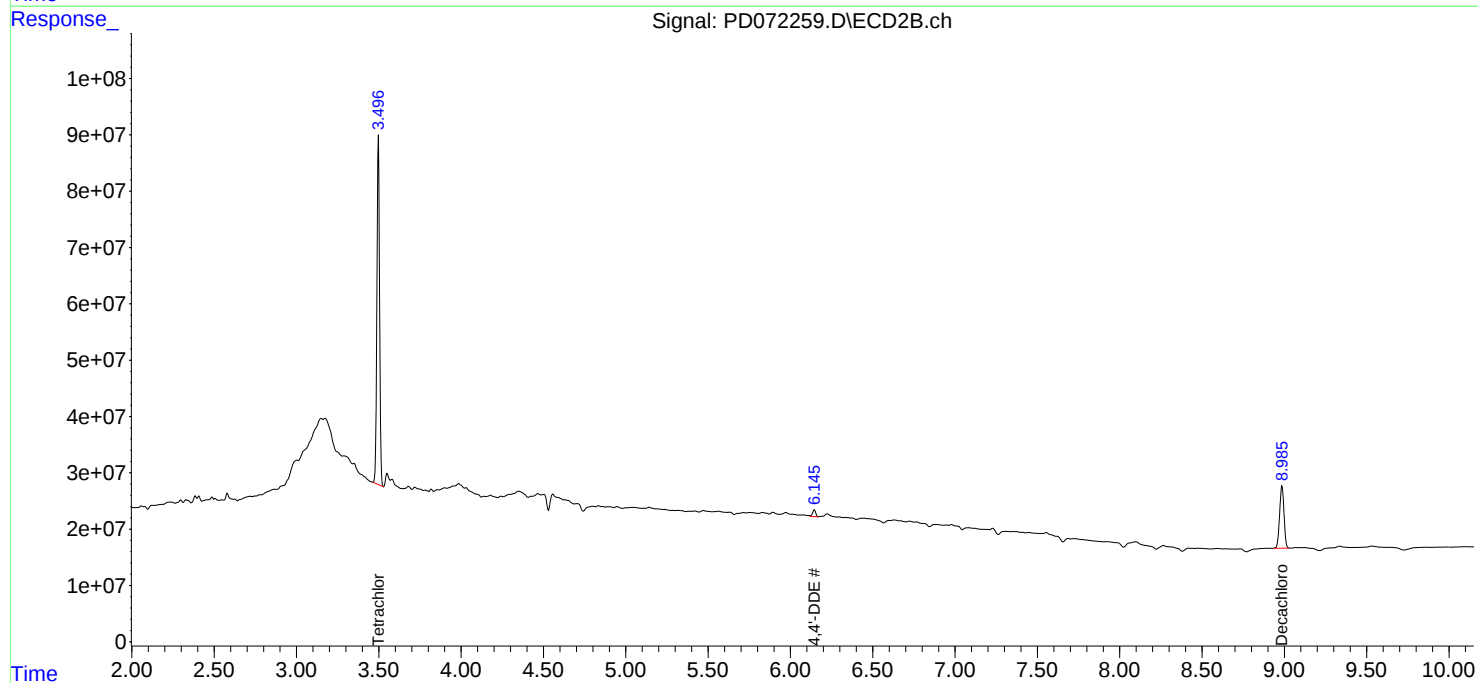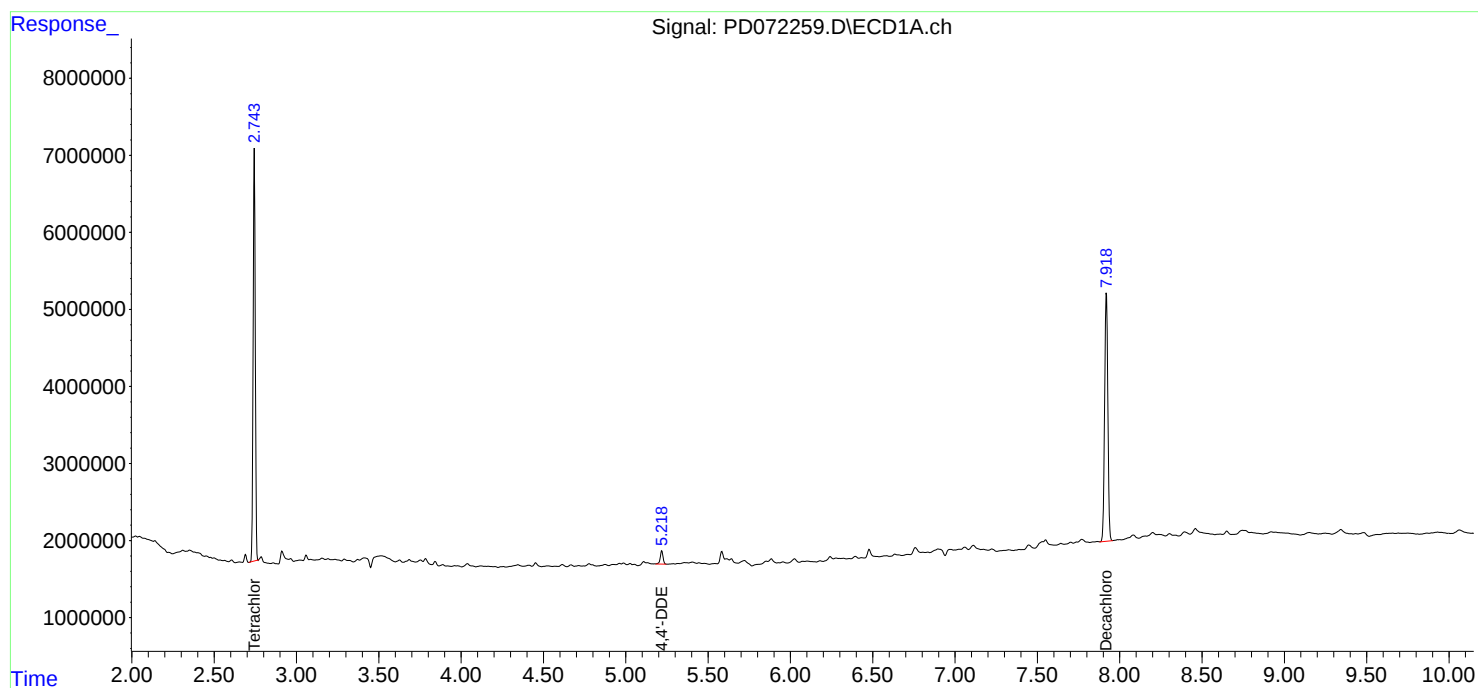


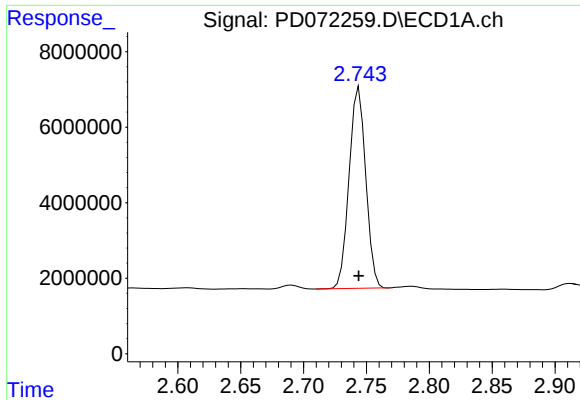

#1 Tetrachloro-m-xylene


R.T.: 2.744 min
Delta R.T.: 0.000 min
Response: 48790251
Conc: 19.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-09-2.0-3.0

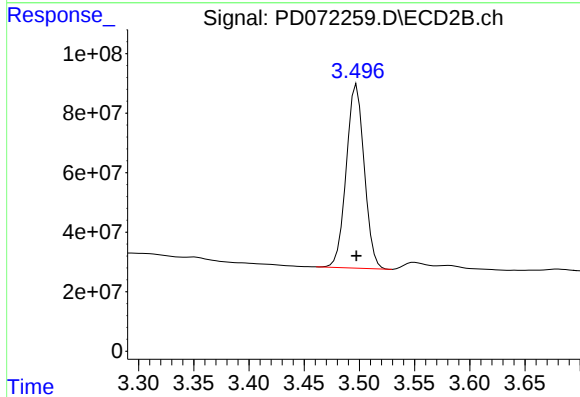


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 699189360
Conc: 19.29 ng/ml

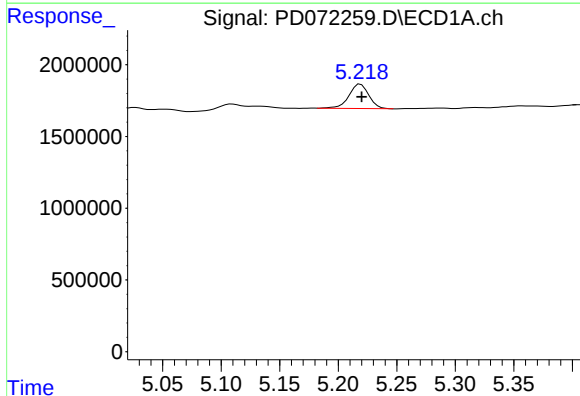


#12 4,4'-DDE

R.T.: 5.218 min
Delta R.T.: -0.003 min
Response: 2020736
Conc: 0.66 ng/ml m

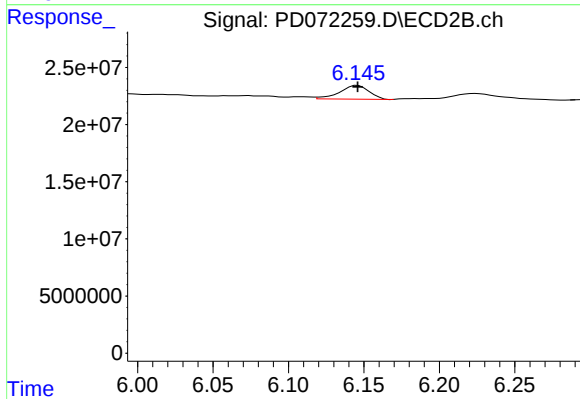

#12 4,4'-DDE


R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 16340971
Conc: 0.92 ng/ml

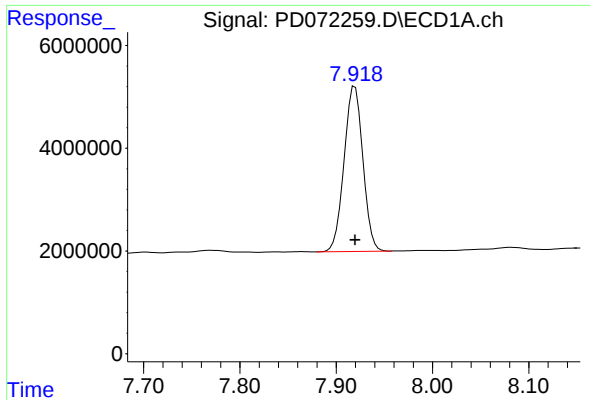

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: 0.000 min
Response: 43478279
Conc: 17.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-09-2.0-3.0

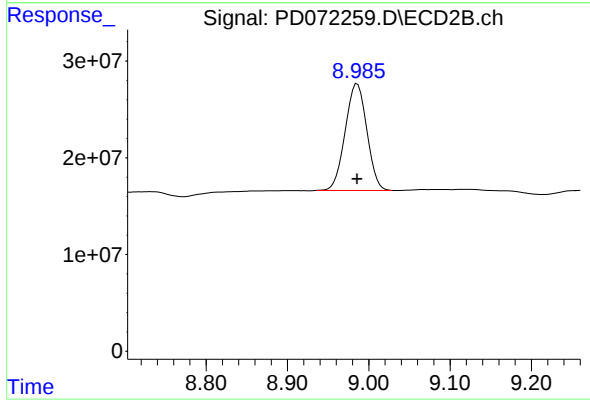

#28 Decachlorobiphenyl

R.T.: 8.986 min
Delta R.T.: 0.000 min
Response: 203833483
Conc: 20.29 ng/ml