

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100622\
 Data File : PD072263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2022 20:01
 Operator : AR\AJ
 Sample : N5014-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-01-0-2.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 00:42:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 15:15:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.745	3.498	46068208	678.8E6	18.357	18.724
28)	SA Decachlor...	7.917	8.985	31449399	143.5E6	12.337m	14.282
Target Compounds							
12)	B 4,4'-DDE	5.220	6.146	37269846	234.6E6	12.246	13.190
17)	MA 4,4'-DDT	6.030	6.979	6043721	41969778	2.306	2.975m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100622\
Data File : PD072263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2022 20:01
Operator : AR\AJ
Sample : N5014-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SB-01-0-2.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 00:42:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 15:15:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

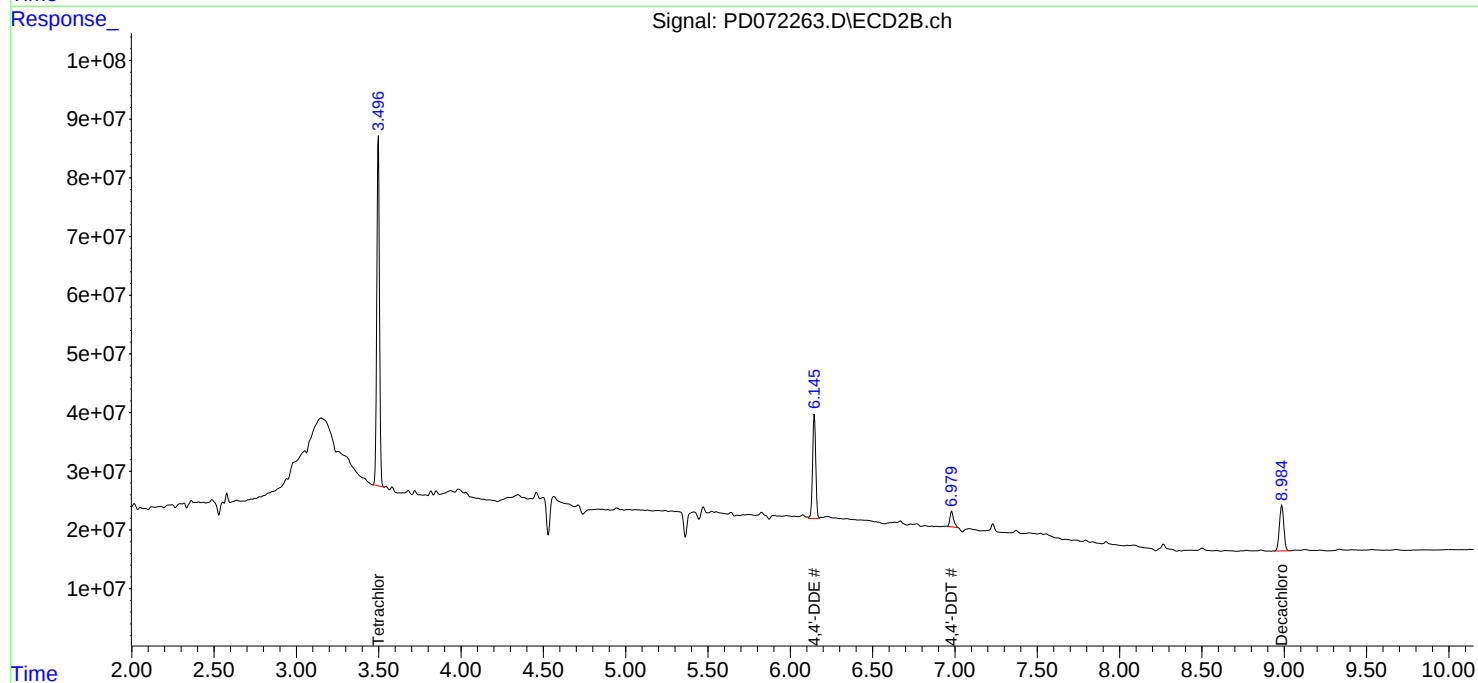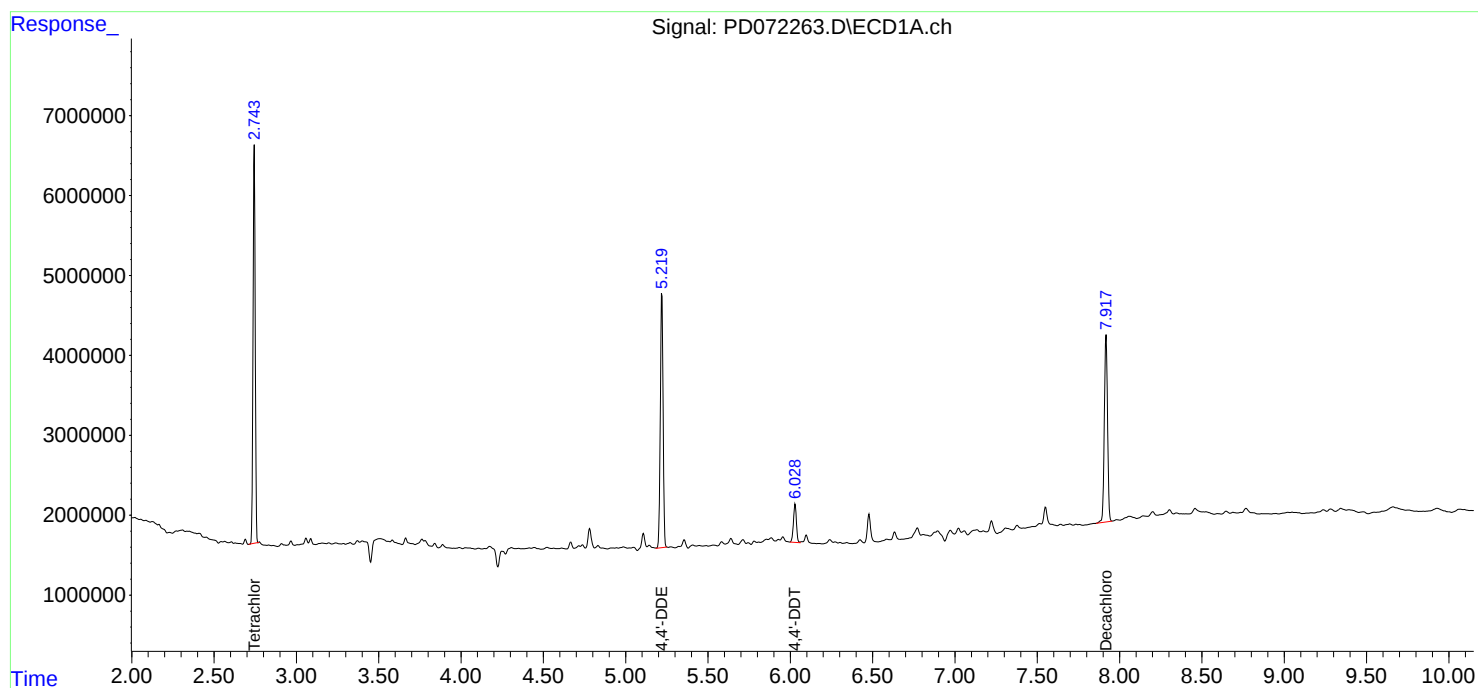


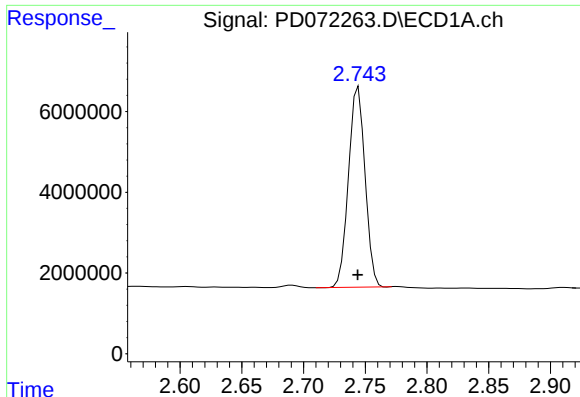

#1 Tetrachloro-m-xylene


R.T.: 2.745 min
Delta R.T.: 0.000 min
Response: 46068208
Conc: 18.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-01-0-2.0

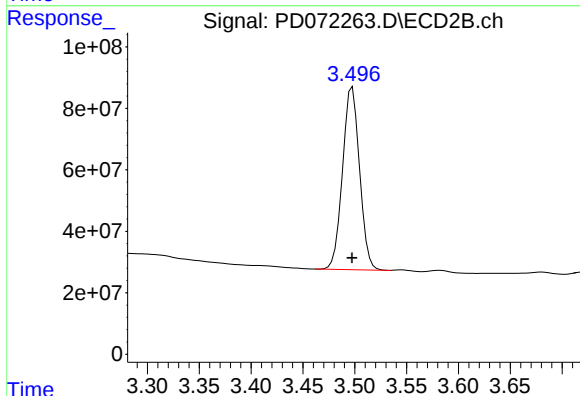


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 678755856
Conc: 18.72 ng/ml

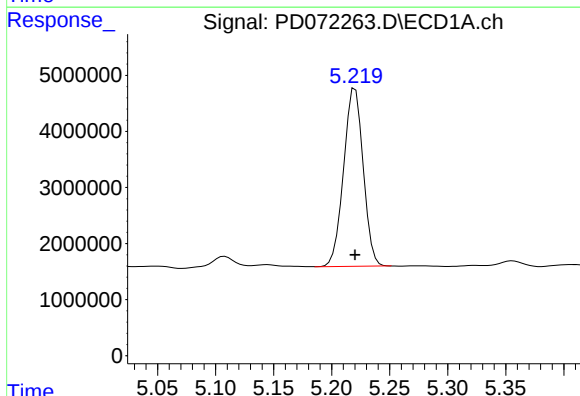


#12 4,4'-DDE

R.T.: 5.220 min
Delta R.T.: 0.000 min
Response: 37269846
Conc: 12.25 ng/ml

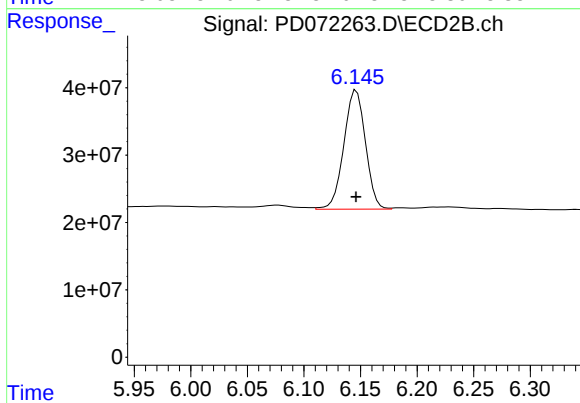

#12 4,4'-DDE


R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 234625839
Conc: 13.19 ng/ml

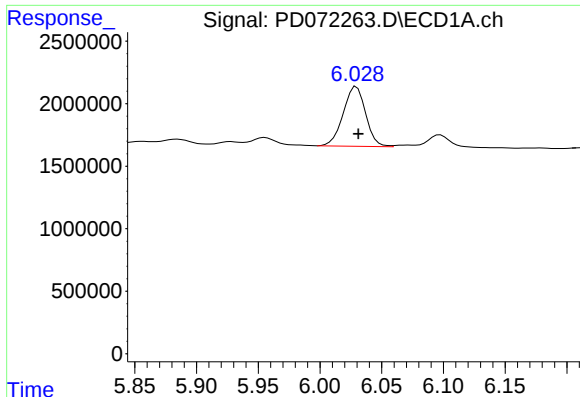

#17 4,4'-DDT


R.T.: 6.030 min
Delta R.T.: -0.002 min
Response: 6043721
Conc: 2.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-01-0-2.0

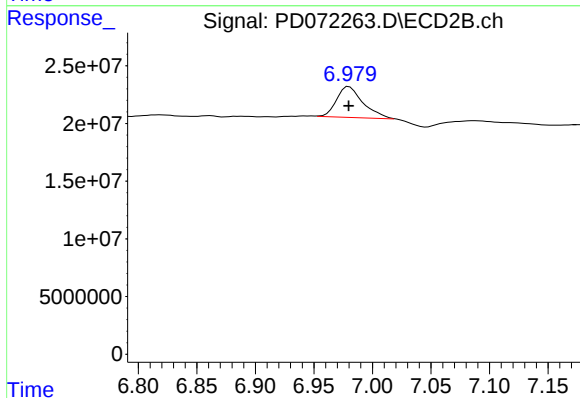


#17 4,4'-DDT

R.T.: 6.979 min
Delta R.T.: -0.001 min
Response: 41969778
Conc: 2.97 ng/ml m

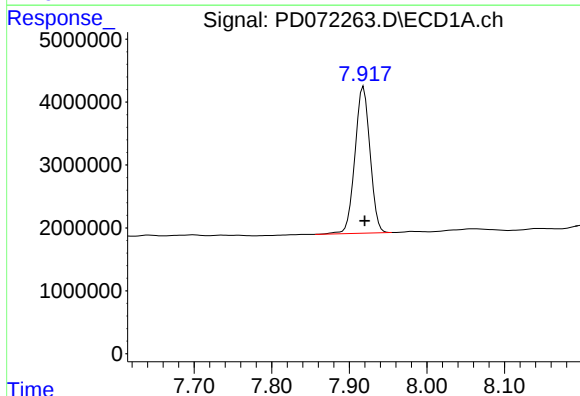

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: -0.003 min
Response: 31449399
Conc: 12.34 ng/ml m

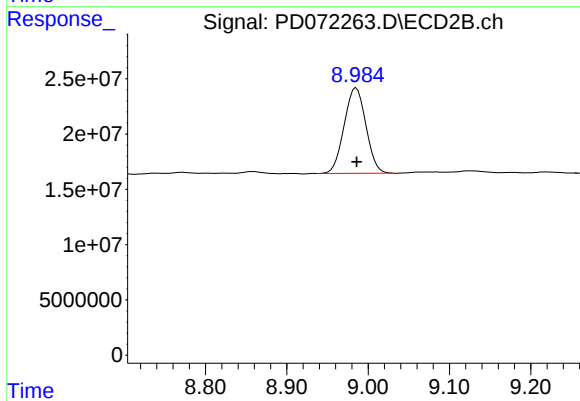

#28 Decachlorobiphenyl

R.T.: 8.985 min
Delta R.T.: 0.000 min
Response: 143489756
Conc: 14.28 ng/ml