

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100622\
 Data File : PD072264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2022 20:15
 Operator : AR\AJ
 Sample : N5014-14
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-02-0-2.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 00:42:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 15:15:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.744	3.497	52362611	763.3E6	20.865	21.056
28)	SA Decachlor...	7.918	8.984	46301161	212.4E6	18.163	21.144
Target Compounds							
12)	B 4,4'-DDE	5.220	6.146	16085758	105.0E6	5.286	5.904
17)	MA 4,4'-DDT	6.029	6.978	4844499	31365925	1.848	2.223m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100622\
Data File : PD072264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2022 20:15
Operator : AR\AJ
Sample : N5014-14
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SB-02-0-2.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 00:42:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 15:15:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

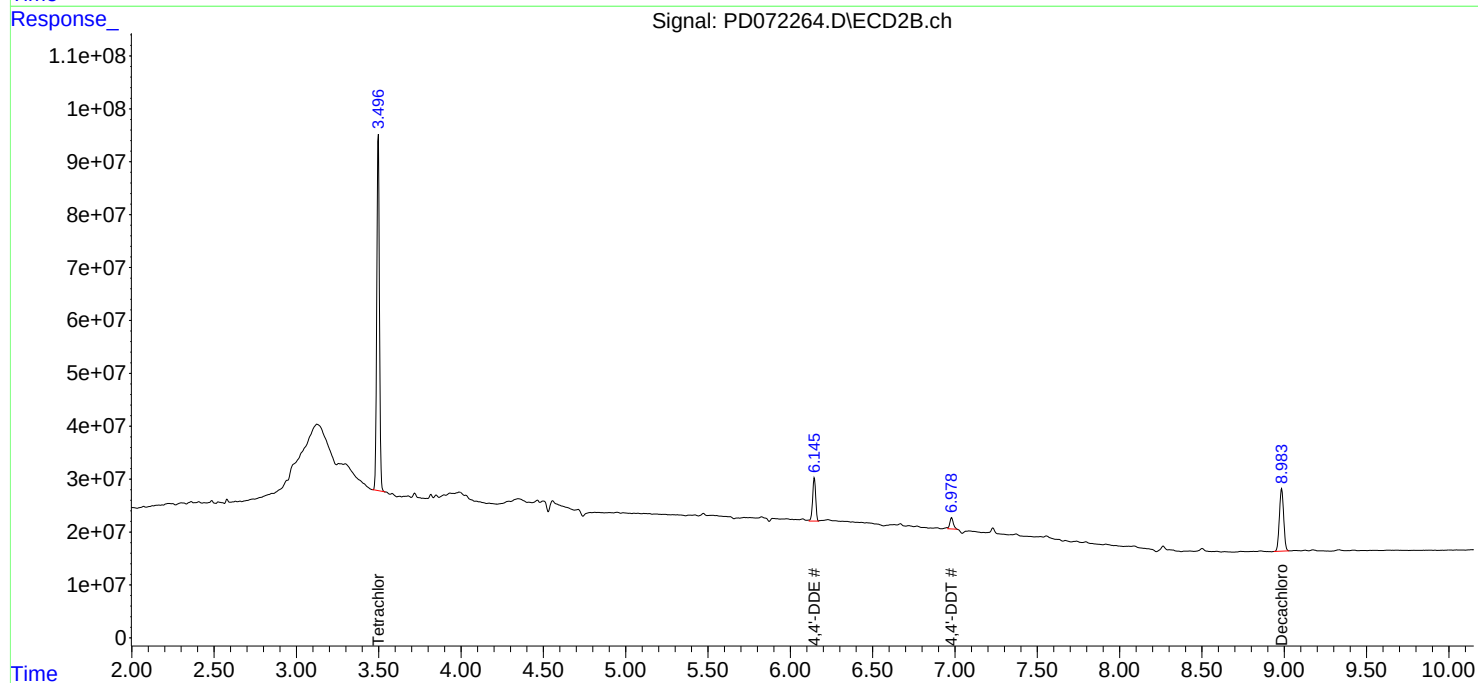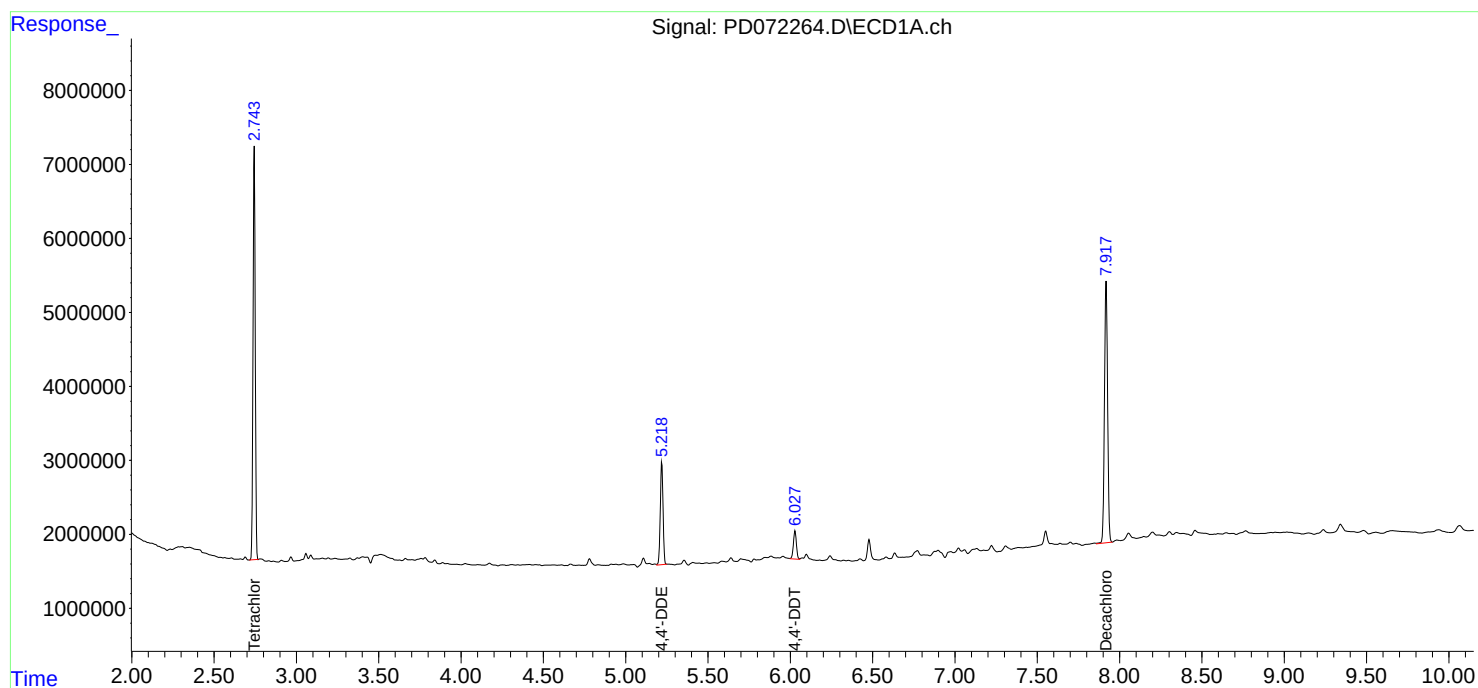


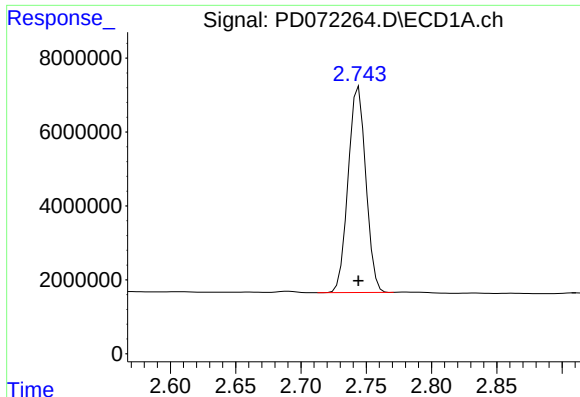

#1 Tetrachloro-m-xylene


R.T.: 2.744 min
Delta R.T.: 0.000 min
Response: 52362611
Conc: 20.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-02-0-2.0

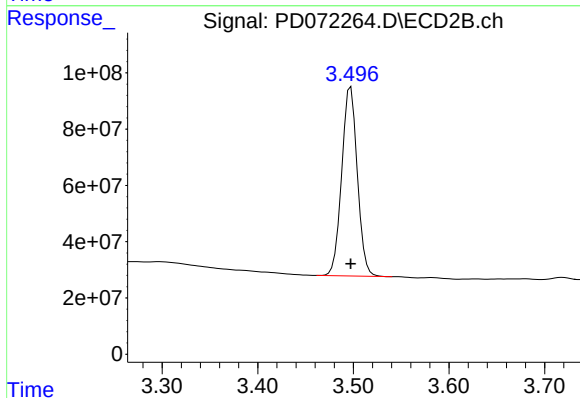


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 763296436
Conc: 21.06 ng/ml

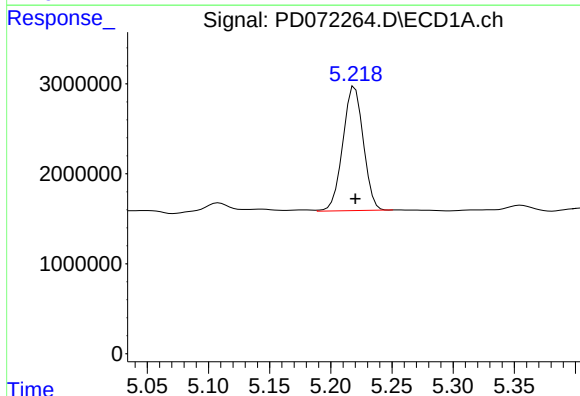


#12 4,4'-DDE

R.T.: 5.220 min
Delta R.T.: 0.000 min
Response: 16085758
Conc: 5.29 ng/ml

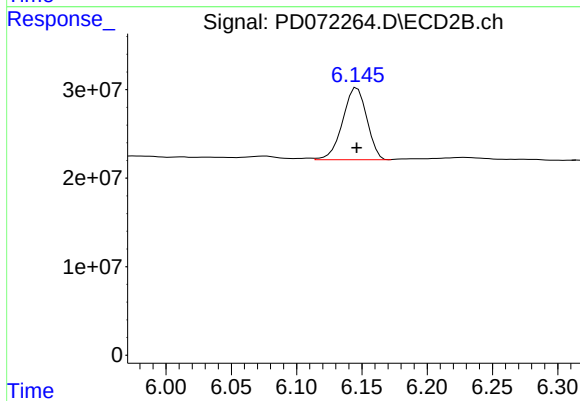

#12 4,4'-DDE


R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 105012438
Conc: 5.90 ng/ml

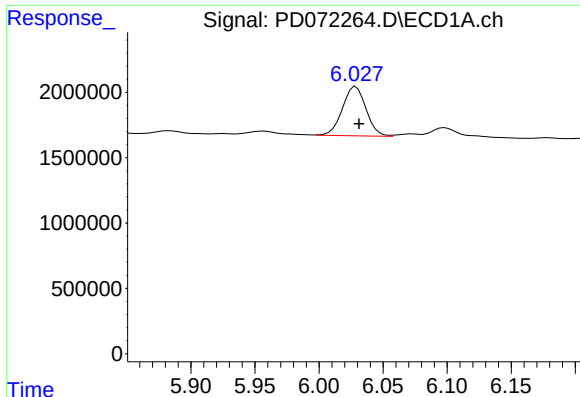

#17 4,4'-DDT


R.T.: 6.029 min
Delta R.T.: -0.002 min
Response: 4844499
Conc: 1.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-02-0-2.0

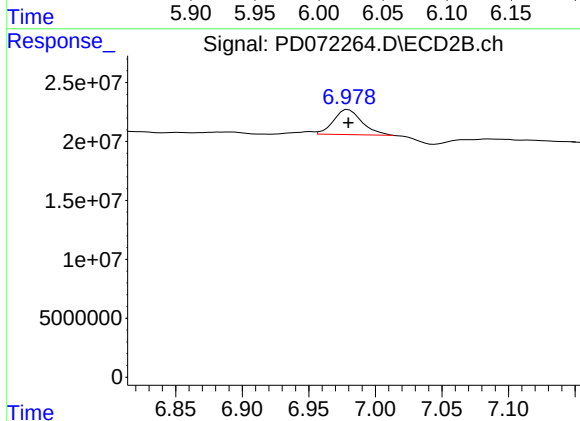


#17 4,4'-DDT

R.T.: 6.978 min
Delta R.T.: -0.002 min
Response: 31365925
Conc: 2.22 ng/ml m

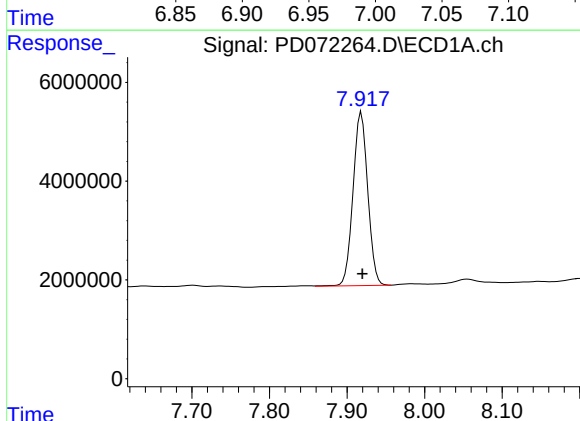

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: -0.001 min
Response: 46301161
Conc: 18.16 ng/ml

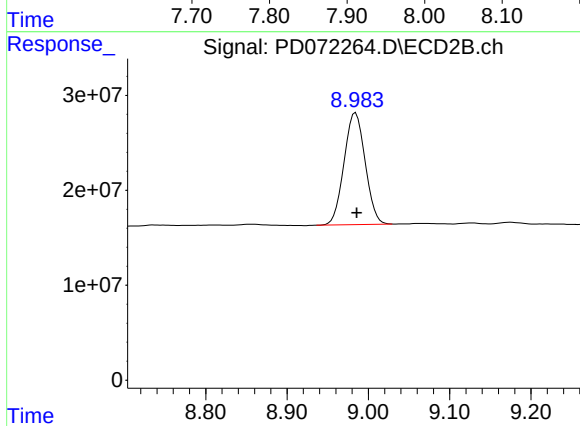

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: -0.001 min
Response: 212438742
Conc: 21.14 ng/ml