

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100623\
 Data File : PD078734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2023 12:33
 Operator : AR\AJ
 Sample : 04469-08 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYM2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/06/2023
 Supervised By : Ankita Jodhani 10/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 04:53:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 11 14:09:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.757	36245748	25515337	14.228	16.126
2) SA Decachlor...	9.075	7.892	57152765	31414053	18.319	18.212
Target Compounds						
8) B Heptachlo...	5.684	4.707	6174961	2924105	1.603	1.313
12) B 4,4'-DDE	6.197	5.209	7821670	7440213	2.208	3.665 #
17) MA 4,4'-DDT	7.002	6.008	8833115	6210396	3.248m	4.029m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100623\
Data File : PD078734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2023 12:33
Operator : AR\AJ
Sample : 04469-08 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 04:53:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Mon Sep 11 14:09:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

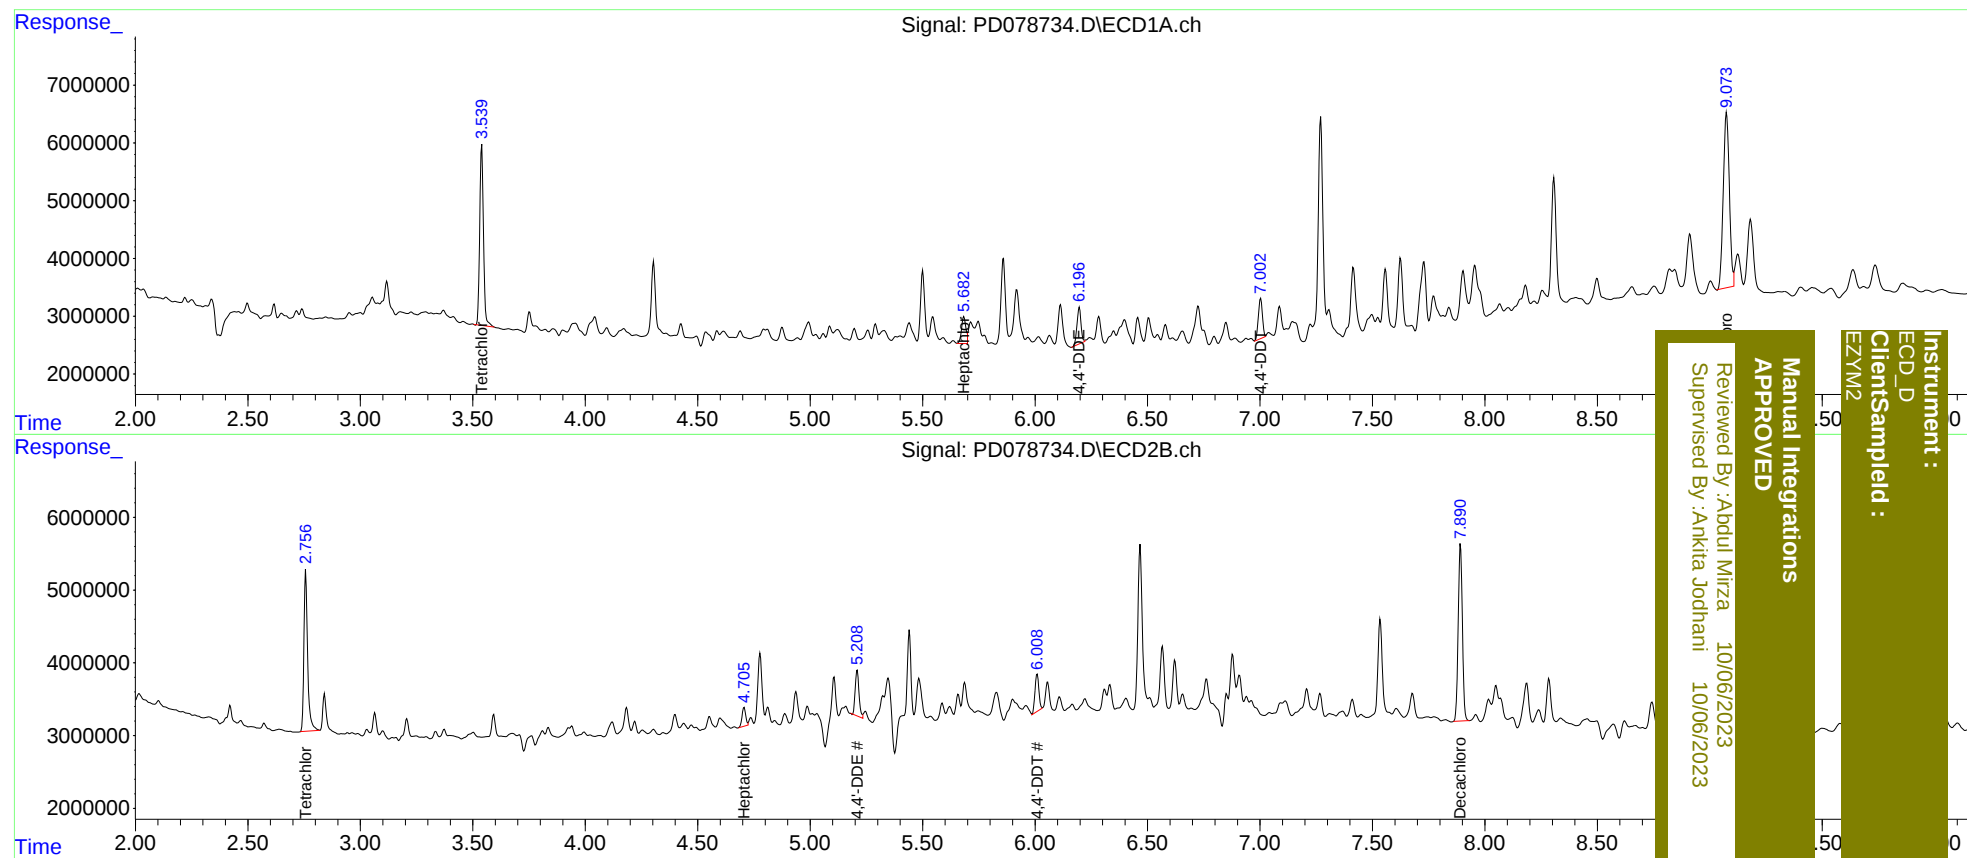

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/06/2023
Supervised By: Ankita Jodhani 10/06/2023

Instrument :
ECD_D
ClientSampled :
EZYM2