

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100722\
 Data File : PD072275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2022 12:31
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 23:40:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 15:15:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.751	3.495	146.7E6	1559.2E6	58.437	43.011 #
28)	SA Decachlor...	7.928	8.986	116.5E6	524.3E6	45.708	52.186
Target Compounds							
23)	Chlordane-1	3.757	4.652	46253188	508.7E6	458.880	435.824
24)	Chlordane-2	4.338	5.183	48664253	413.0E6	422.383	475.486
25)	Chlordane-3	4.973	5.894	149.2E6	1168.9E6	470.856	463.229
26)	Chlordane-4	5.036	5.971	144.6E6	1358.6E6	465.161	475.240
27)	Chlordane-5	5.936	6.831	47361972	267.2E6	457.419	498.428



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100722\
Data File : PD072275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2022 12:31
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 23:40:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 15:15:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

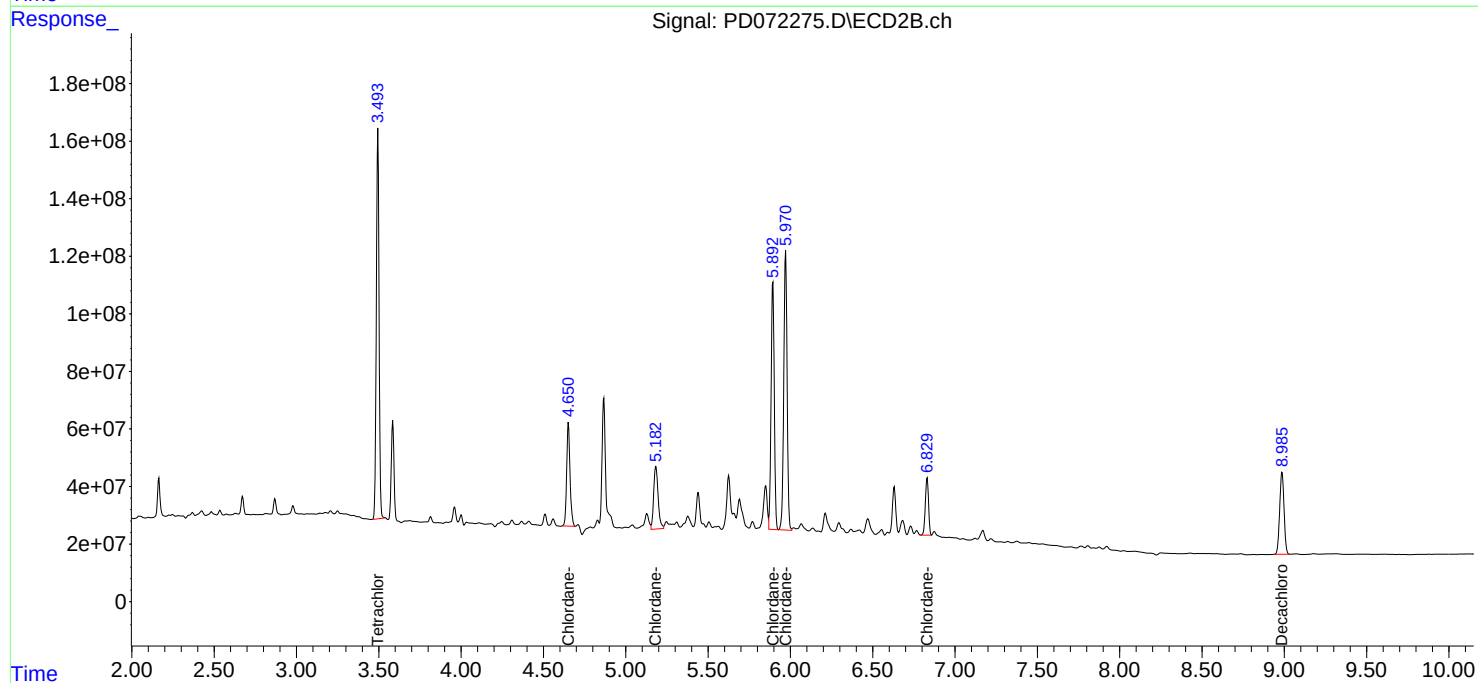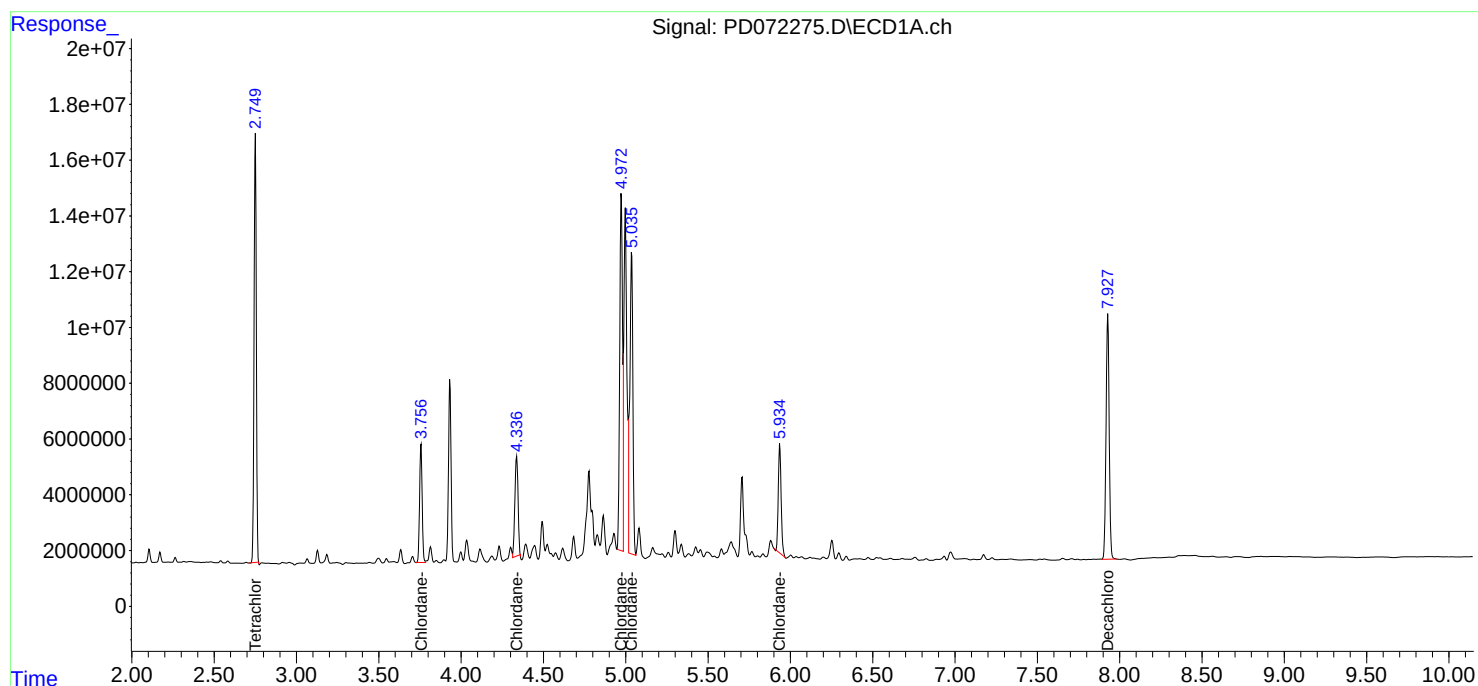


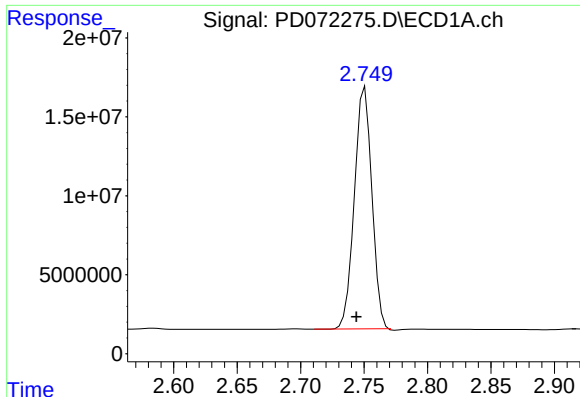

#1 Tetrachloro-m-xylene


R.T.: 2.751 min
Delta R.T.: 0.007 min
Response: 146652257
Conc: 58.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

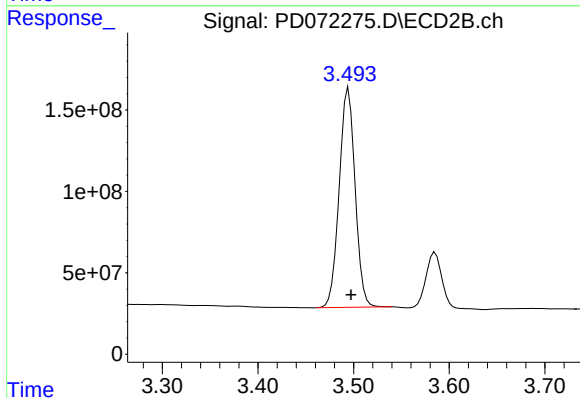


#1 Tetrachloro-m-xylene

R.T.: 3.495 min
Delta R.T.: -0.003 min
Response: 1559183407
Conc: 43.01 ng/ml

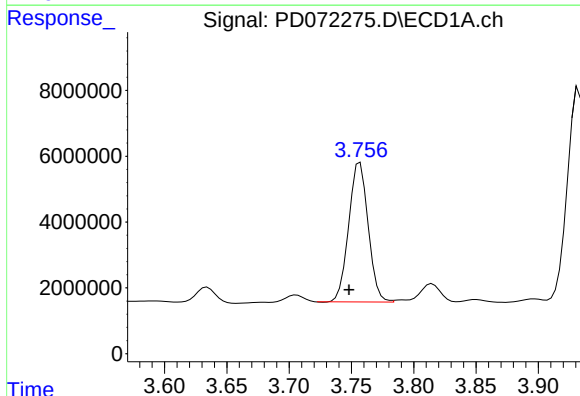


#23 Chlordane-1

R.T.: 3.757 min
Delta R.T.: 0.009 min
Response: 46253188
Conc: 458.88 ng/ml

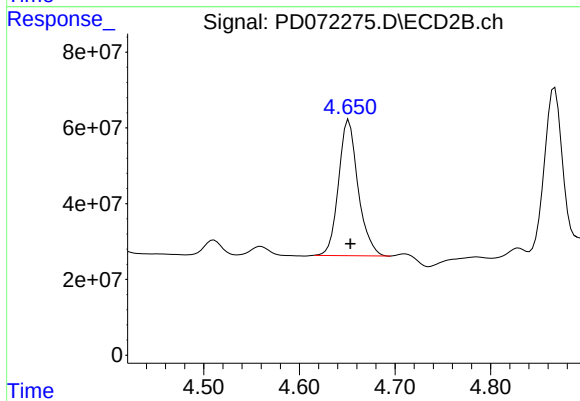

#23 Chlordane-1


R.T.: 4.652 min
Delta R.T.: -0.001 min
Response: 508725026
Conc: 435.82 ng/ml

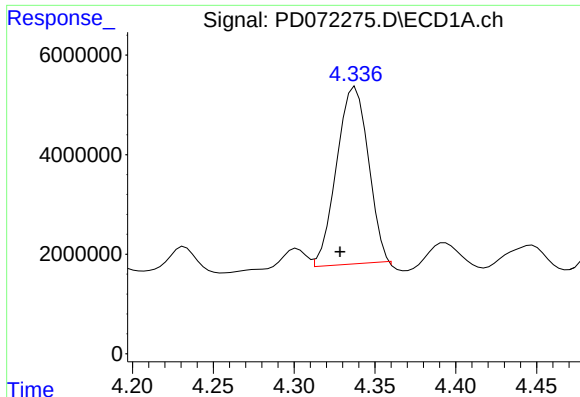

#24 Chlordane-2


R.T.: 4.338 min
Delta R.T.: 0.010 min
Response: 48664253
Conc: 422.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

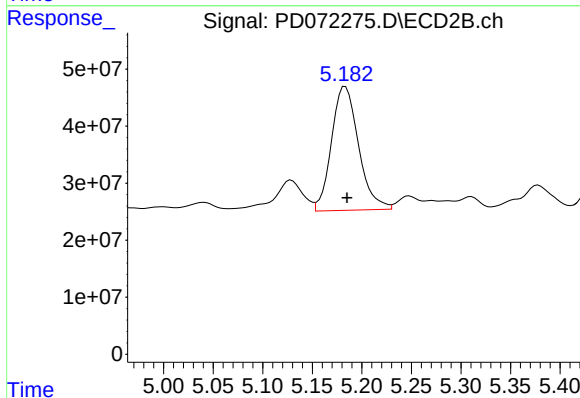


#24 Chlordane-2

R.T.: 5.183 min
Delta R.T.: -0.002 min
Response: 413032701
Conc: 475.49 ng/ml

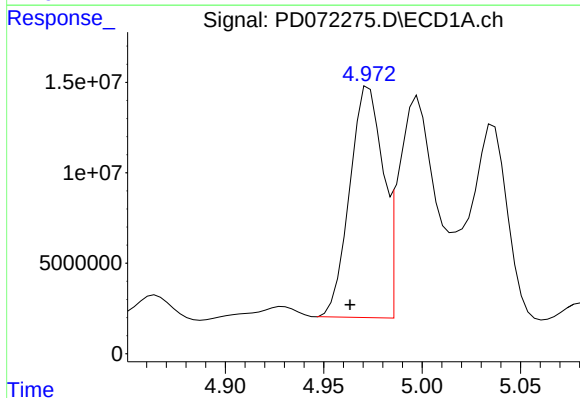


#25 Chlordane-3

R.T.: 4.973 min
Delta R.T.: 0.010 min
Response: 149219552
Conc: 470.86 ng/ml

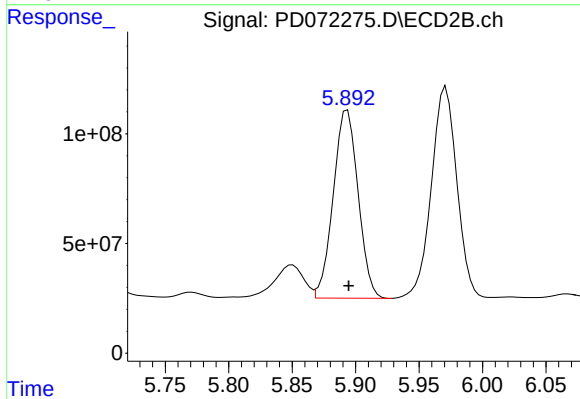

#25 Chlordane-3


R.T.: 5.894 min
Delta R.T.: 0.000 min
Response: 1168947449
Conc: 463.23 ng/ml

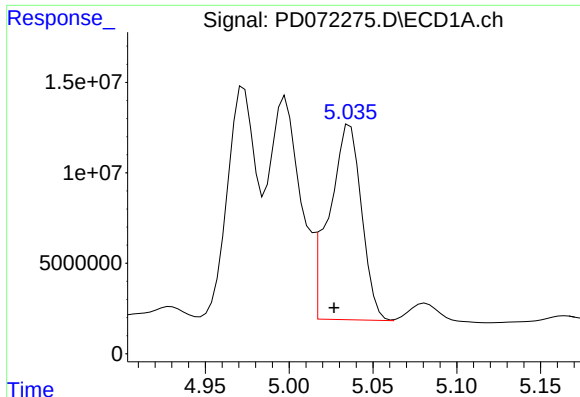

#26 Chlordane-4


R.T.: 5.036 min
Delta R.T.: 0.009 min
Response: 144558280
Conc: 465.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

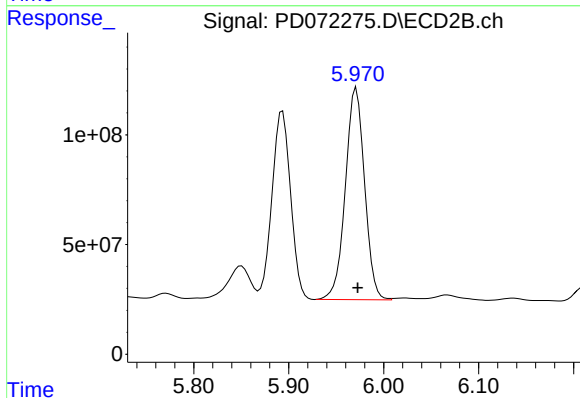


#26 Chlordane-4

R.T.: 5.971 min
Delta R.T.: -0.001 min
Response: 1358569873
Conc: 475.24 ng/ml

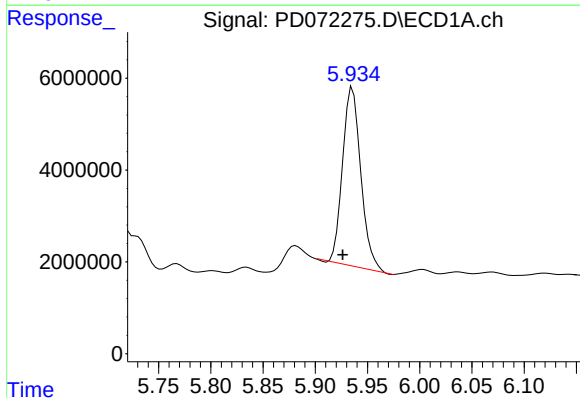


#27 Chlordane-5

R.T.: 5.936 min
Delta R.T.: 0.009 min
Response: 47361972
Conc: 457.42 ng/ml

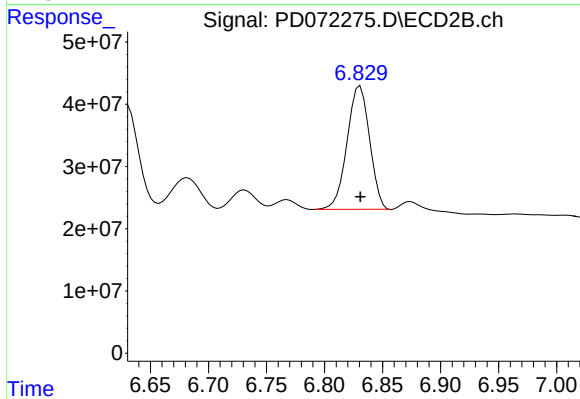

#27 Chlordane-5

R.T.: 6.831 min
Delta R.T.: 0.000 min
Response: 267249132
Conc: 498.43 ng/ml

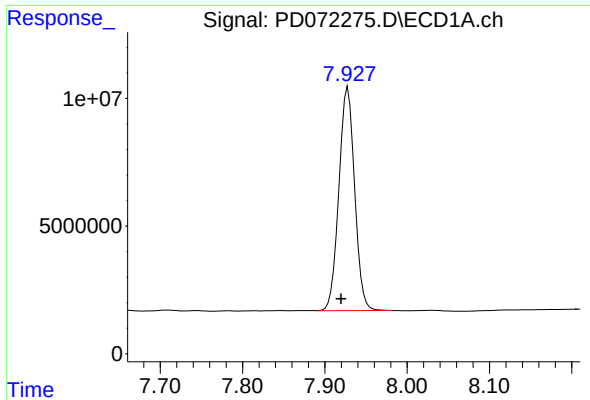

#28 Decachlorobiphenyl


R.T.: 7.928 min

Delta R.T.: 0.008 min

Response: 116518345

Conc: 45.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

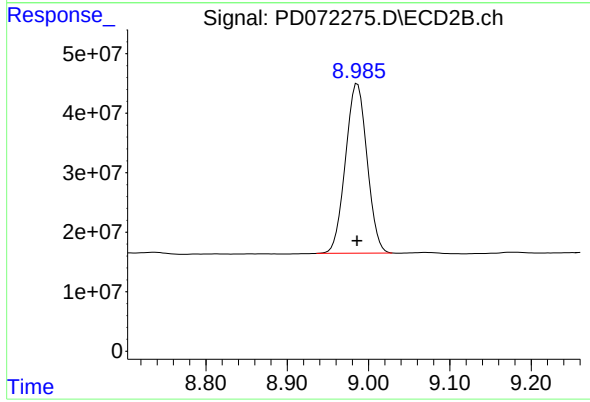

#28 Decachlorobiphenyl

R.T.: 8.986 min

Delta R.T.: 0.000 min

Response: 524310950

Conc: 52.19 ng/ml