

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100722\
 Data File : PD072280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2022 13:41
 Operator : AR\AJ
 Sample : N5047-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OR-3-100622

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/10/2022
 Supervised By :Ankita Jodhani 10/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 23:46:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 15:15:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.744	3.496	34940517	424.9E6	13.923	11.722m
28)	SA Decachlor...	7.918	8.985	28976006	139.1E6	11.367	13.846
Target Compounds							
11)	B alpha-Chl...	5.025	5.971	1014985	17765937	0.316m	0.990m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100722\
Data File : PD072280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2022 13:41
Operator : AR\AJ
Sample : N5047-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
OR-3-100622


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/10/2022
Supervised By : Ankita Jodhani 10/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 23:46:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 15:15:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

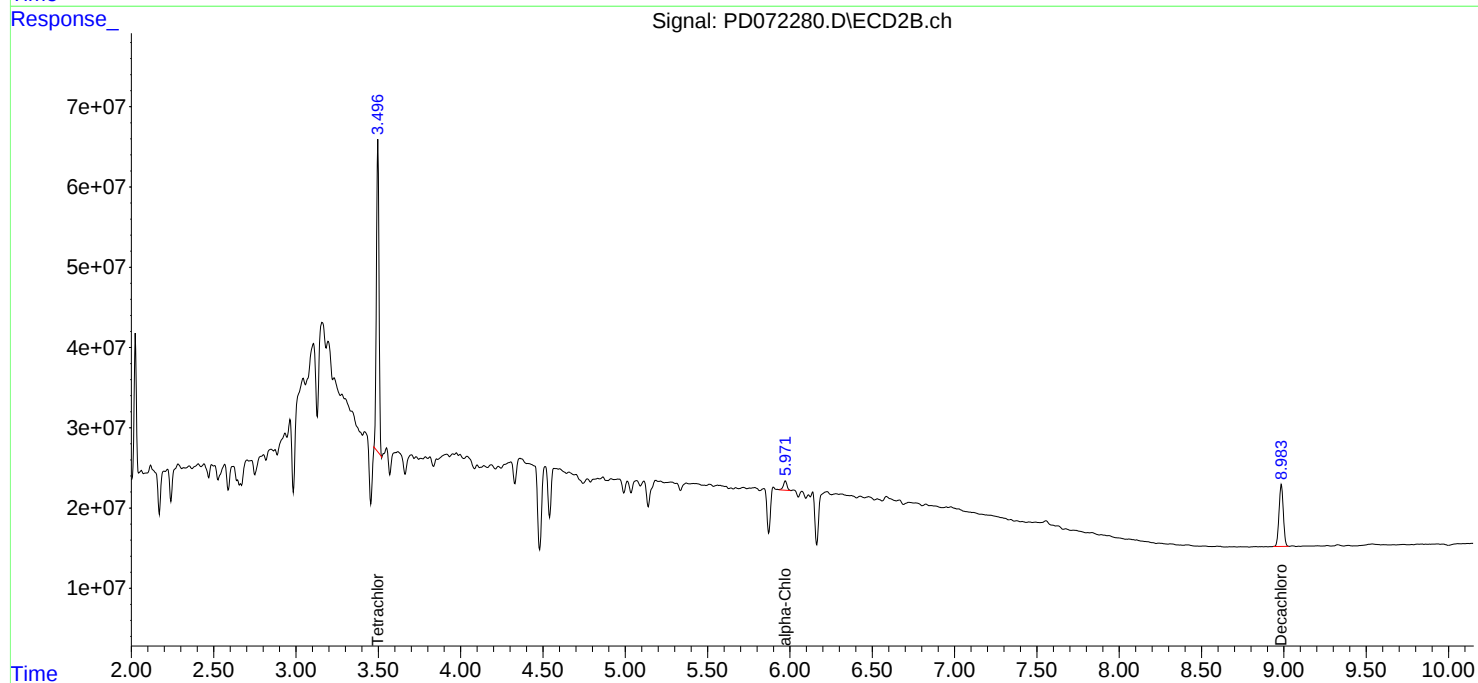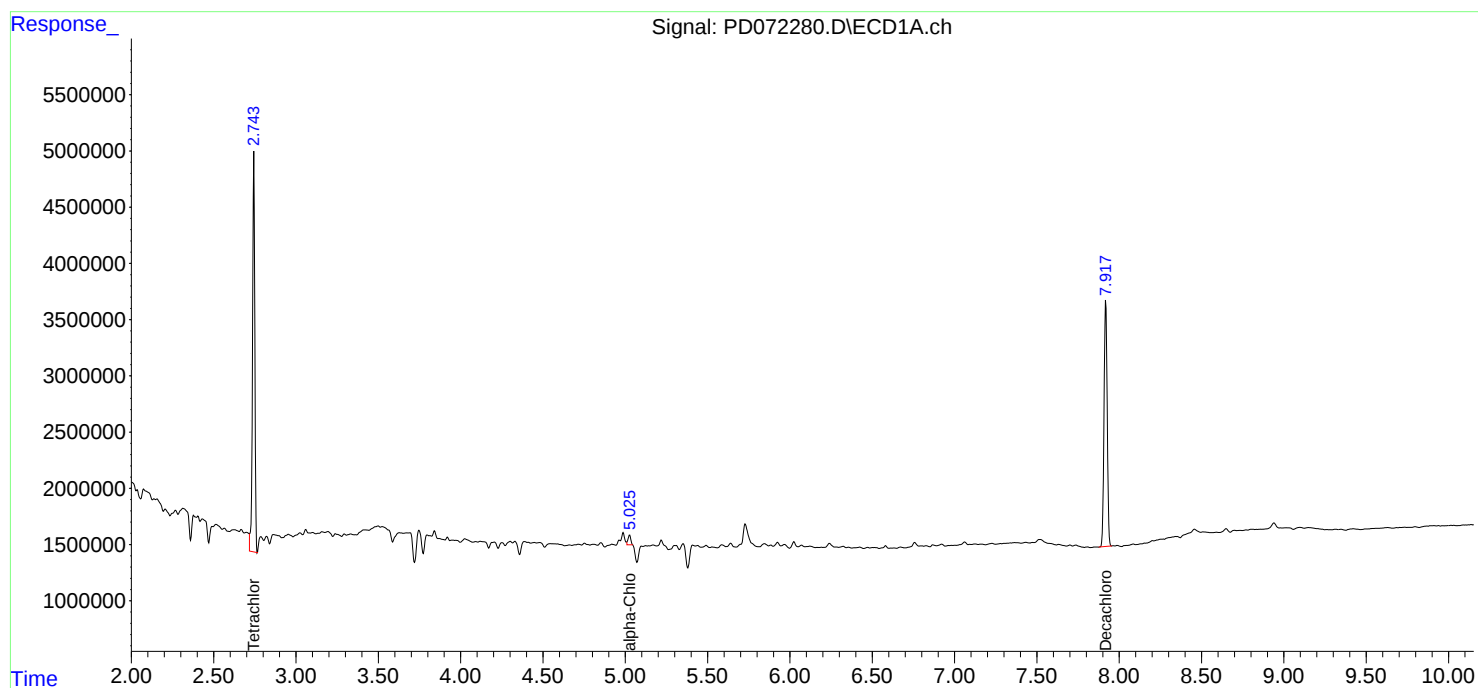

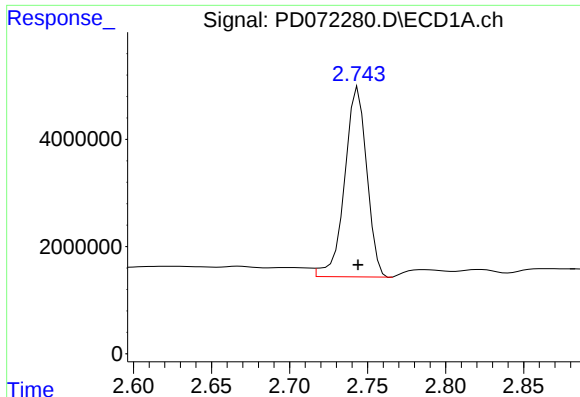


#1 Tetrachloro-m-xylene

R.T.: 2.744 min
Delta R.T.: 0.000 min
Response: 34940517
Conc: 13.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
OR-3-100622


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/10/2022
Supervised By :Ankita Jodhani 10/10/2022

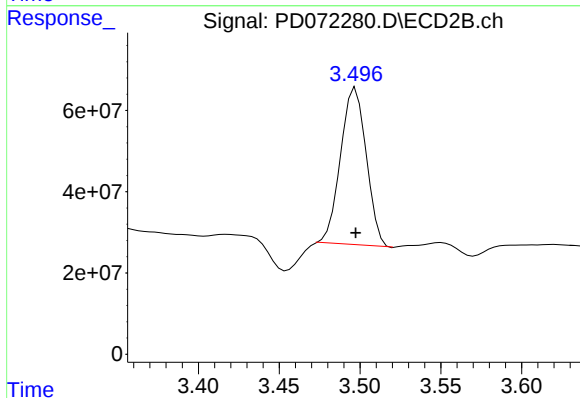


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: -0.001 min
Response: 424933031
Conc: 11.72 ng/ml m

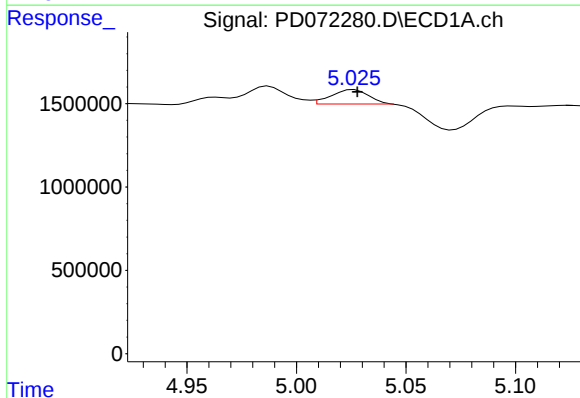


#11 alpha-Chlordane

R.T.: 5.025 min
Delta R.T.: -0.003 min
Response: 1014985
Conc: 0.32 ng/ml m

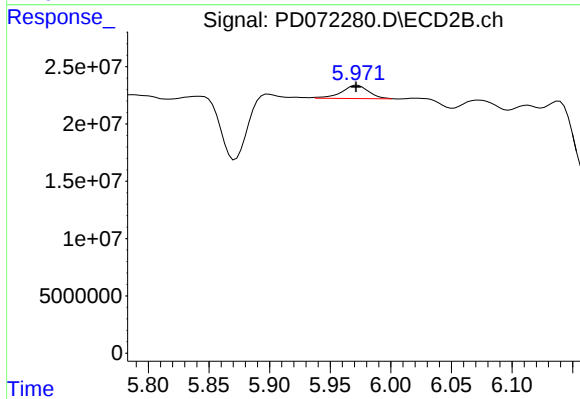

#11 alpha-Chlordane

R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 17765937
Conc: 0.99 ng/ml m

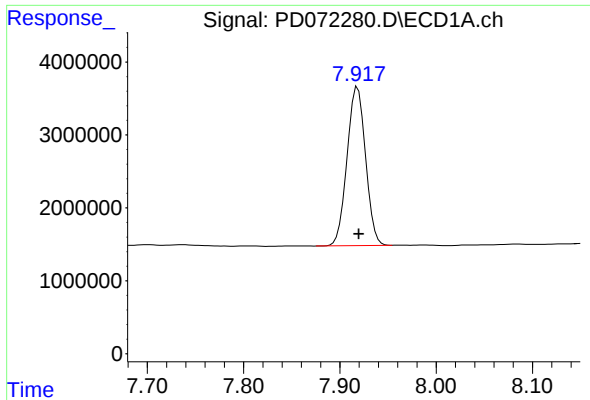


#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: -0.001 min
Response: 28976006
Conc: 11.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
OR-3-100622

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/10/2022
Supervised By :Ankita Jodhani 10/10/2022

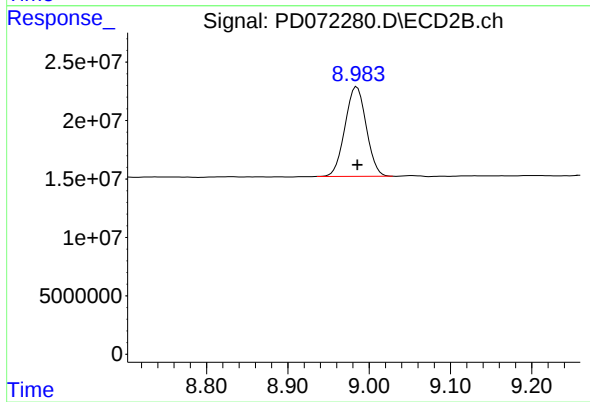

#28 Decachlorobiphenyl

R.T.: 8.985 min
Delta R.T.: 0.000 min
Response: 139115354
Conc: 13.85 ng/ml