

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100722\
 Data File : PD072302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2022 18:41
 Operator : AR\AJ
 Sample : N5018-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SASP2-T-3-(10-14)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 00:00:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 15:15:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.744	3.498	46980647	681.1E6	18.721	18.789
28)	SA Decachlor...	7.918	8.985	41521563	192.6E6	16.288	19.167

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100722\
Data File : PD072302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2022 18:41
Operator : AR\AJ
Sample : N5018-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SASP2-T-3-(10-14)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 00:00:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 15:15:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

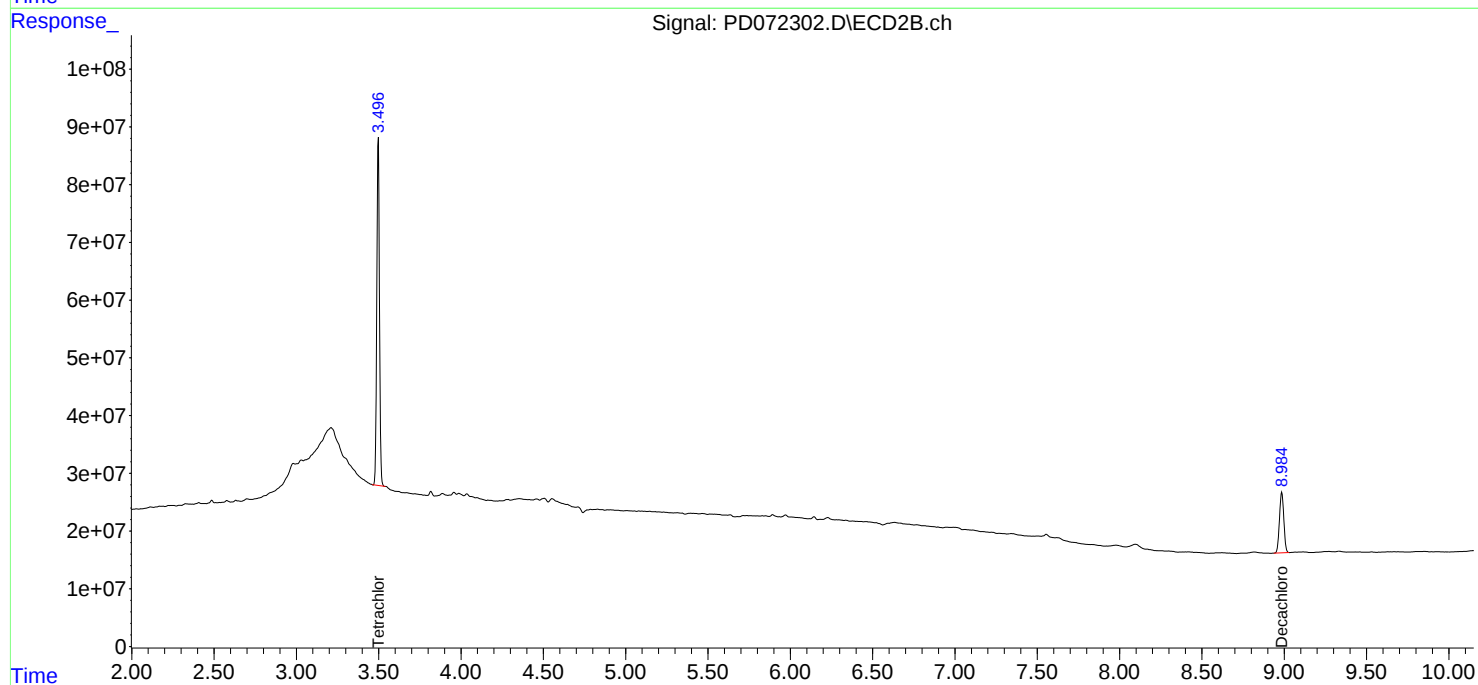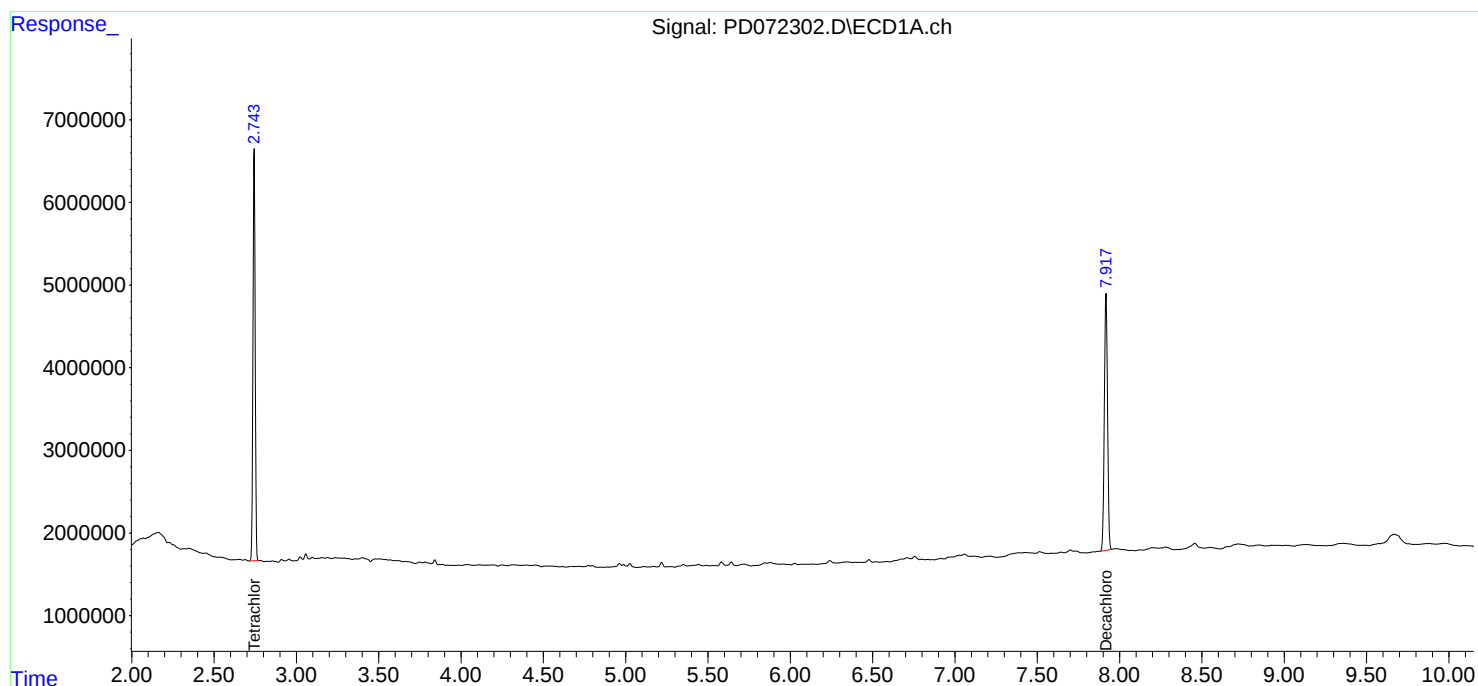


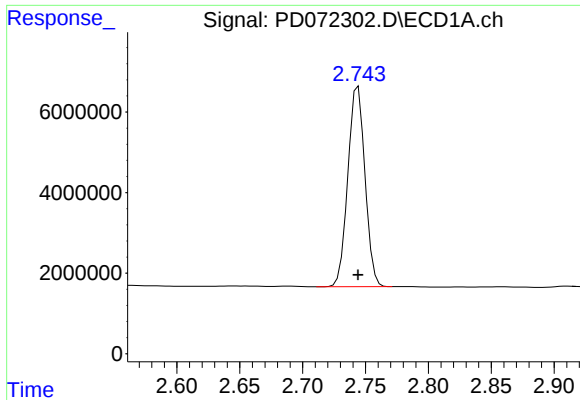

#1 Tetrachloro-m-xylene


R.T.: 2.744 min
Delta R.T.: 0.000 min
Response: 46980647
Conc: 18.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
SASP2-T-3-(10-14)

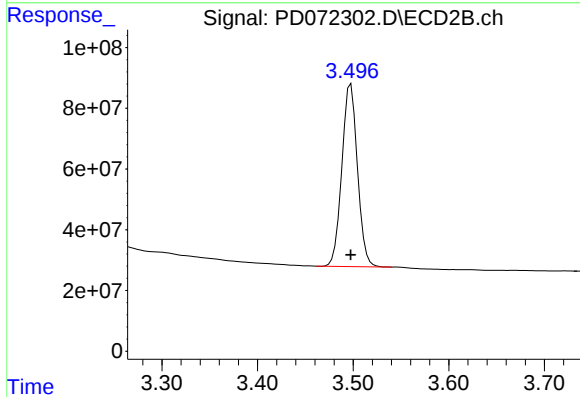


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 681116313
Conc: 18.79 ng/ml

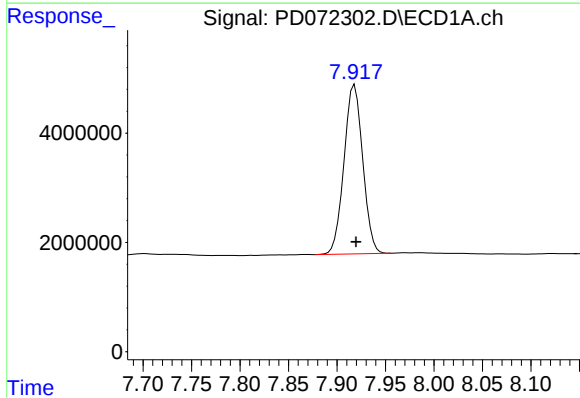

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: -0.002 min
Response: 41521563
Conc: 16.29 ng/ml

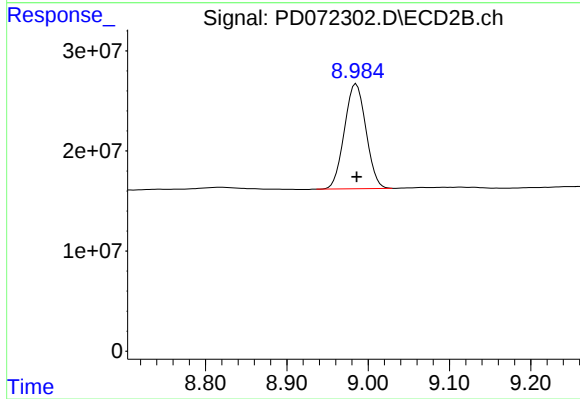

#28 Decachlorobiphenyl

R.T.: 8.985 min
Delta R.T.: 0.000 min
Response: 192576073
Conc: 19.17 ng/ml