

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100724\
 Data File : PD085921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2024 10:39
 Operator : AR\AJ
 Sample : P4221-15
 Misc : E3806(LOT#M06518)
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 FLORISIL-CHECK

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/08/2024
 Supervised By :Ankita Jodhani 10/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 01:25:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 08:04:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	2.873	12308743	44114817	10.759m	10.403
2)	SA Decachlor...	8.886	8.056	42660547	71200086	23.458	19.370
Target Compounds							
2)	A alpha-BHC	3.878	3.380	20523520	62588012	9.858m	9.919m
3)	MA gamma-BHC...	4.207	3.715	21576977	59253038	9.881	9.817
4)	MA Heptachlor	4.799	4.064	18223073	55300901	8.858	9.618m
9)	A Endosulfan I	5.936	5.227	18106651	49482823	9.956m	9.974m
13)	MA Dieldrin	6.210	5.495	37615249	107.0E6	18.773	19.302
14)	MA Endrin	6.435	5.772	30438494	86842647	19.160	18.139
16)	A 4,4'-DDD	6.569	5.911	26318882	75288845	21.104m	19.246m
17)	MA 4,4'-DDT	6.884	6.165	27919253	80357436	20.083m	18.981m
20)	A Methoxychlor	7.358	6.738	82739423	207.0E6	101.153	100.353

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100724\
Data File : PD085921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2024 10:39
Operator : AR\AJ
Sample : P4221-15
Misc : E3806(LOT#M06518)
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 01:25:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

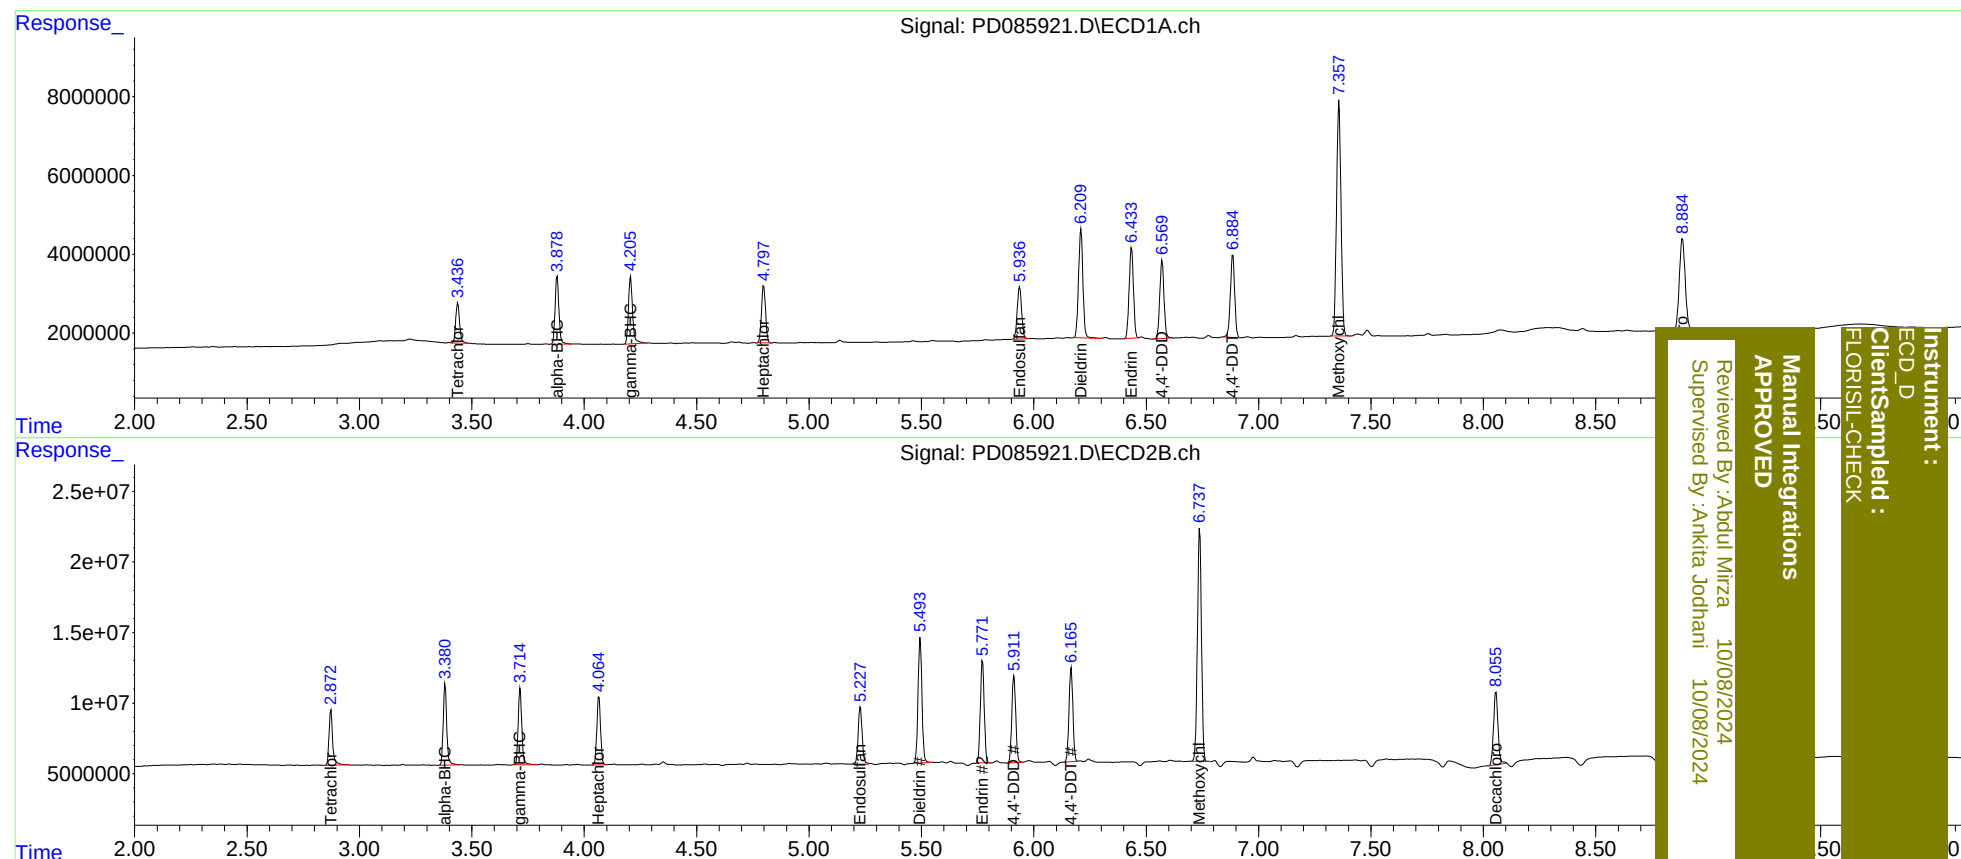

Reviewed By: Abdul Mirza 10/08/2024
Supervised By: Ankita Jodhani 10/08/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
FLORISIL-CHECK