



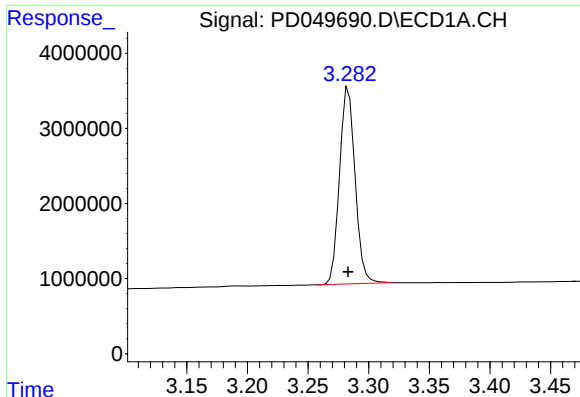

#1 Tetrachloro-m-xylene

R.T.: 3.283 min
Delta R.T.: 0.000 min
Response: 23414280
Conc: 19.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

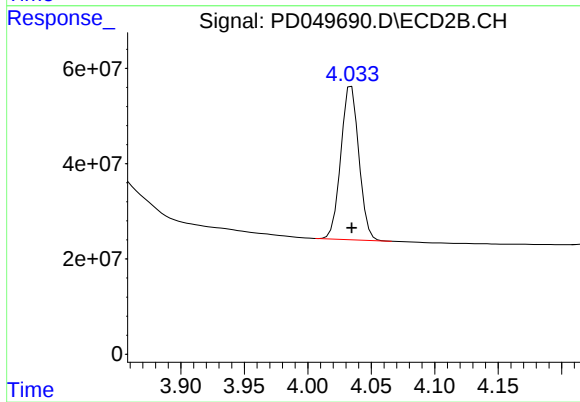

#1 Tetrachloro-m-xylene

R.T.: 4.034 min
Delta R.T.: 0.000 min
Response: 318753889
Conc: 22.95 ng/ml