

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100818\
 Data File : PD049658.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2018 18:34
 Operator : AJ\SJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 02:23:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100818.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 09 02:11:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	4.035	29672115	351.8E6	24.243	25.695
28)	SA Decachlor...	7.877	9.126	28712060	318.7E6	26.065	26.363
Target Compounds							
23)	Chlordane-1	4.109	5.036	12894321	176.6E6	244.942	255.335
24)	Chlordane-2	4.588	5.505	14290872	169.2E6	258.450	261.732
25)	Chlordane-3	5.127	6.152	40701912	575.6E6	235.186	254.789
26)	Chlordane-4	5.183	6.227	40532720	654.0E6	239.250	256.426
27)	Chlordane-5	5.982	7.034	13486424	127.5E6	246.528m	252.669



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100818\
Data File : PD049658.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2018 18:34
Operator : AJ\SJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 02:23:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100818.M
Quant Title : GC Extractables
QLast Update : Tue Oct 09 02:11:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

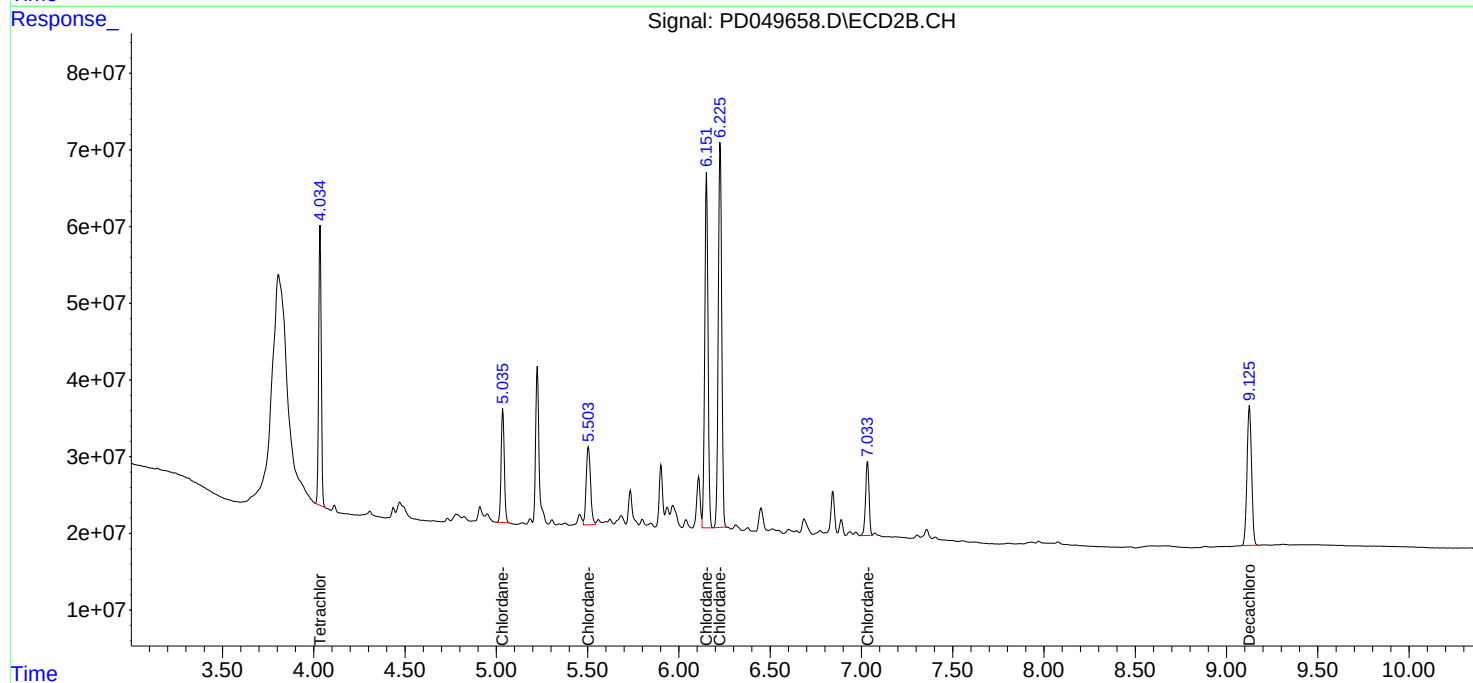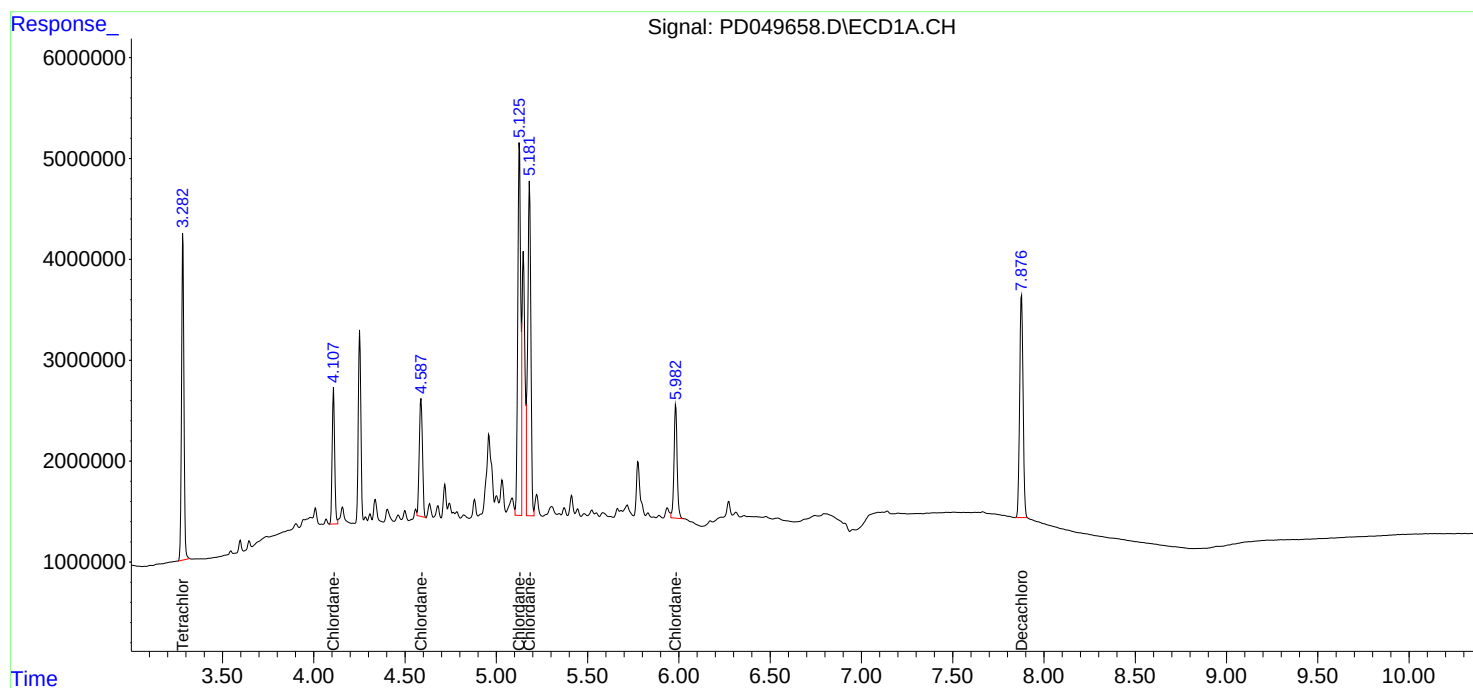


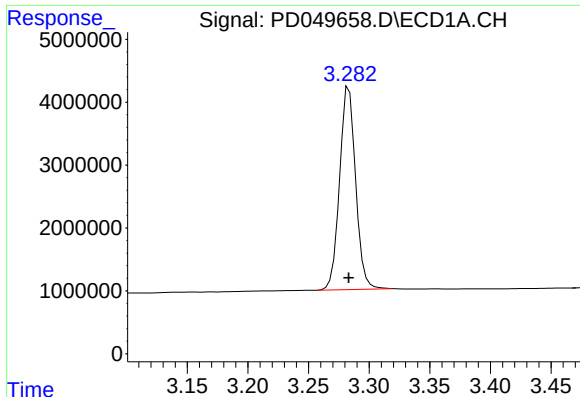

#1 Tetrachloro-m-xylene


R.T.: 3.283 min
Delta R.T.: 0.000 min
Response: 29672115
Conc: 24.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

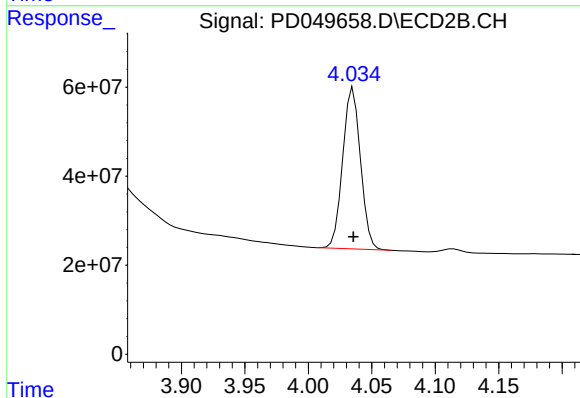


#1 Tetrachloro-m-xylene

R.T.: 4.035 min
Delta R.T.: 0.000 min
Response: 351843949
Conc: 25.69 ng/ml

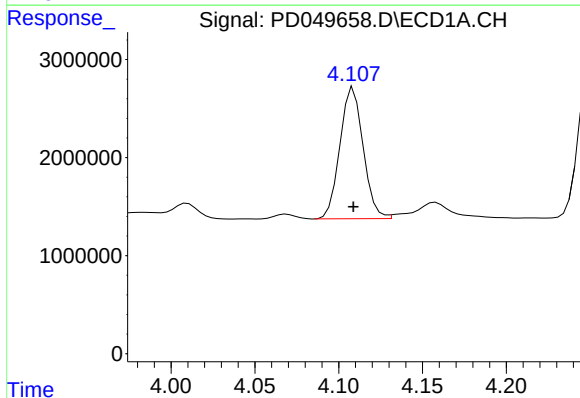


#23 Chlordane-1

R.T.: 4.109 min
Delta R.T.: 0.000 min
Response: 12894321
Conc: 244.94 ng/ml

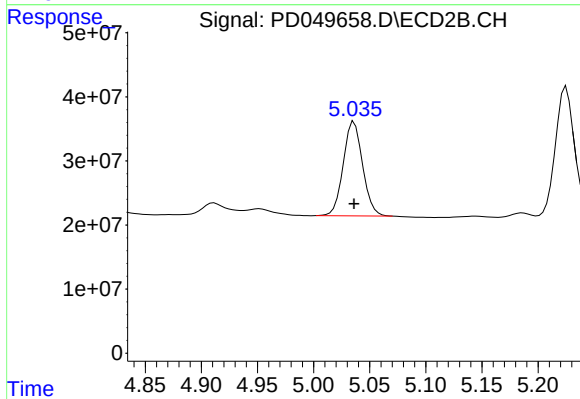

#23 Chlordane-1


R.T.: 5.036 min
Delta R.T.: 0.000 min
Response: 176590124
Conc: 255.33 ng/ml

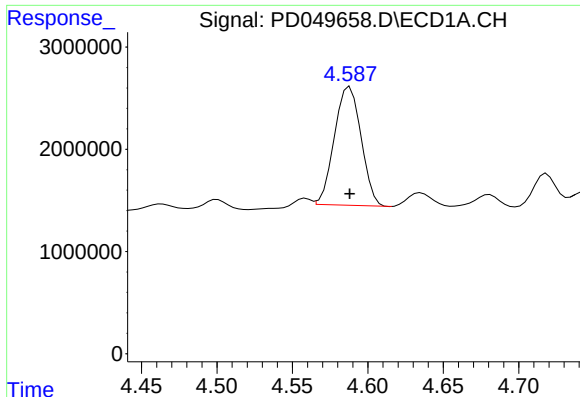

#24 Chlordane-2


R.T.: 4.588 min
Delta R.T.: 0.000 min
Response: 14290872
Conc: 258.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

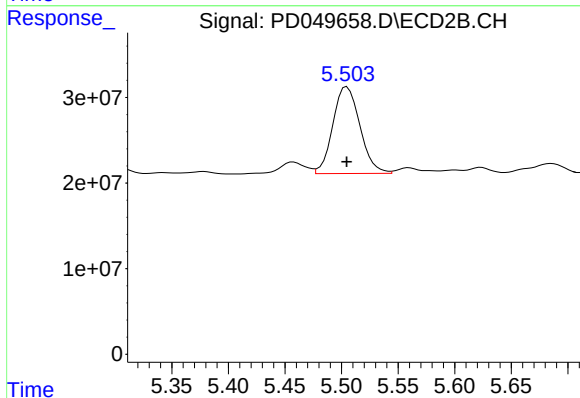


#24 Chlordane-2

R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 169209401
Conc: 261.73 ng/ml

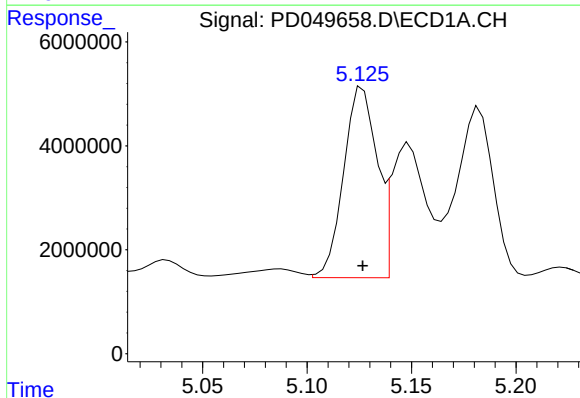


#25 Chlordane-3

R.T.: 5.127 min
Delta R.T.: 0.000 min
Response: 40701912
Conc: 235.19 ng/ml

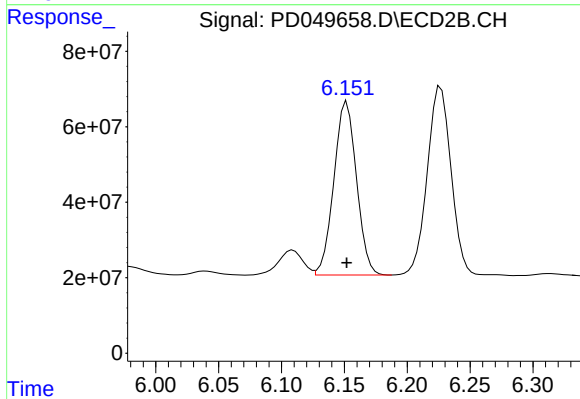

#25 Chlordane-3


R.T.: 6.152 min
Delta R.T.: 0.000 min
Response: 575643870
Conc: 254.79 ng/ml

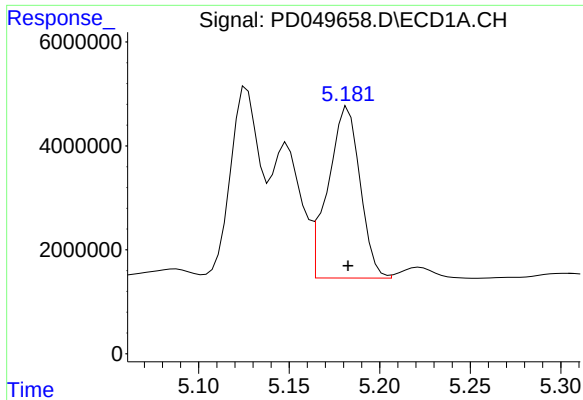

#26 Chlordane-4


R.T.: 5.183 min
Delta R.T.: 0.000 min
Response: 40532720
Conc: 239.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

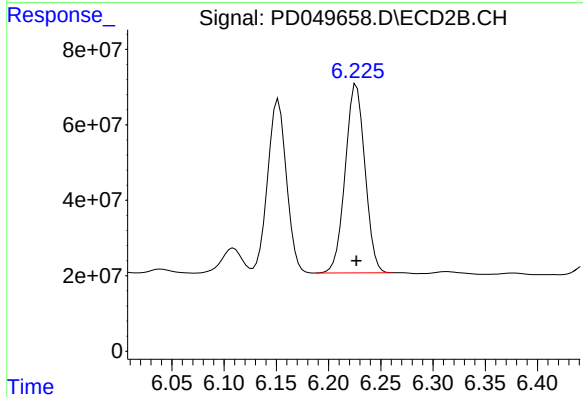


#26 Chlordane-4

R.T.: 6.227 min
Delta R.T.: 0.000 min
Response: 654030574
Conc: 256.43 ng/ml

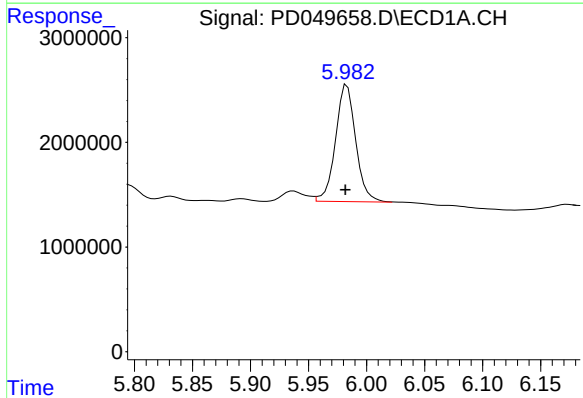


#27 Chlordane-5

R.T.: 5.982 min
Delta R.T.: 0.000 min
Response: 13486424
Conc: 246.53 ng/ml m

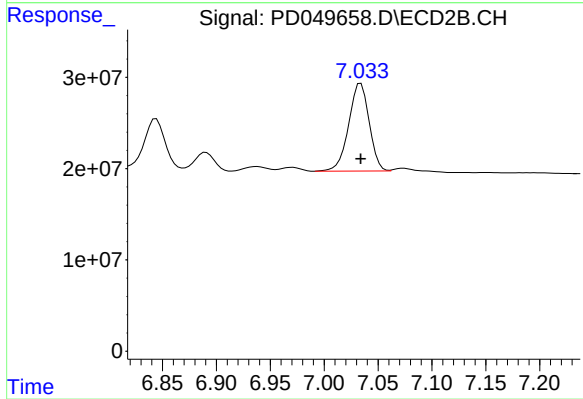

#27 Chlordane-5


R.T.: 7.034 min
Delta R.T.: 0.000 min
Response: 127484120
Conc: 252.67 ng/ml

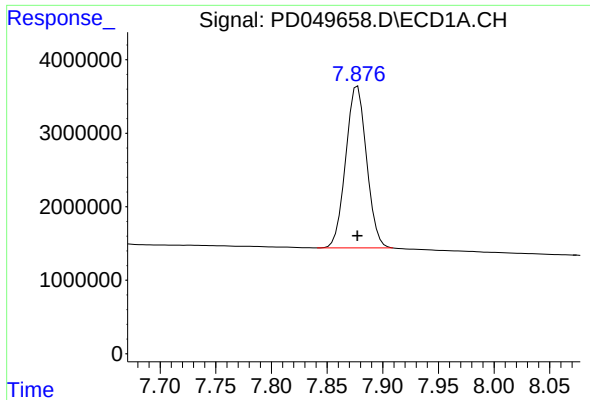

#28 Decachlorobiphenyl

R.T.: 7.877 min
Delta R.T.: 0.000 min
Response: 28712060
Conc: 26.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

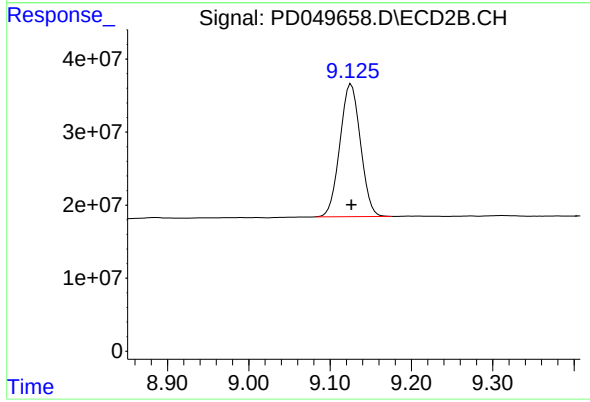

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 318671202
Conc: 26.36 ng/ml