

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100818\
 Data File : PD049659.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2018 18:48
 Operator : AJ\SJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 02:25:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100818.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 09 02:11:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	4.036	5562093	66189826	4.629	4.866
28)	SA Decachlor...	7.877	9.127	6041777	64902156	5.380	5.291
Target Compounds							
23)	Chlordane-1	4.109	5.036	2205004	32753905	43.292	47.865
24)	Chlordane-2	4.586	5.505	2820891	34024266	50.802m	52.081
25)	Chlordane-3	5.127	6.152	7342011	113.0E6	43.750	50.009
26)	Chlordane-4	5.182	6.227	7367360	128.9E6	44.650	50.429
27)	Chlordane-5	5.981	7.033	2455064	24352357	45.886m	48.528m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100818\
Data File : PD049659.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2018 18:48
Operator : AJ\SJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 02:25:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100818.M
Quant Title : GC Extractables
QLast Update : Tue Oct 09 02:11:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

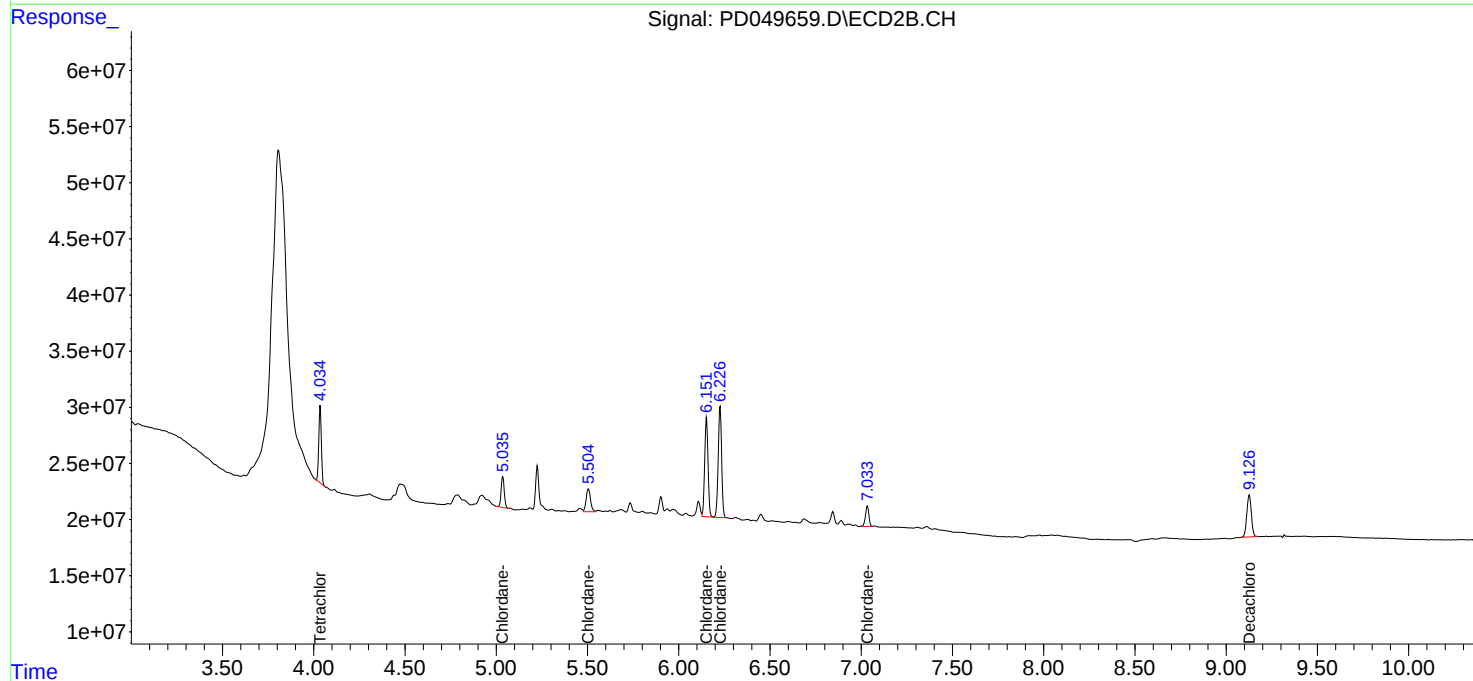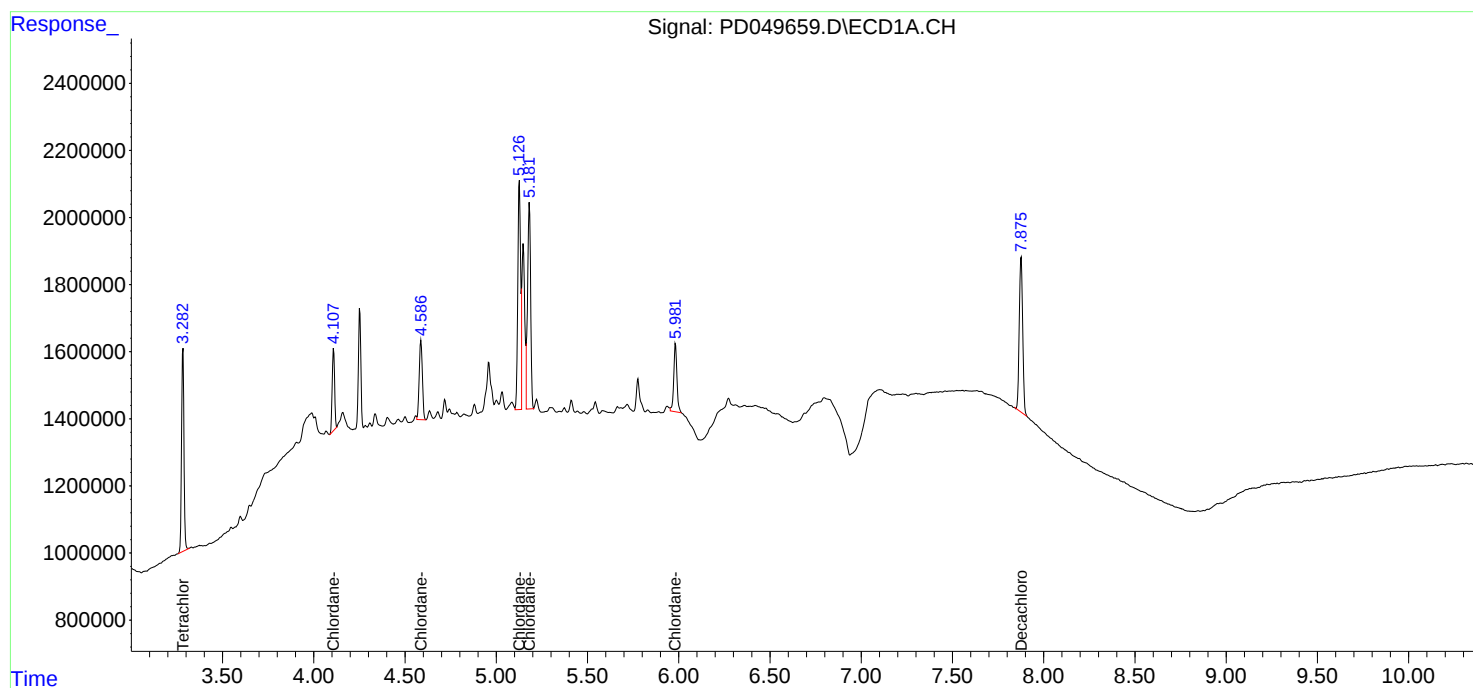


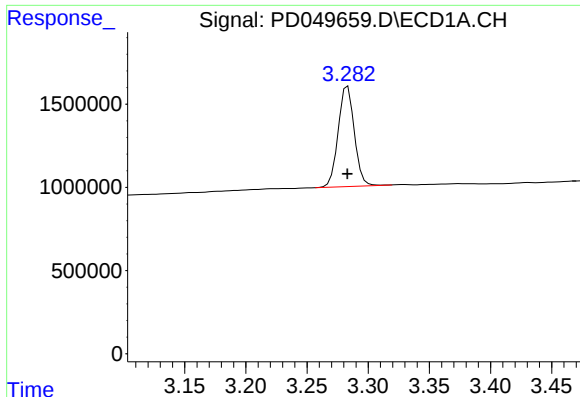

#1 Tetrachloro-m-xylene


R.T.: 3.283 min
Delta R.T.: 0.000 min
Response: 5562093
Conc: 4.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

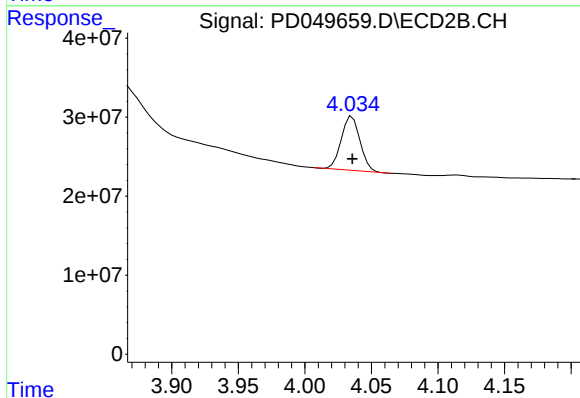


#1 Tetrachloro-m-xylene

R.T.: 4.036 min
Delta R.T.: 0.000 min
Response: 66189826
Conc: 4.87 ng/ml

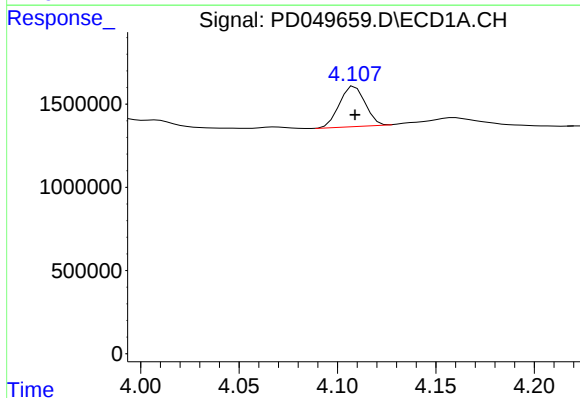


#23 Chlordane-1

R.T.: 4.109 min
Delta R.T.: 0.000 min
Response: 2205004
Conc: 43.29 ng/ml

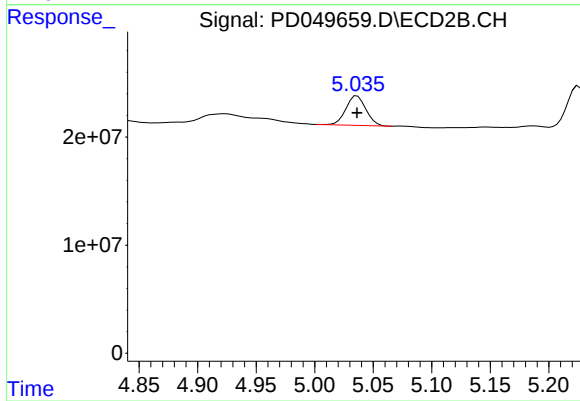

#23 Chlordane-1


R.T.: 5.036 min
Delta R.T.: 0.000 min
Response: 32753905
Conc: 47.87 ng/ml

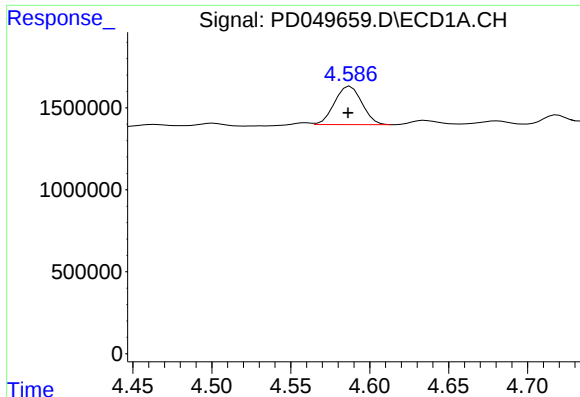

#24 Chlordane-2


R.T.: 4.586 min
Delta R.T.: 0.000 min
Response: 2820891
Conc: 50.80 ng/ml m

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

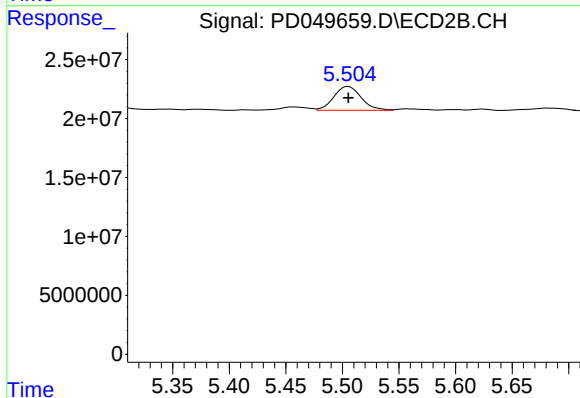


#24 Chlordane-2

R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 34024266
Conc: 52.08 ng/ml

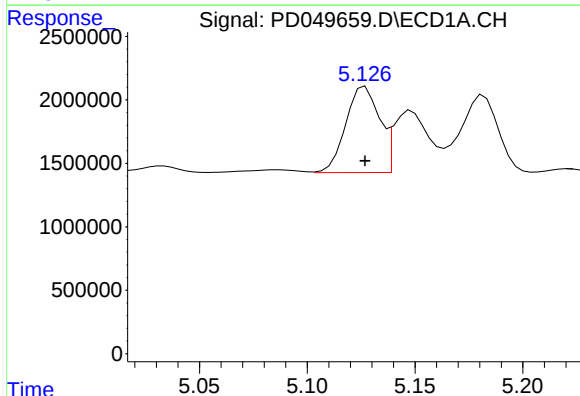


#25 Chlordane-3

R.T.: 5.127 min
Delta R.T.: 0.000 min
Response: 7342011
Conc: 43.75 ng/ml

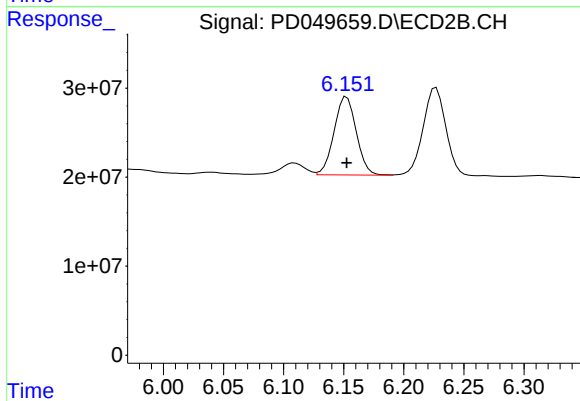

#25 Chlordane-3


R.T.: 6.152 min
Delta R.T.: 0.000 min
Response: 112991476
Conc: 50.01 ng/ml

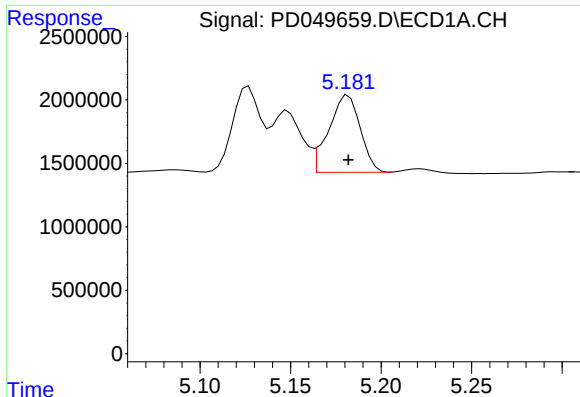

#26 Chlordane-4


R.T.: 5.182 min
Delta R.T.: 0.000 min
Response: 7367360
Conc: 44.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

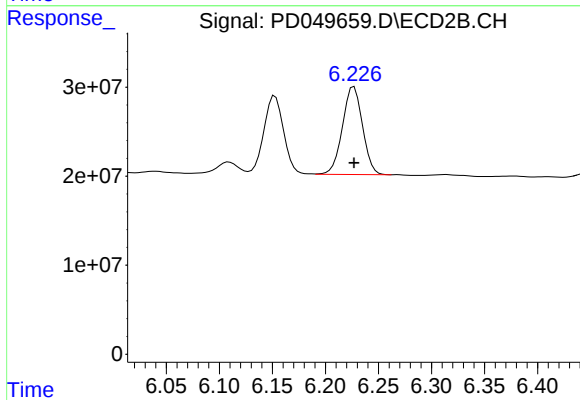


#26 Chlordane-4

R.T.: 6.227 min
Delta R.T.: 0.000 min
Response: 128898372
Conc: 50.43 ng/ml

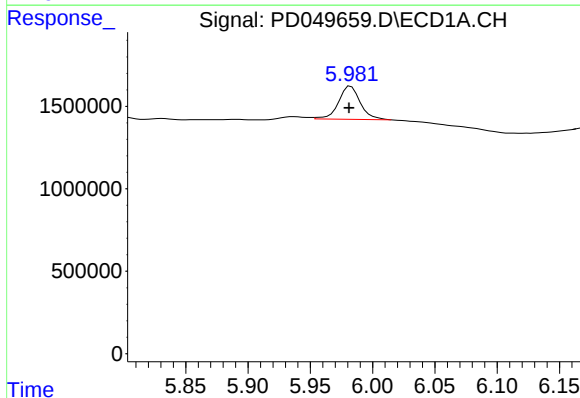


#27 Chlordane-5

R.T.: 5.981 min
Delta R.T.: 0.000 min
Response: 2455064
Conc: 45.89 ng/ml m

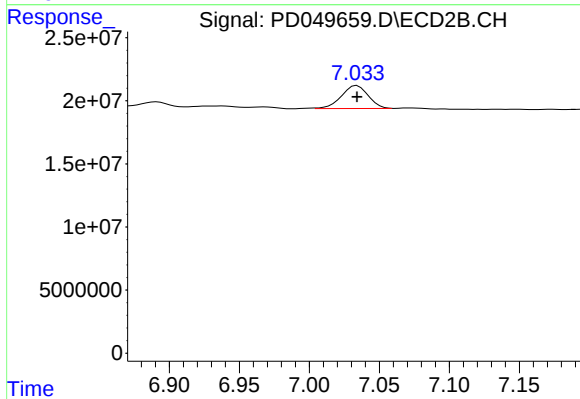

#27 Chlordane-5


R.T.: 7.033 min
Delta R.T.: -0.001 min
Response: 24352357
Conc: 48.53 ng/ml m

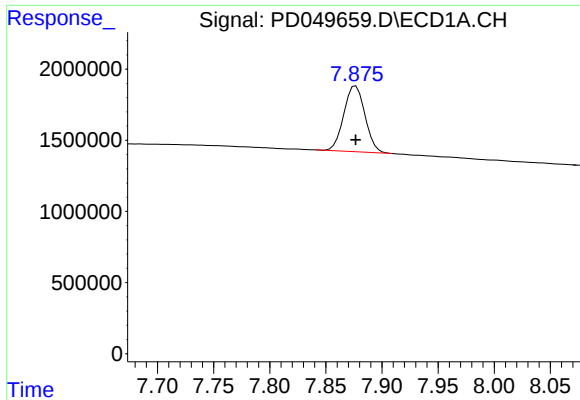

#28 Decachlorobiphenyl

R.T.: 7.877 min
Delta R.T.: 0.000 min
Response: 6041777
Conc: 5.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

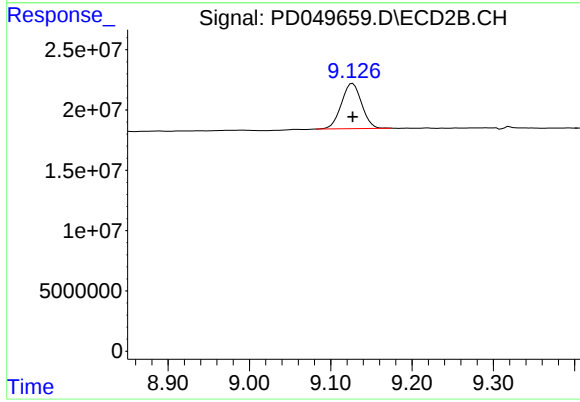

#28 Decachlorobiphenyl

R.T.: 9.127 min
Delta R.T.: 0.000 min
Response: 64902156
Conc: 5.29 ng/ml