

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100818\
 Data File : PD049682.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2018 00:04
 Operator : AJ\SJ
 Sample : MDL CHLOR
 Misc : ECD_D MDL CHLOR 50 PPB WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:07:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100818.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 09 04:09:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	4.035	22712944	290.3E6	19.157	20.904
28)	SA Decachlor...	7.876	9.126	23805461	280.2E6	20.459	22.178
Target Compounds							
23)	Chlordane-1	4.109	5.036	1918650	27570274	37.669	40.290
24)	Chlordane-2	4.586	5.503	2549327	30524862	45.918m	46.724m
25)	Chlordane-3	5.125	6.150	7193678	107.7E6	42.866m	47.656m
26)	Chlordane-4	5.182	6.226	6529655	122.4E6	39.573	47.887
27)	Chlordane-5	5.983	7.032	2031304	23304891	37.895	46.512m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100818\
Data File : PD049682.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2018 00:04
Operator : AJ\SJ
Sample : MDL CHLOR
Misc : ECD_D MDL CHLOR 50 PPB WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:07:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100818.M
Quant Title : GC Extractables
QLast Update : Tue Oct 09 04:09:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

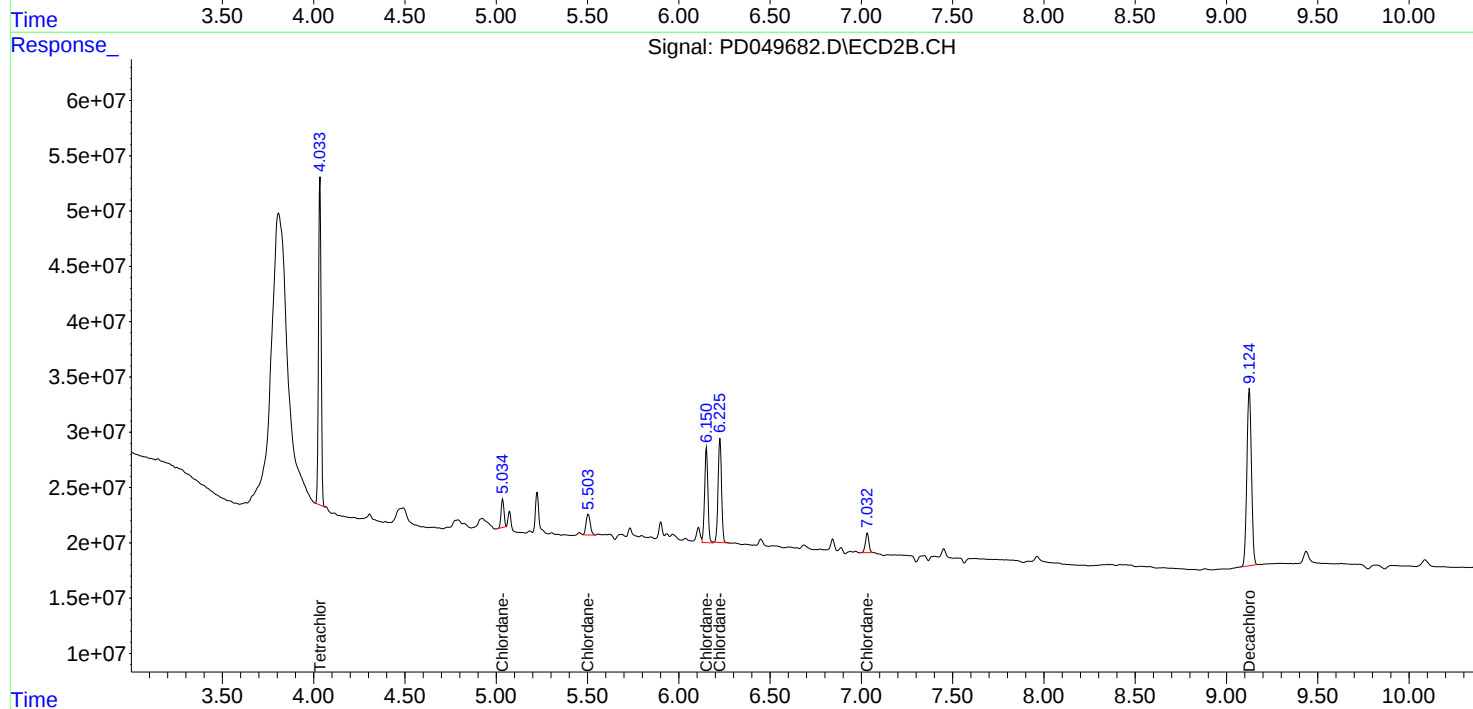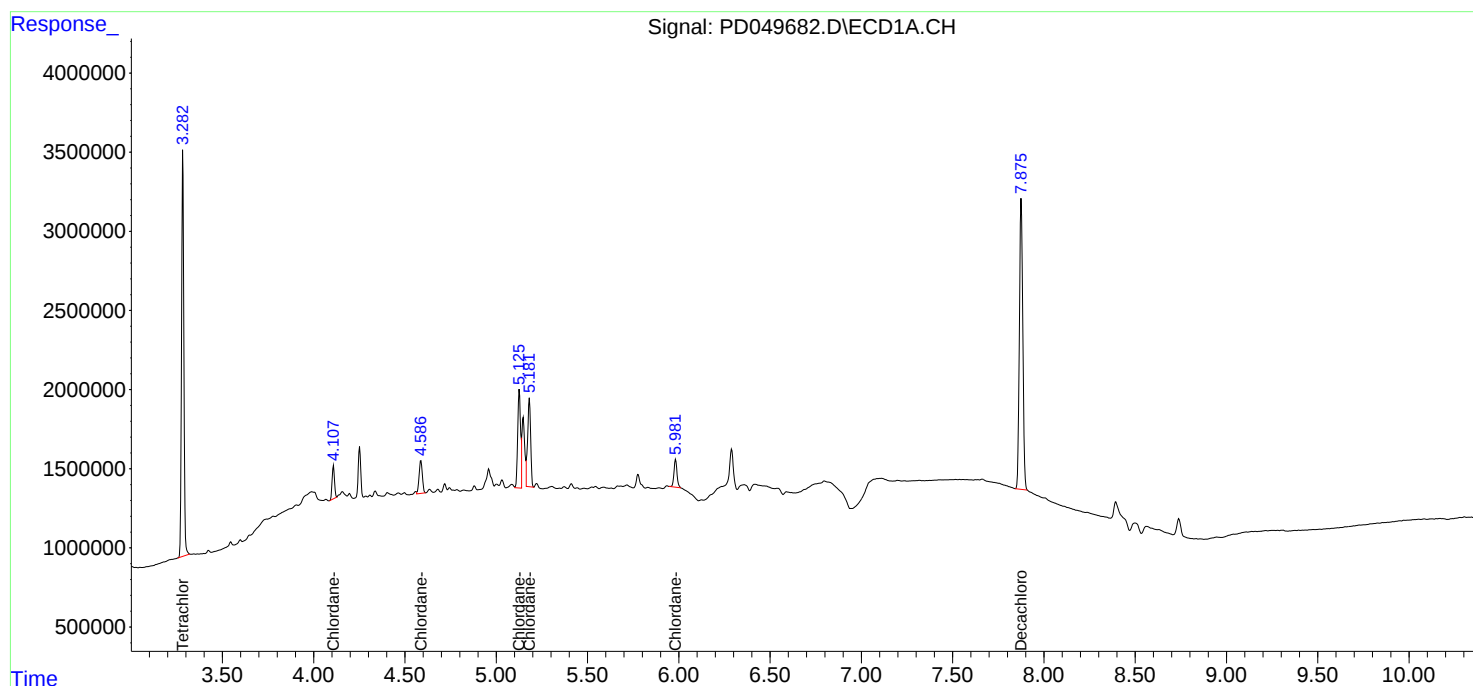


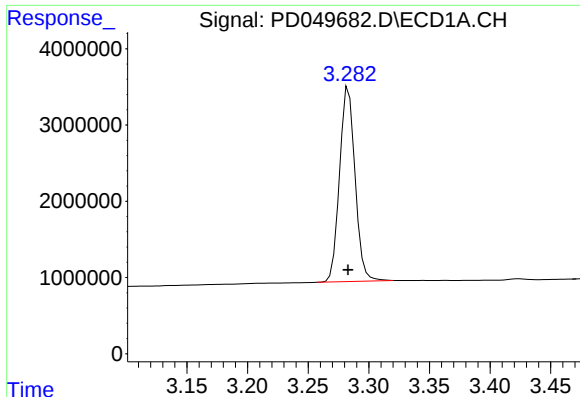

#1 Tetrachloro-m-xylene


R.T.: 3.283 min
Delta R.T.: 0.000 min
Response: 22712944
Conc: 19.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL CHLOR

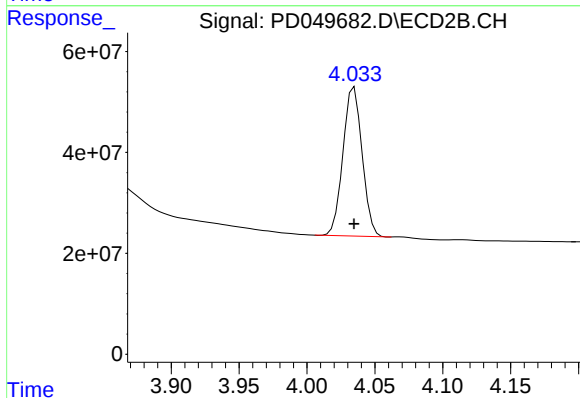


#1 Tetrachloro-m-xylene

R.T.: 4.035 min
Delta R.T.: 0.000 min
Response: 290319935
Conc: 20.90 ng/ml

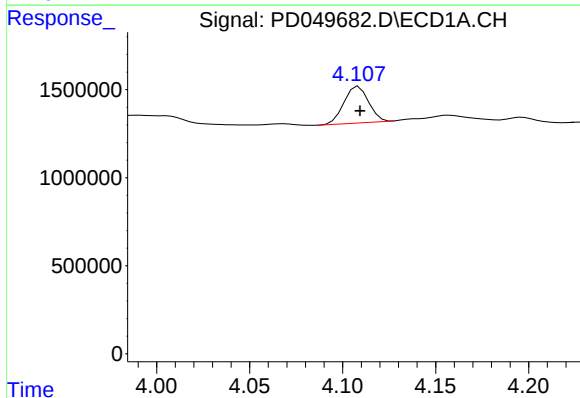


#23 Chlordane-1

R.T.: 4.109 min
Delta R.T.: 0.000 min
Response: 1918650
Conc: 37.67 ng/ml

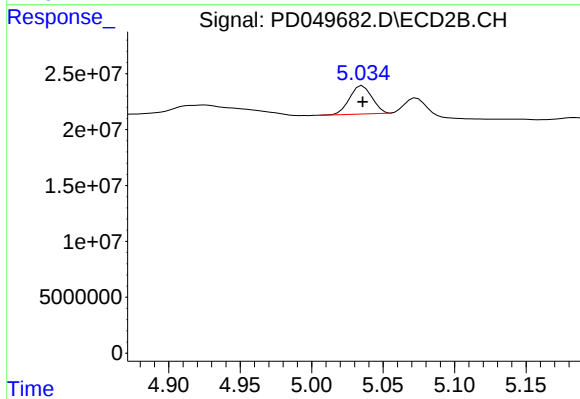

#23 Chlordane-1


R.T.: 5.036 min
Delta R.T.: 0.000 min
Response: 27570274
Conc: 40.29 ng/ml

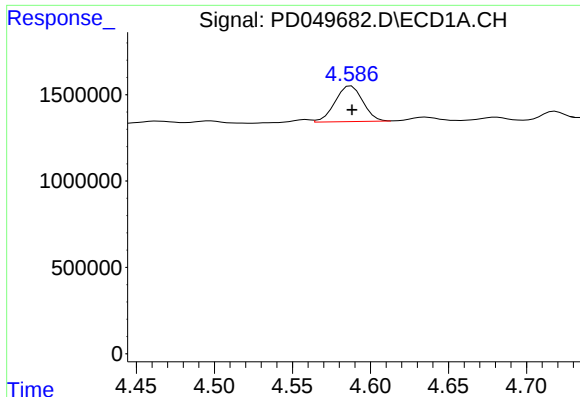

#24 Chlordane-2


R.T.: 4.586 min
Delta R.T.: -0.002 min
Response: 2549327
Conc: 45.92 ng/ml m

Instrument :
ECD_D
ClientSampleId :
MDL CHLOR

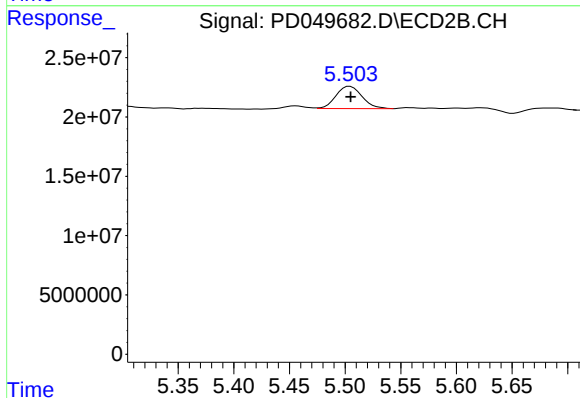


#24 Chlordane-2

R.T.: 5.503 min
Delta R.T.: -0.002 min
Response: 30524862
Conc: 46.72 ng/ml m

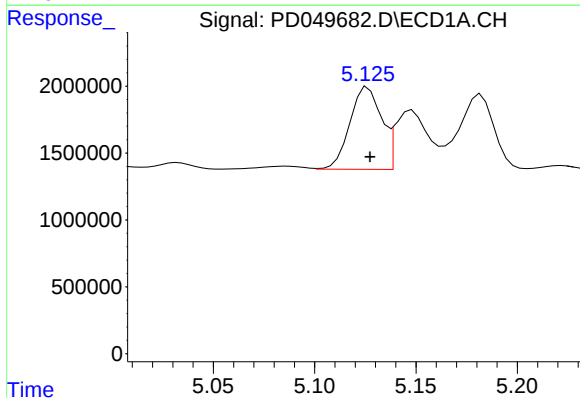


#25 Chlordane-3

R.T.: 5.125 min
Delta R.T.: -0.002 min
Response: 7193678
Conc: 42.87 ng/ml m

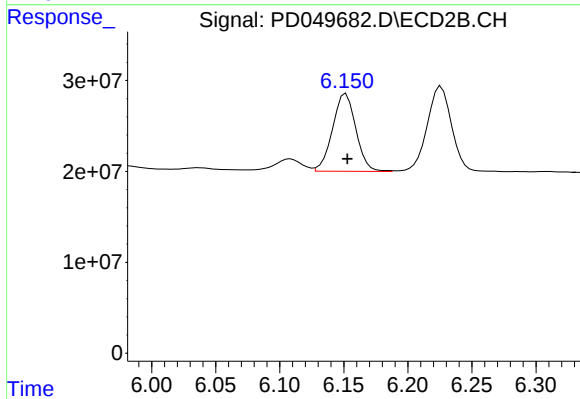

#25 Chlordane-3


R.T.: 6.150 min
Delta R.T.: -0.002 min
Response: 107673932
Conc: 47.66 ng/ml m

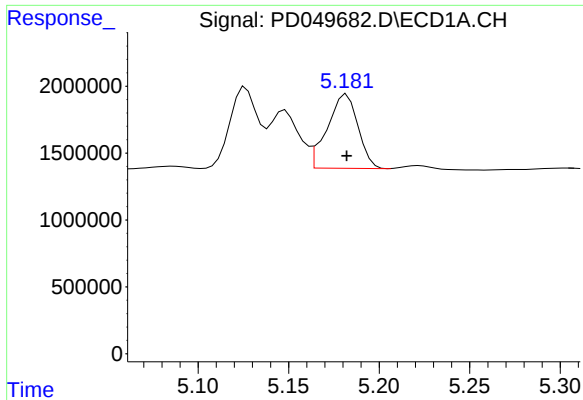

#26 Chlordane-4


R.T.: 5.182 min
Delta R.T.: 0.000 min
Response: 6529655
Conc: 39.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL CHLOR

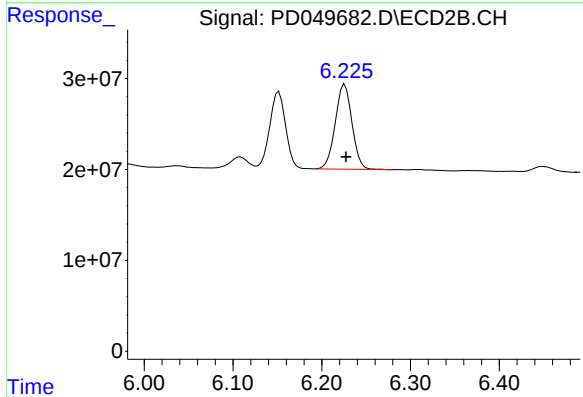


#26 Chlordane-4

R.T.: 6.226 min
Delta R.T.: -0.001 min
Response: 122400171
Conc: 47.89 ng/ml

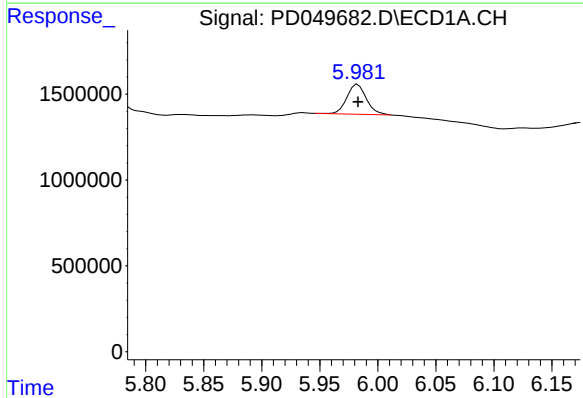


#27 Chlordane-5

R.T.: 5.983 min
Delta R.T.: 0.000 min
Response: 2031304
Conc: 37.89 ng/ml

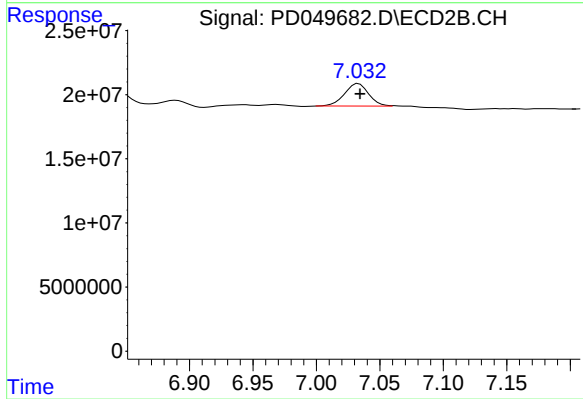

#27 Chlordane-5


R.T.: 7.032 min
Delta R.T.: -0.003 min
Response: 23304891
Conc: 46.51 ng/ml m

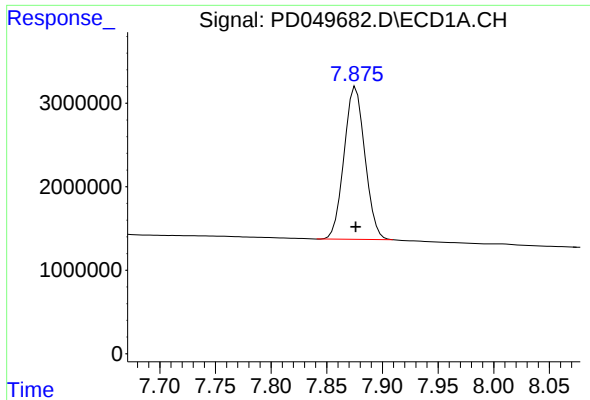

#28 Decachlorobiphenyl

R.T.: 7.876 min
Delta R.T.: 0.000 min
Response: 23805461
Conc: 20.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL CHLOR

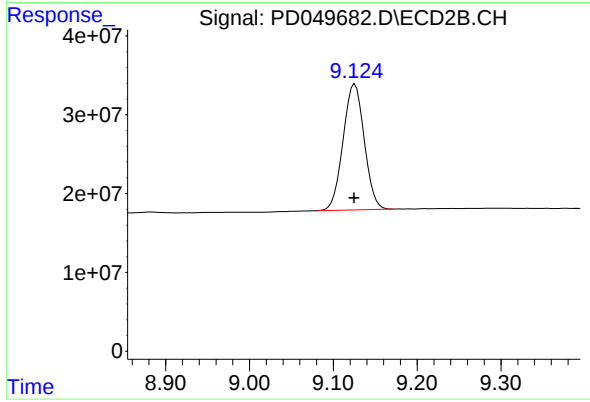

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 280225954
Conc: 22.18 ng/ml