

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100819\
 Data File : PD055195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2019 10:50
 Operator : SG\AJ
 Sample : K5214-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 02:06:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds							
3) MA	gamma-BHC...	3.954f	0.000	184841	0	0.172	N.D. #
7) B	delta-BHC	4.403f	0.000	87615	0	<MDL	N.D. #
8) B	Heptachlo...	4.940	0.000	131335	0	0.143	N.D. #
10) B	trans-Chl...	5.179	0.000	116421	0	0.123	N.D. #
18) B	Endrin al...	6.247	0.000	450901	0	0.620	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100819\
Data File : PD055195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2019 10:50
Operator : SG\AJ
Sample : K5214-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 02:06:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

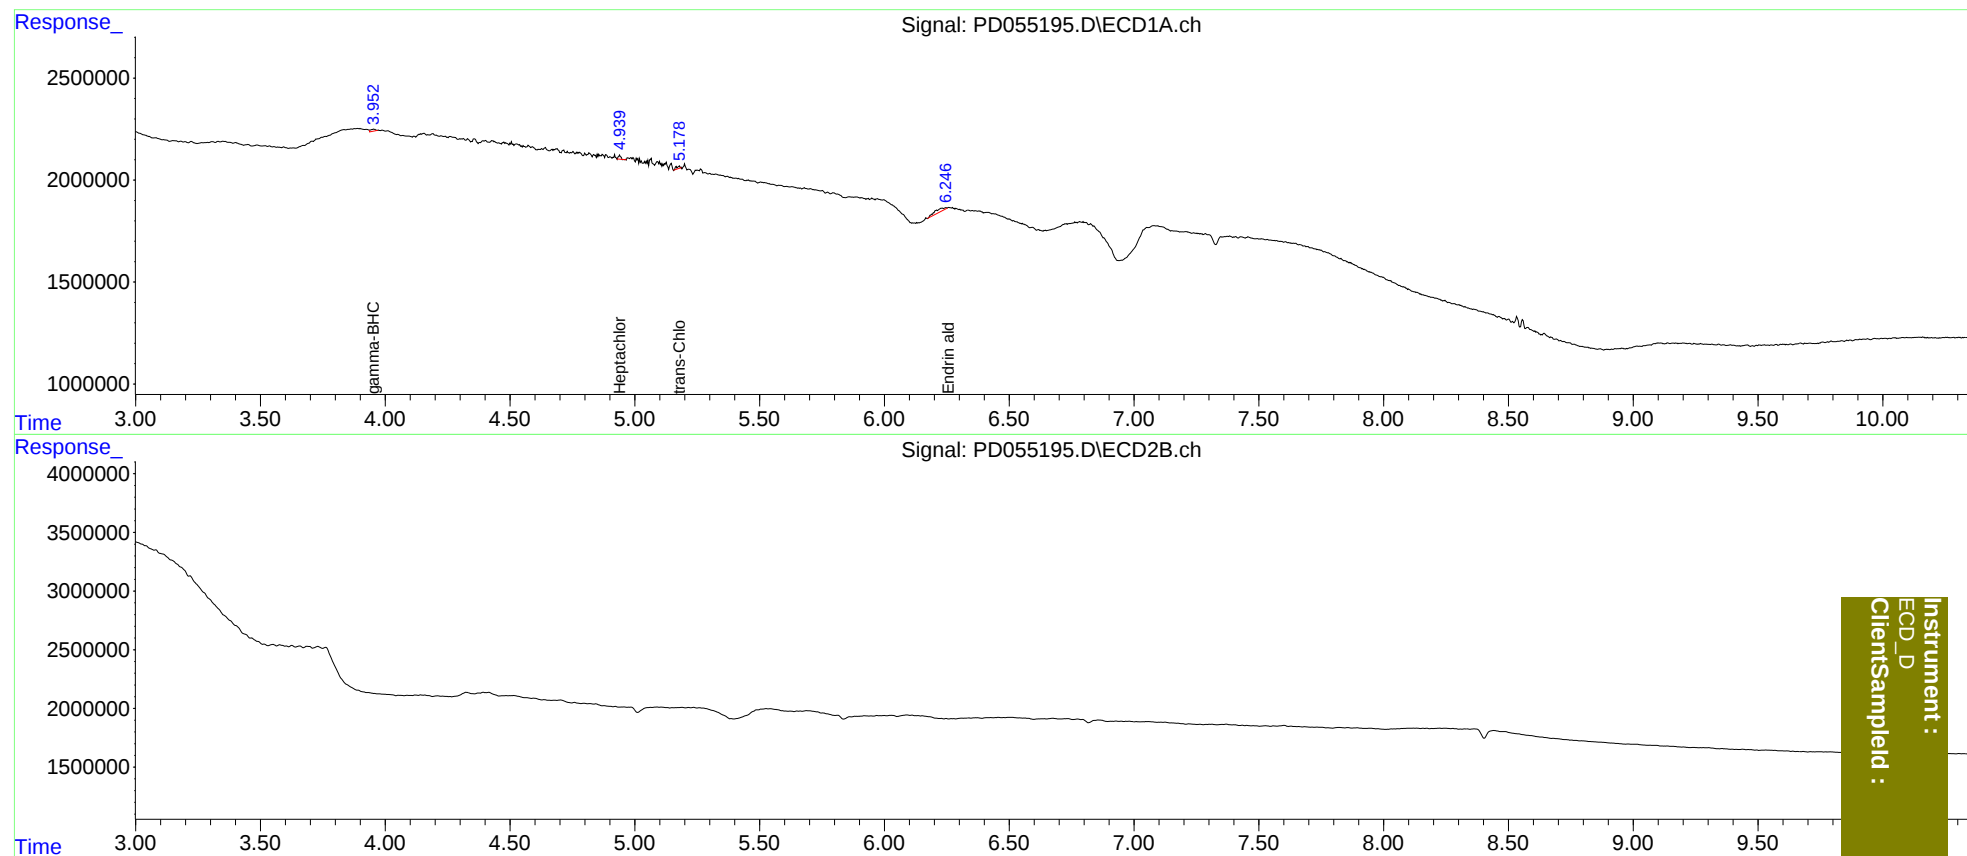


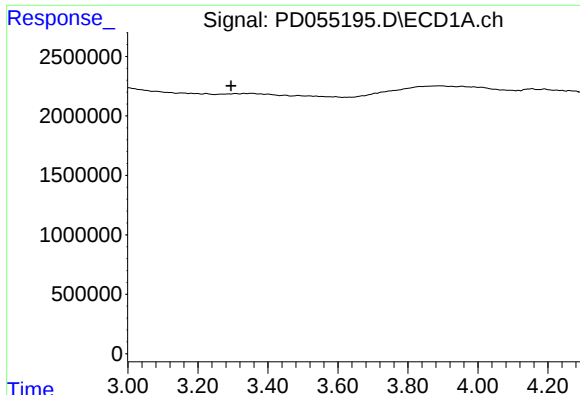

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.295 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

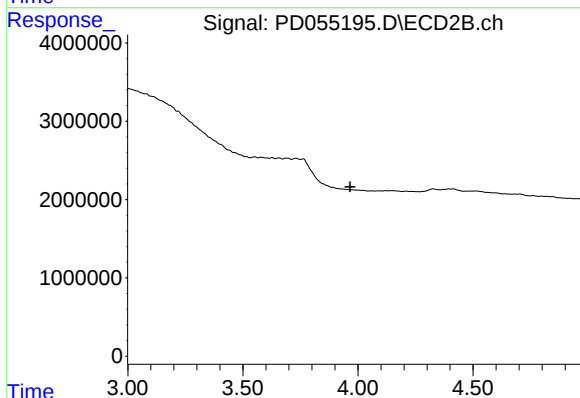


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.966 min
Response: 0
Conc: N.D.

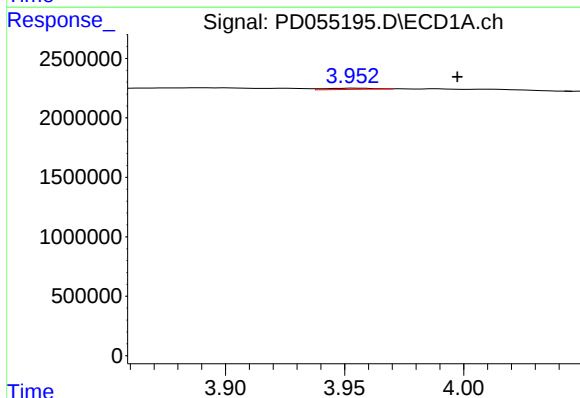


#3 gamma-BHC (Lindane)

R.T.: 3.954 min
Delta R.T.: -0.043 min
Response: 184841
Conc: 0.17 ng/ml

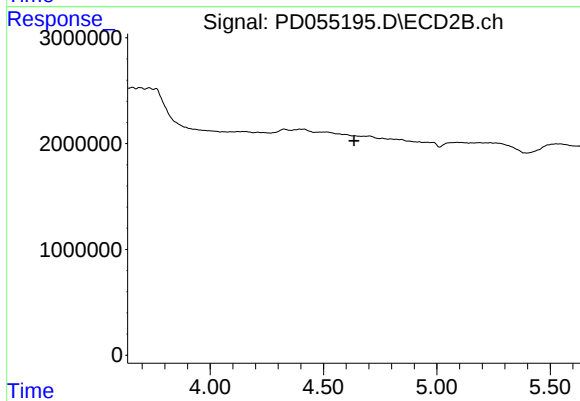

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.635 min
Response: 0
Conc: N.D.

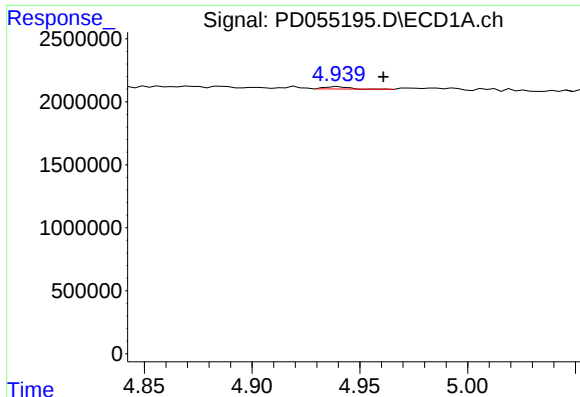

#8 Heptachlor epoxide


R.T.: 4.940 min
Delta R.T.: -0.021 min
Response: 131335
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

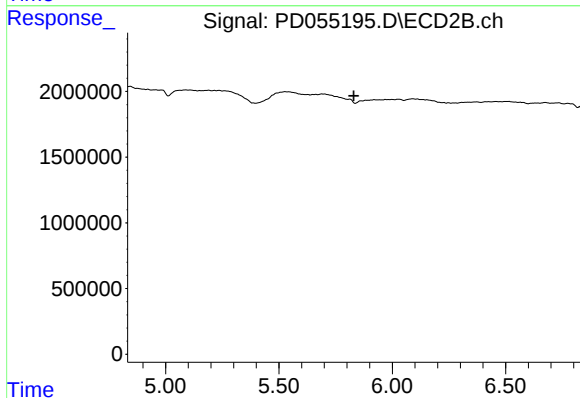


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.831 min
Response: 0
Conc: N.D.

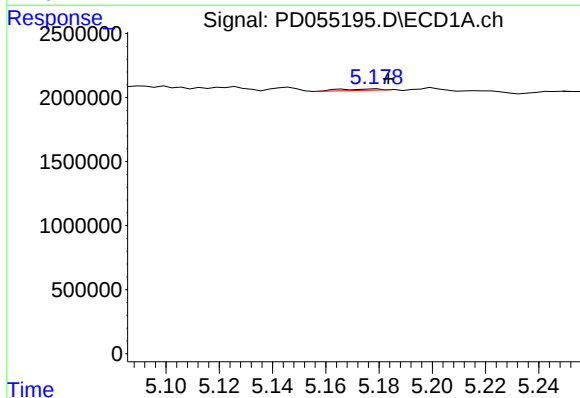


#10 trans-Chlordane

R.T.: 5.179 min
Delta R.T.: -0.004 min
Response: 116421
Conc: 0.12 ng/ml

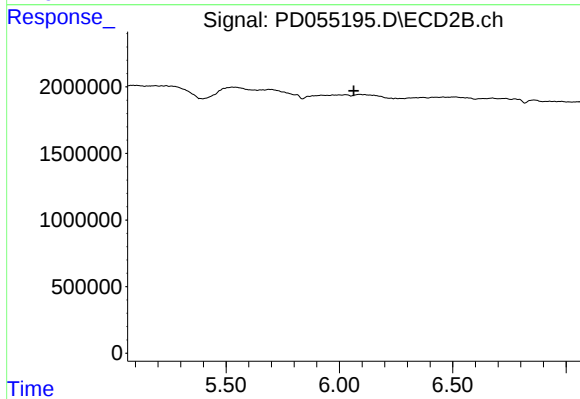

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.063 min
Response: 0
Conc: N.D.

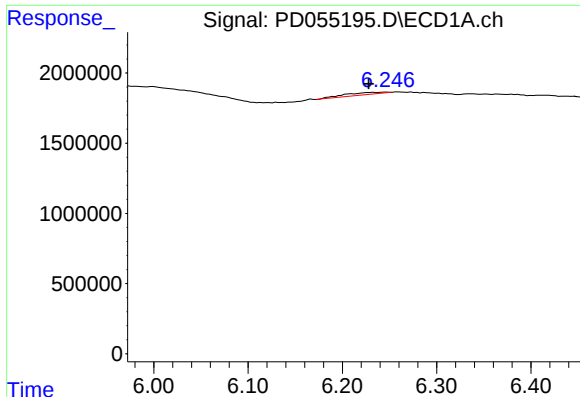

#18 Endrin aldehyde


R.T.: 6.247 min
Delta R.T.: 0.019 min
Response: 450901
Conc: 0.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

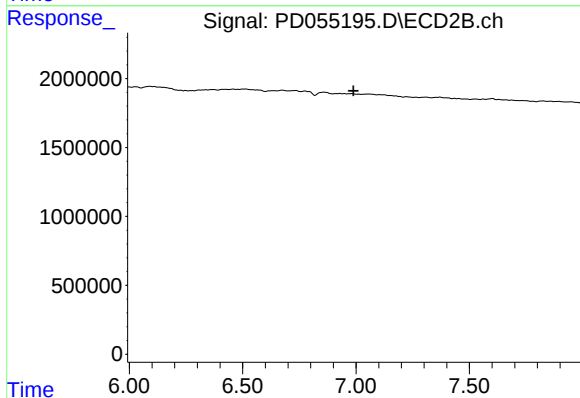


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

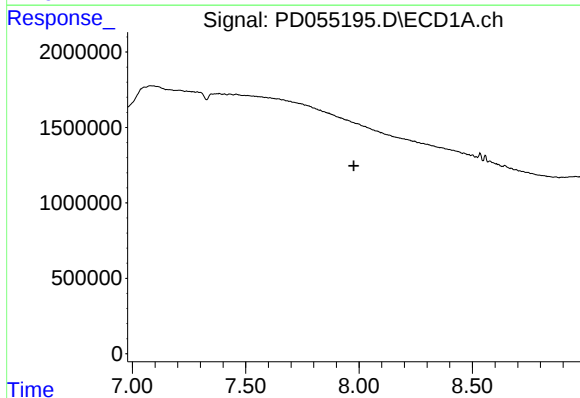

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.977 min
Response: 0
Conc: N.D.

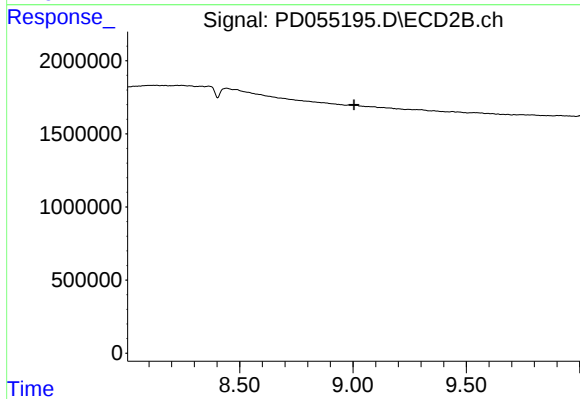

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.005 min
Response: 0
Conc: N.D.