

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
 Data File : PD059540.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2020 09:42
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 13:22:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.526f	4.001f	851789	2810901	0.591	1.293 #
Target Compounds							
18)	B Endrin al...	0.000	7.076	0	4918481	N.D.	2.791 #
20)	A Methoxychlor	7.035f	0.000	534359	0	0.712	N.D. #
22)	Mirex	7.457	0.000	6147827	0	0.893	N.D. #
23)	Chlordane-1	4.415f	0.000	3550247	0	68.334	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
Data File : PD059540.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2020 09:42
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 13:22:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

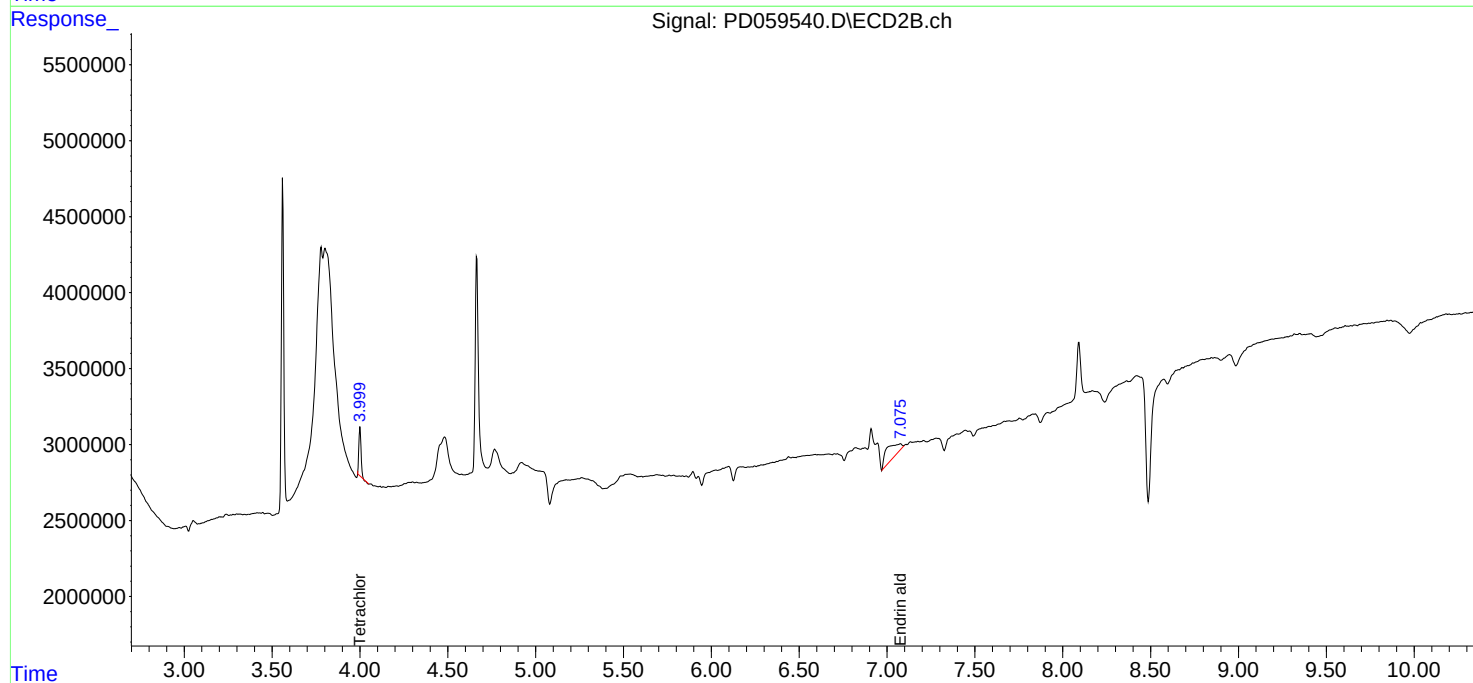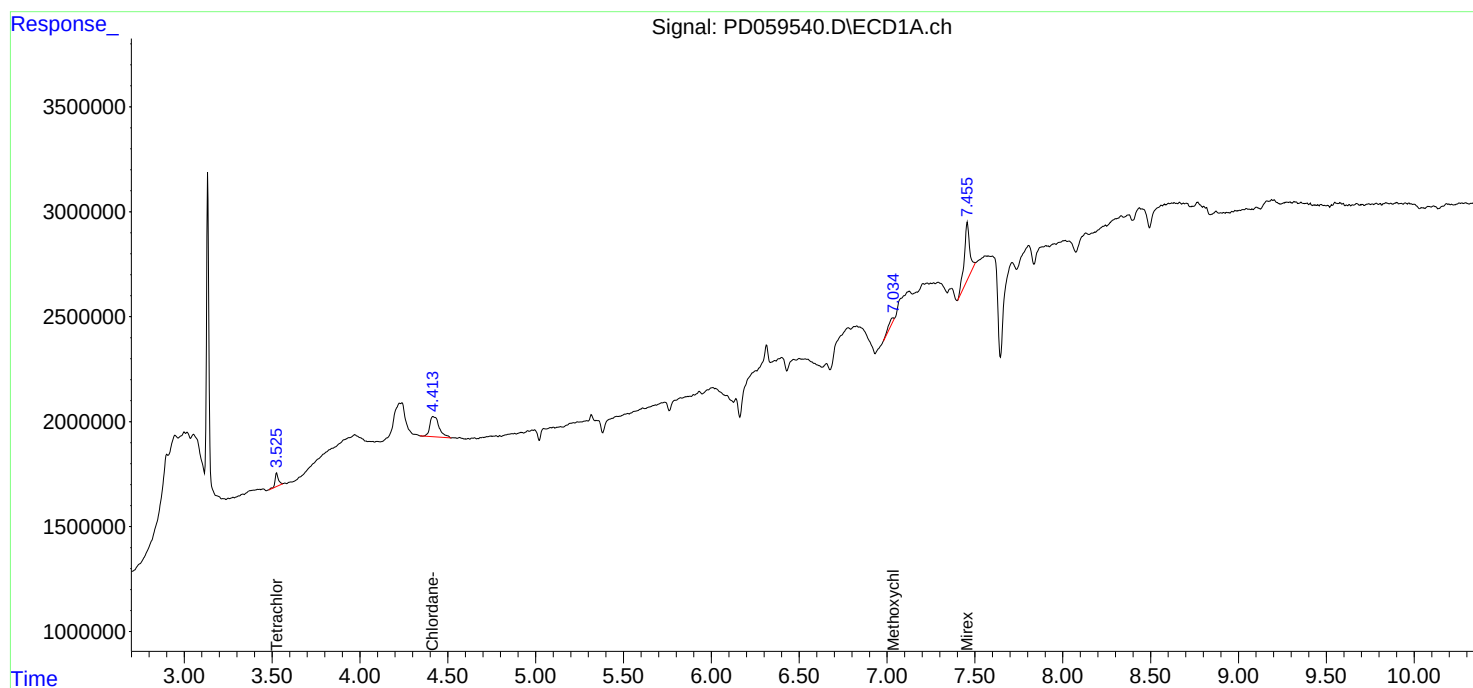


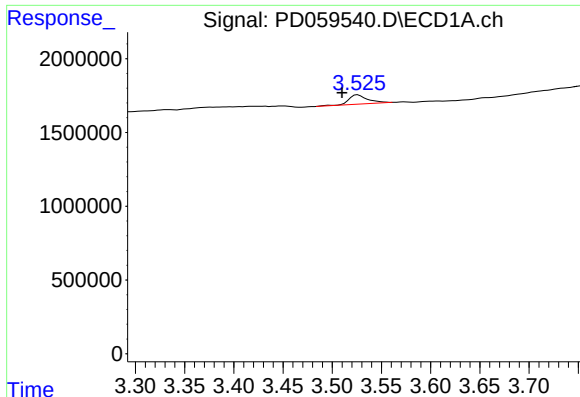

#1 Tetrachloro-m-xylene


R.T.: 3.526 min
Delta R.T.: 0.016 min
Response: 851789
Conc: 0.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

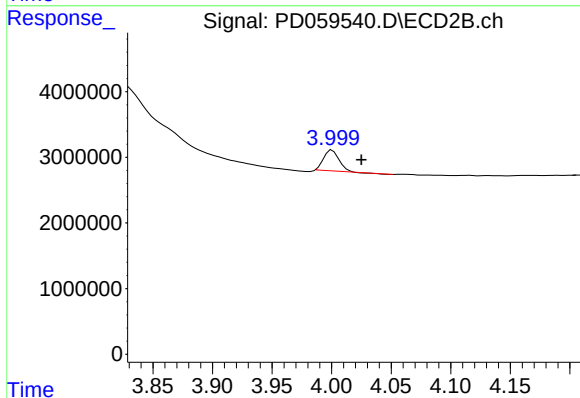


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.024 min
Response: 2810901
Conc: 1.29 ng/ml

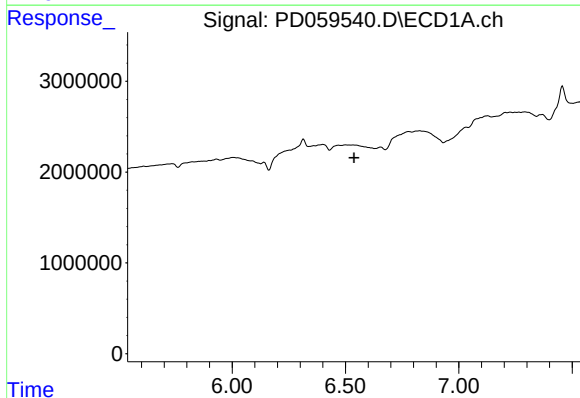


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.538 min
Response: 0
Conc: N.D.

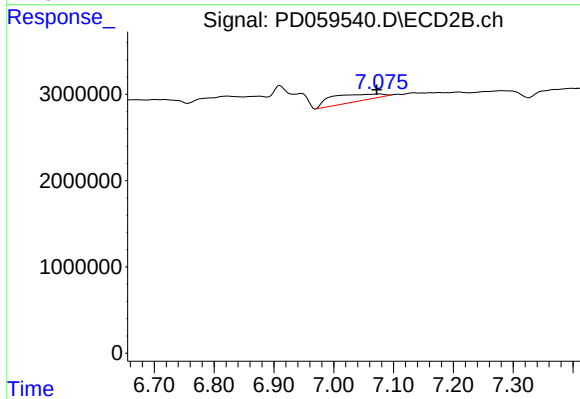

#18 Endrin aldehyde


R.T.: 7.076 min
Delta R.T.: 0.004 min
Response: 4918481
Conc: 2.79 ng/ml

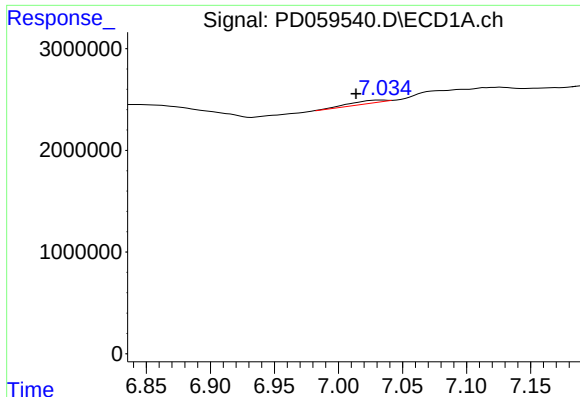

#20 Methoxychlor


R.T.: 7.035 min
Delta R.T.: 0.021 min
Response: 534359
Conc: 0.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

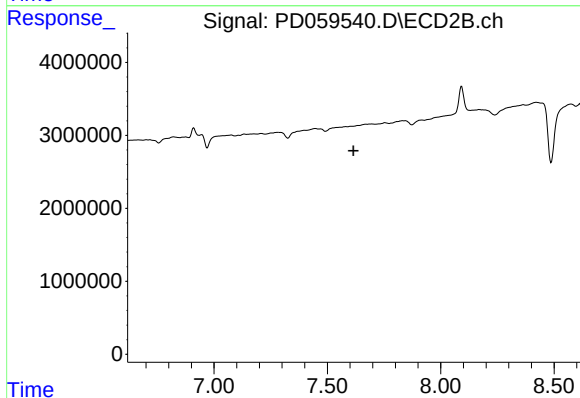


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.616 min
Response: 0
Conc: N.D.

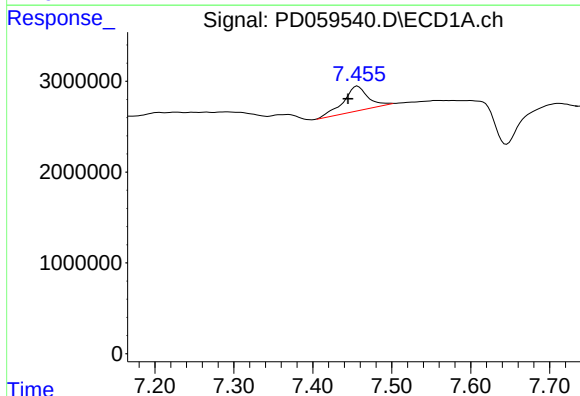


#22 Mirex

R.T.: 7.457 min
Delta R.T.: 0.012 min
Response: 6147827
Conc: 0.89 ng/ml

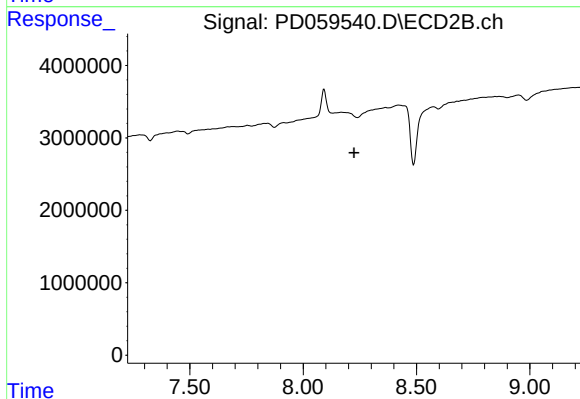

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.224 min
Response: 0
Conc: N.D.

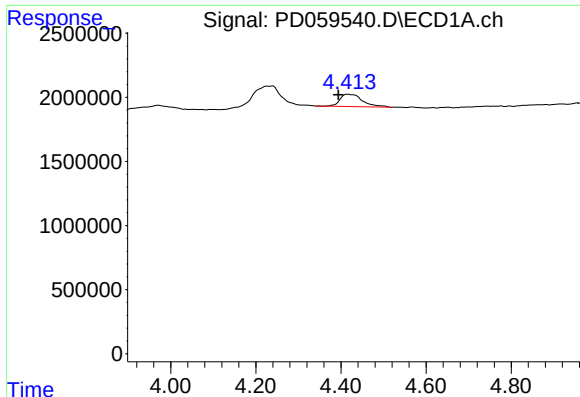

#23 Chlordane-1


R.T.: 4.415 min
Delta R.T.: 0.021 min
Response: 3550247
Conc: 68.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

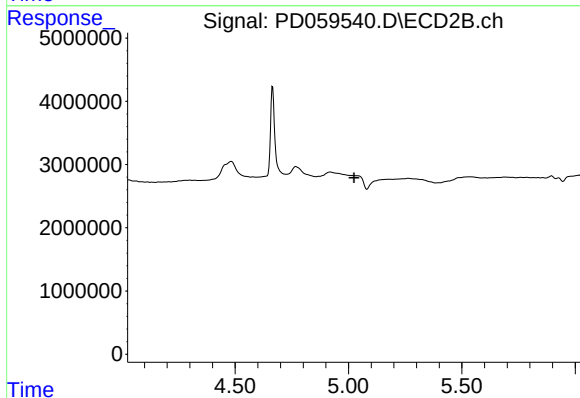


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.024 min
Response: 0
Conc: N.D.

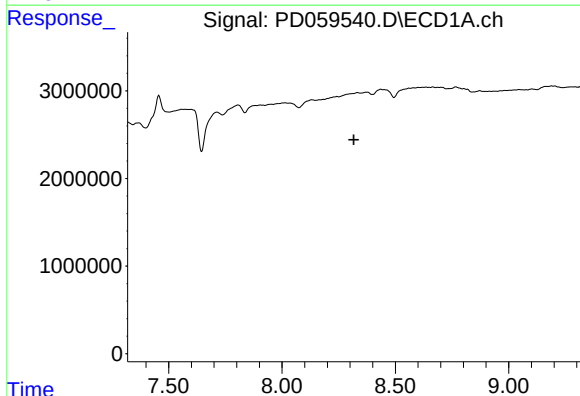

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.316 min
Response: 0
Conc: N.D.

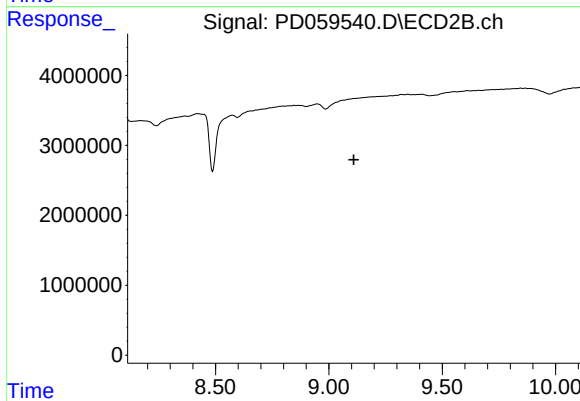

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.110 min
Response: 0
Conc: N.D.