

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
 Data File : PD059541.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2020 09:56
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 13:22:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.509	4.025	33417212	49036770	23.177	22.556
28)	SA Decachlor...	8.315	9.110	25115387	37146502	22.609	23.054
Target Compounds							
17)	MA 4,4'-DDT	0.000	7.136f	0	5793576	N.D.	2.956 #
20)	A Methoxychlor	7.035f	0.000	567195	0	0.756	N.D. #
22)	Mirex	7.456	0.000	5549760	0	0.272	N.D. #
23)	Chlordane-1	4.418f	0.000	3664148	0	70.526	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
Data File : PD059541.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2020 09:56
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 13:22:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

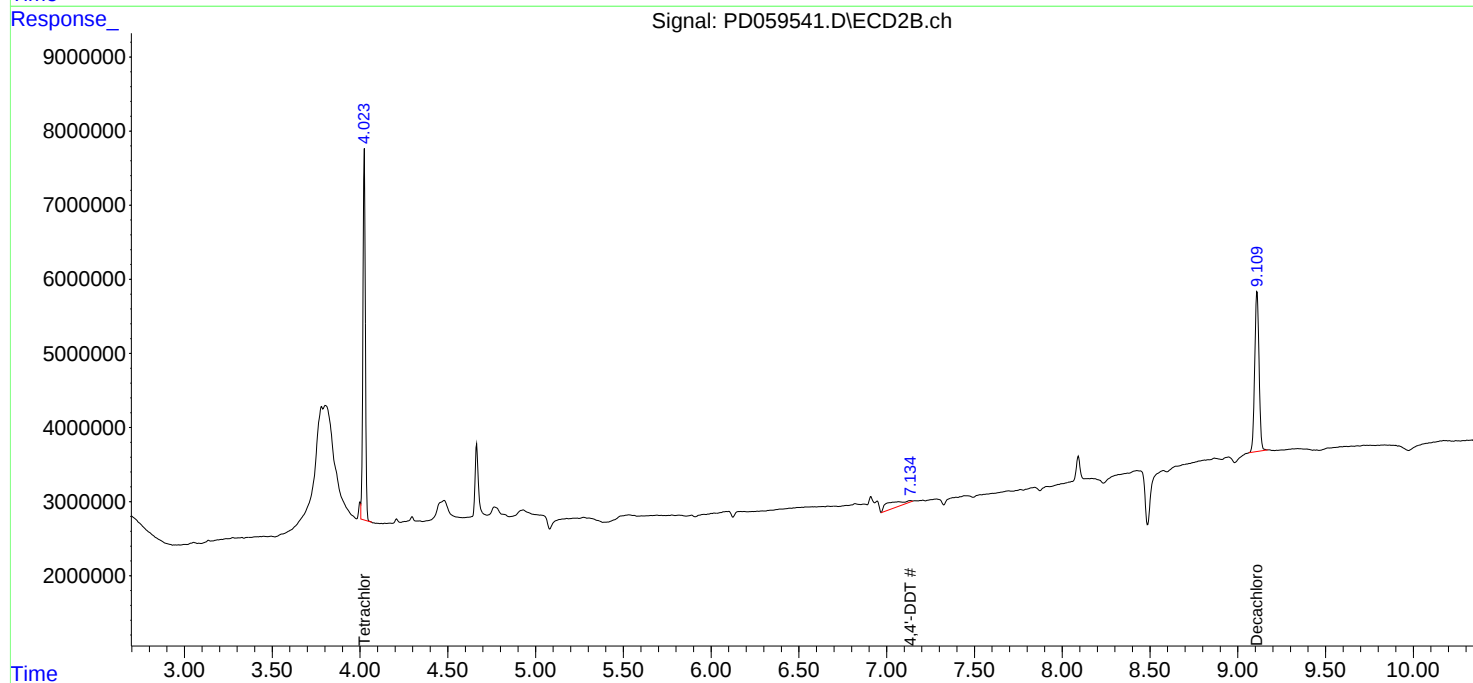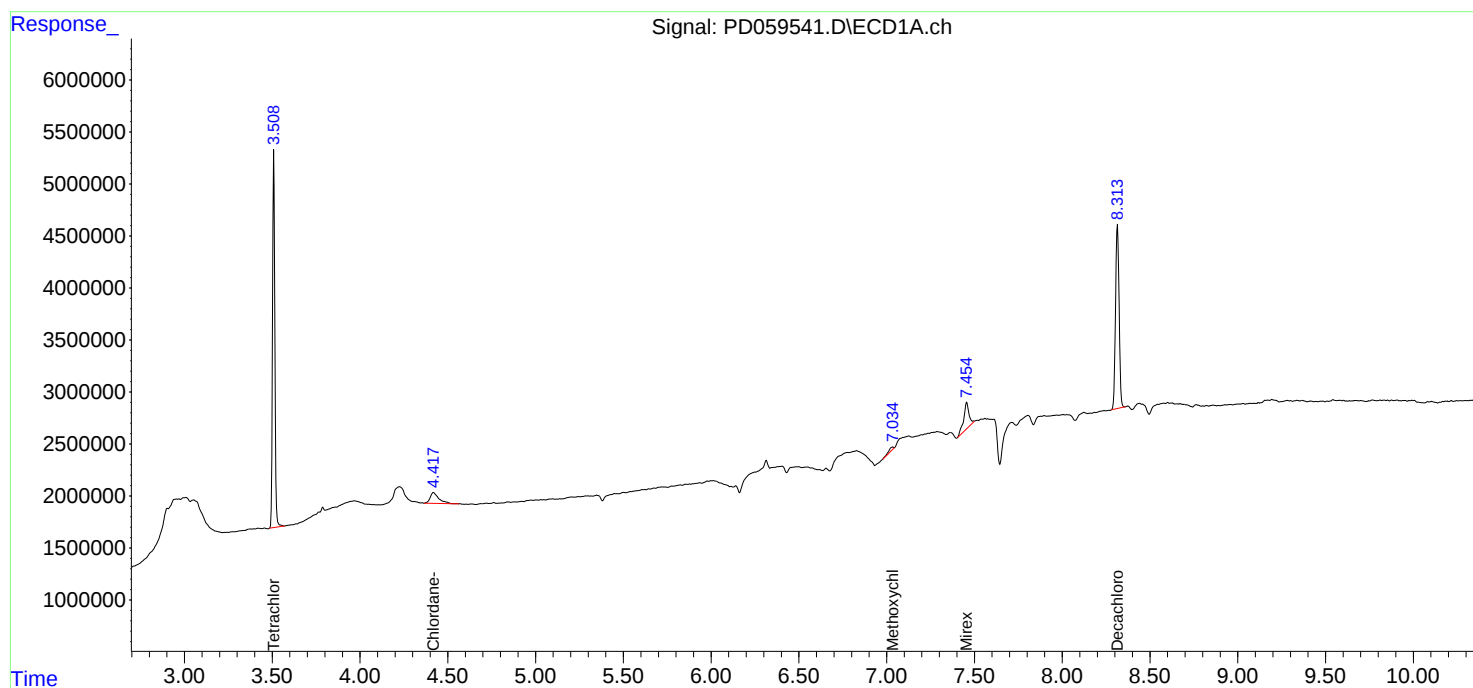


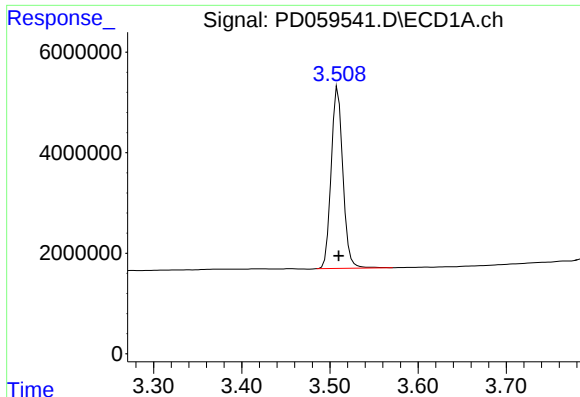

#1 Tetrachloro-m-xylene


R.T.: 3.509 min
Delta R.T.: 0.000 min
Response: 33417212
Conc: 23.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

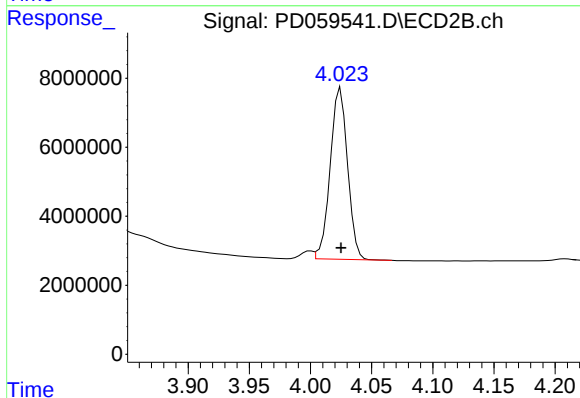


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 49036770
Conc: 22.56 ng/ml

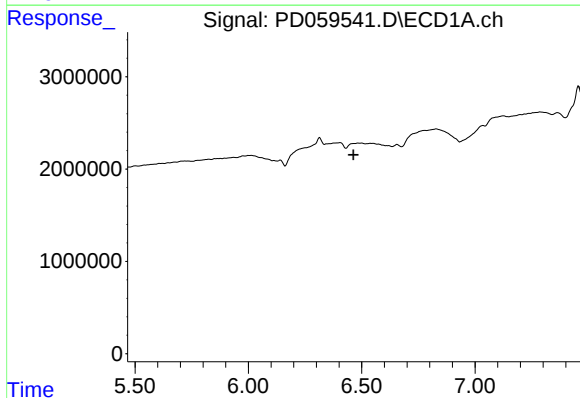


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.464 min
Response: 0
Conc: N.D.

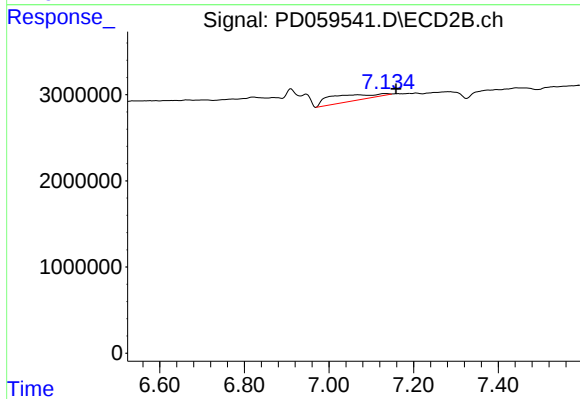

#17 4,4'-DDT


R.T.: 7.136 min
Delta R.T.: -0.023 min
Response: 5793576
Conc: 2.96 ng/ml

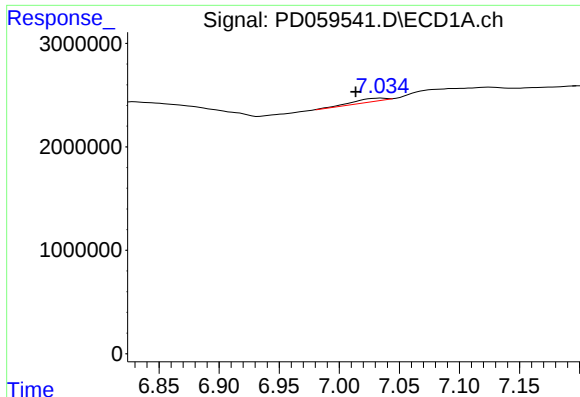

#20 Methoxychlor


R.T.: 7.035 min
Delta R.T.: 0.022 min
Response: 567195
Conc: 0.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

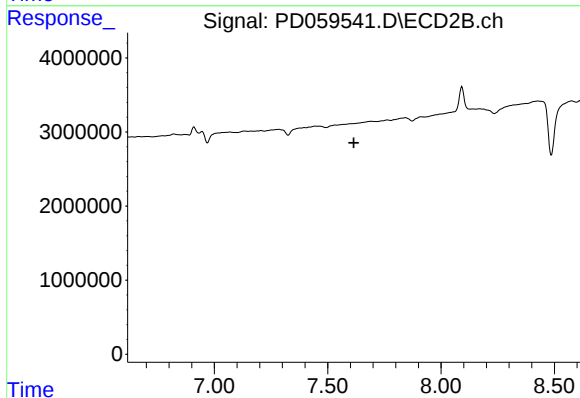


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.616 min
Response: 0
Conc: N.D.

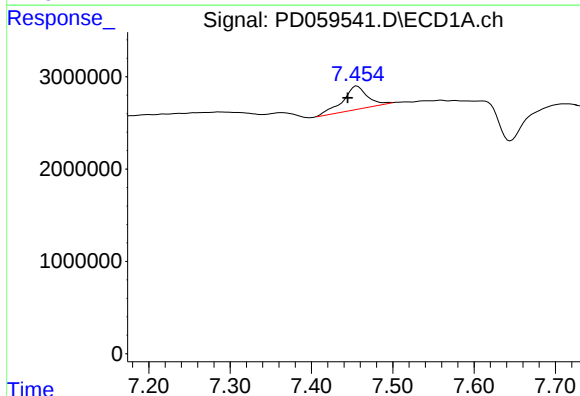


#22 Mirex

R.T.: 7.456 min
Delta R.T.: 0.012 min
Response: 5549760
Conc: 0.27 ng/ml

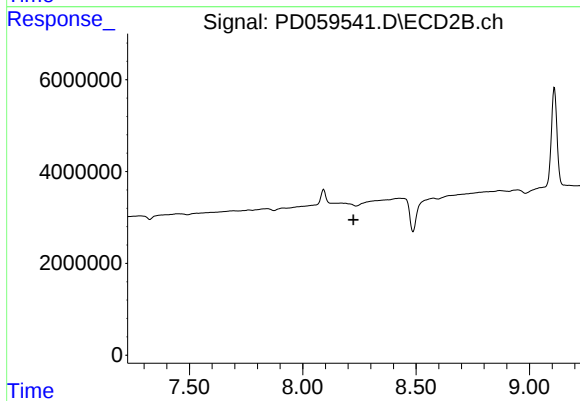

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.224 min
Response: 0
Conc: N.D.

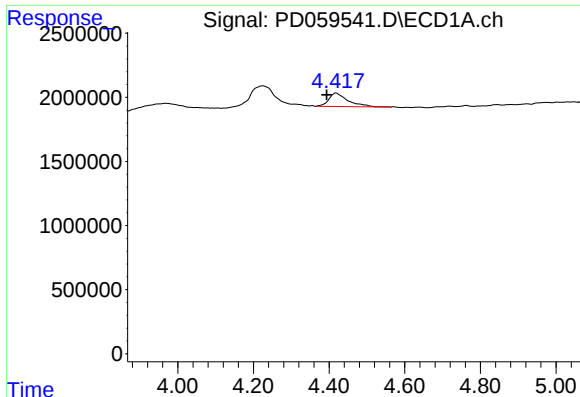

#23 Chlordane-1


R.T.: 4.418 min
Delta R.T.: 0.024 min
Response: 3664148
Conc: 70.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

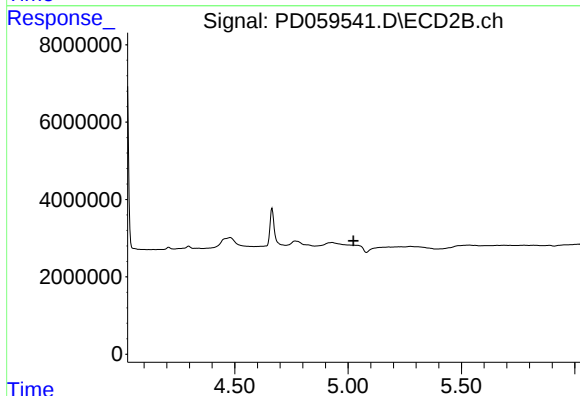


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.024 min
Response: 0
Conc: N.D.

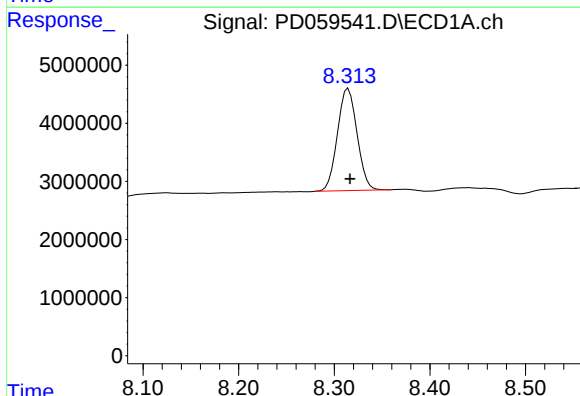

#28 Decachlorobiphenyl

R.T.: 8.315 min
Delta R.T.: -0.002 min
Response: 25115387
Conc: 22.61 ng/ml

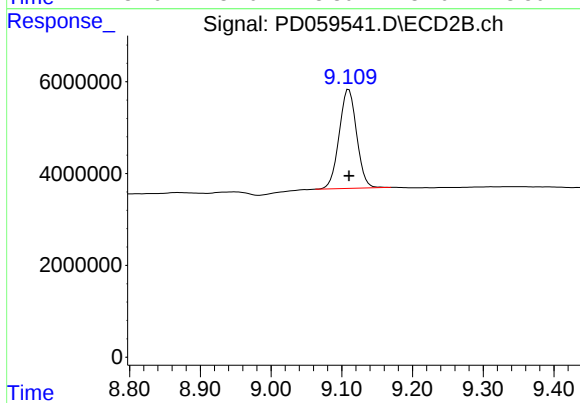

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 37146502
Conc: 23.05 ng/ml