

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
 Data File : PD059549.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2020 11:50
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 13:03:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:03:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.510	4.025	85300382	105.0E6	50.000	50.000
28)	SA Decachlor...	8.316	9.111	53508686	77495473	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.394	5.024	25977268	42483174	500.000	500.000
24)	Chlordane-2	4.901	5.493	26372229	39753853	500.000	500.000
25)	Chlordane-3	5.478	6.140	79049613	157.8E6	500.000	500.000
26)	Chlordane-4	5.536	6.216	63372375	187.9E6	500.000	500.000
27)	Chlordane-5	6.380	7.022	26362358	33106312	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
Data File : PD059549.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2020 11:50
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 13:03:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:03:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

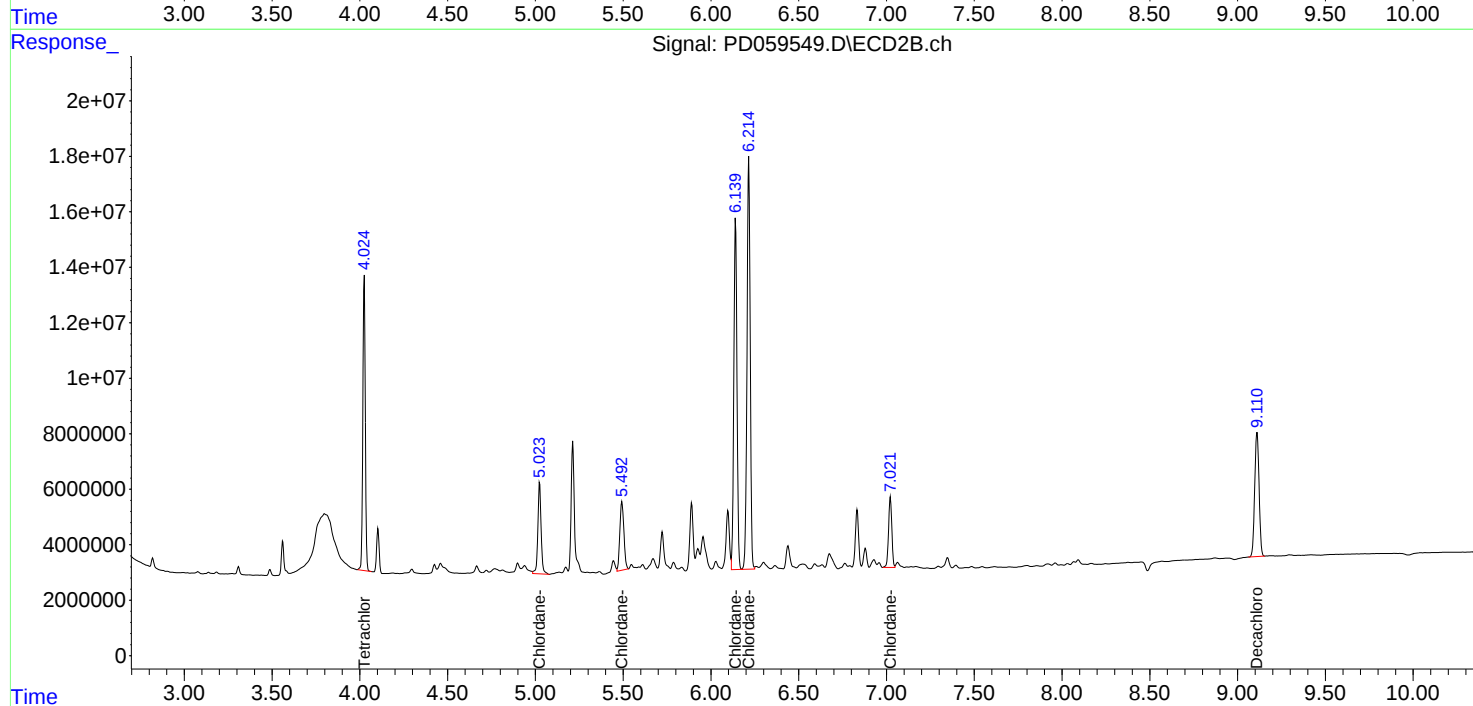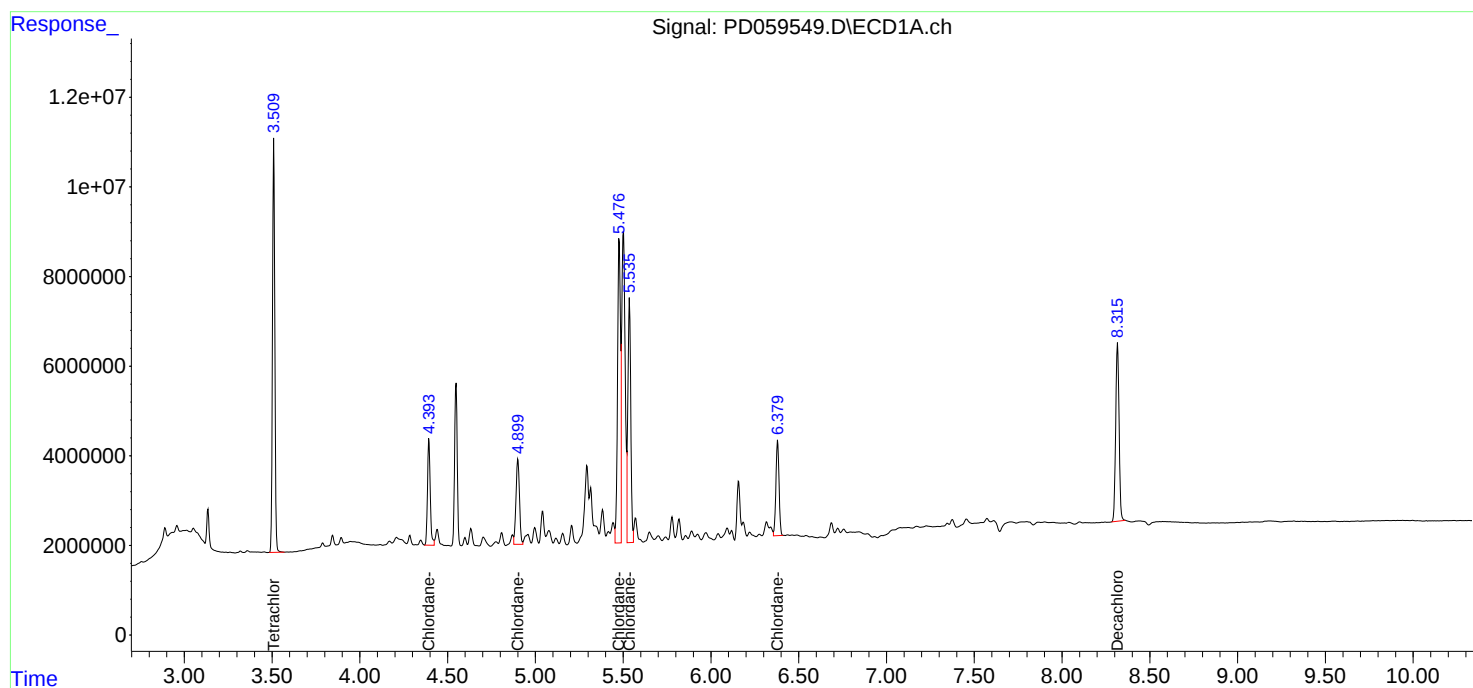


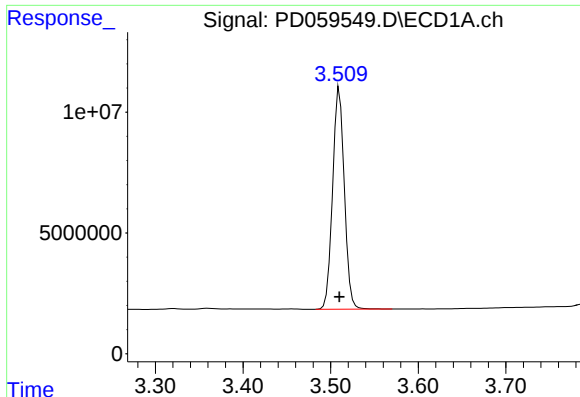

#1 Tetrachloro-m-xylene


R.T.: 3.510 min
Delta R.T.: 0.000 min
Response: 85300382
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

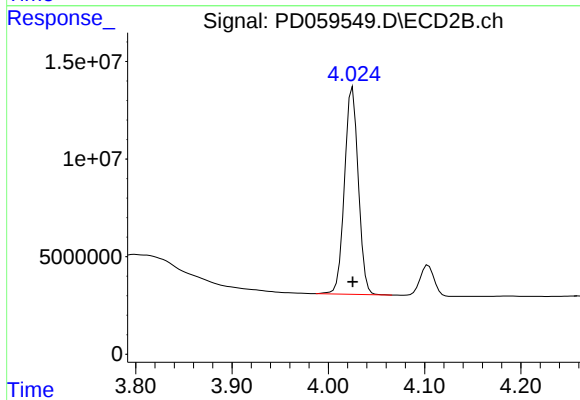


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 105002134
Conc: 50.00 ng/ml

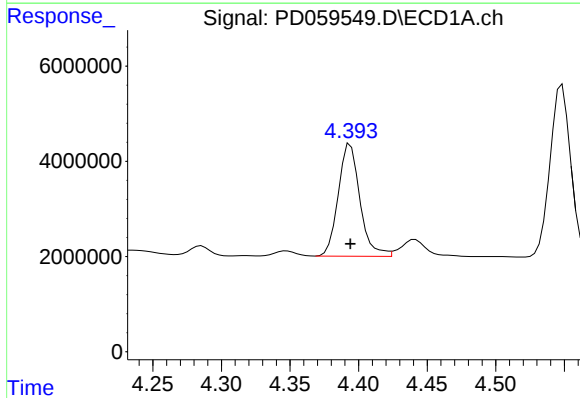


#23 Chlordane-1

R.T.: 4.394 min
Delta R.T.: 0.000 min
Response: 25977268
Conc: 500.00 ng/ml

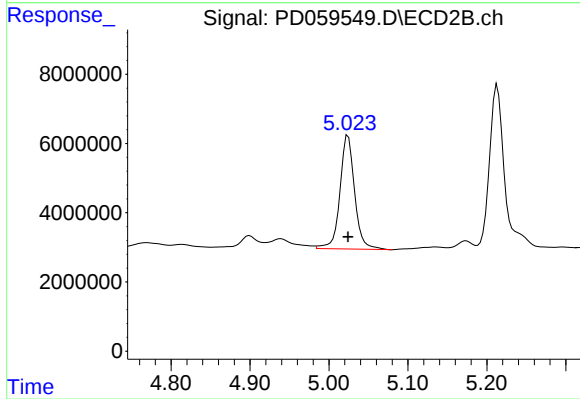

#23 Chlordane-1


R.T.: 5.024 min
Delta R.T.: 0.000 min
Response: 42483174
Conc: 500.00 ng/ml

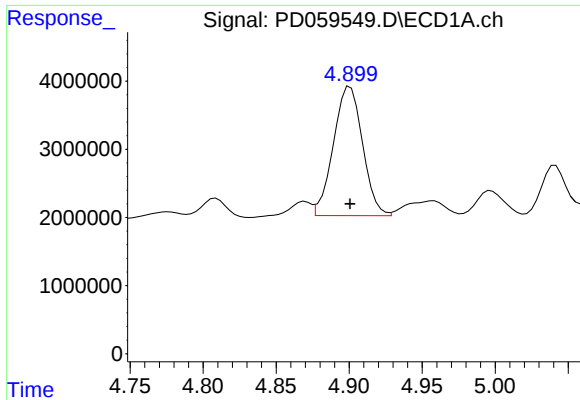

#24 Chlordane-2


R.T.: 4.901 min
Delta R.T.: 0.000 min
Response: 26372229
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

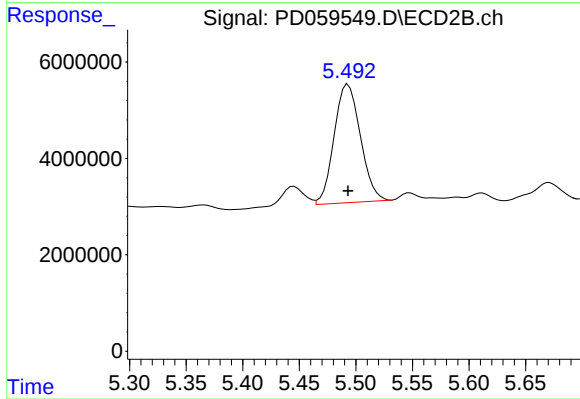


#24 Chlordane-2

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 39753853
Conc: 500.00 ng/ml

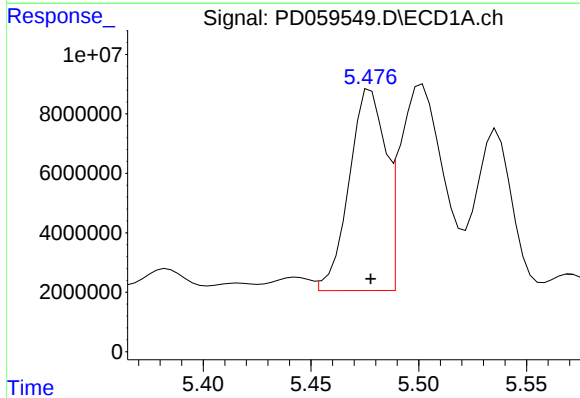


#25 Chlordane-3

R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 79049613
Conc: 500.00 ng/ml

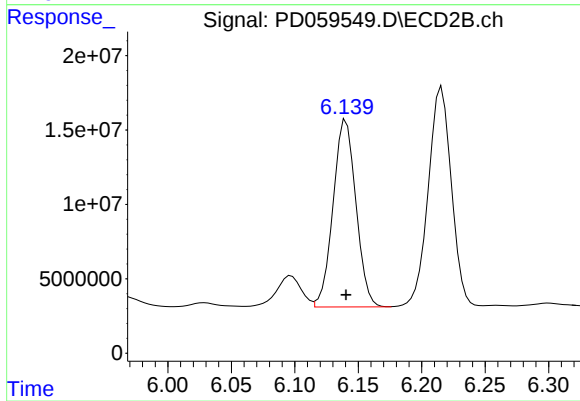

#25 Chlordane-3


R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 157774360
Conc: 500.00 ng/ml

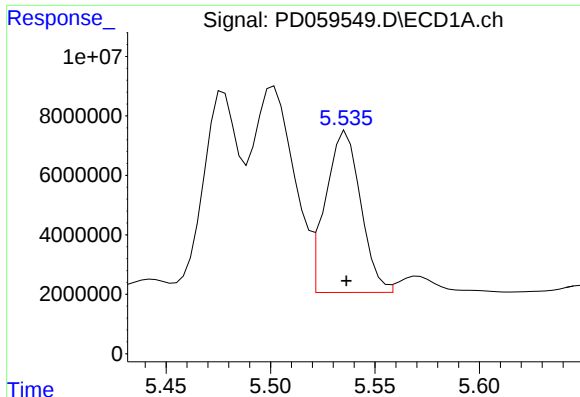

#26 Chlordane-4


R.T.: 5.536 min
Delta R.T.: 0.000 min
Response: 63372375
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

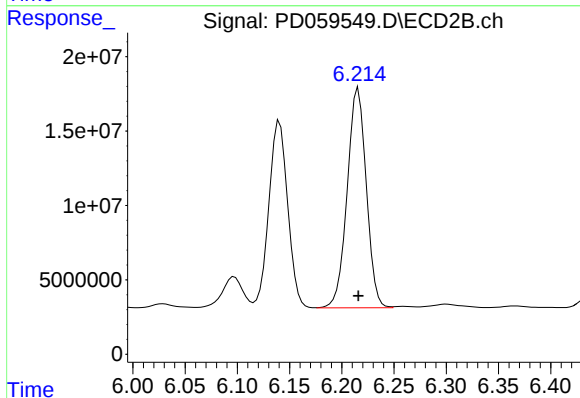


#26 Chlordane-4

R.T.: 6.216 min
Delta R.T.: 0.000 min
Response: 187886276
Conc: 500.00 ng/ml

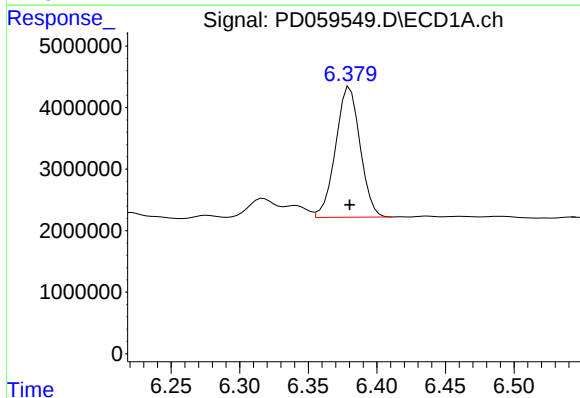


#27 Chlordane-5

R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 26362358
Conc: 500.00 ng/ml

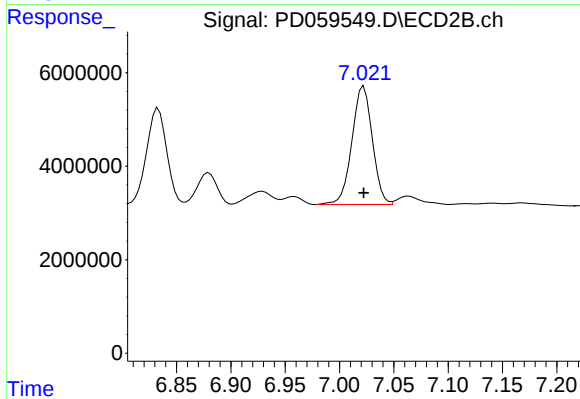

#27 Chlordane-5


R.T.: 7.022 min
Delta R.T.: 0.000 min
Response: 33106312
Conc: 500.00 ng/ml

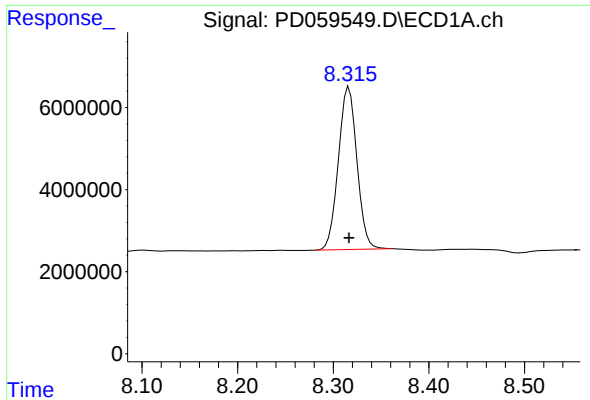

#28 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 53508686
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

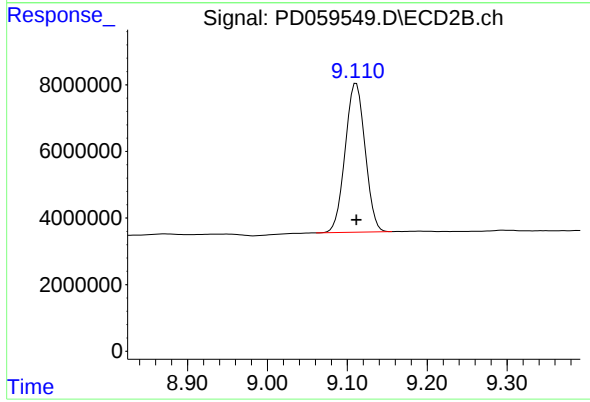

#28 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 77495473
Conc: 50.00 ng/ml