

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
 Data File : PD059559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2020 14:14
 Operator : DD\AJ
 Sample : L4225-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 06:05:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.511	4.026	19973159	26003183	13.853	11.961
28)	SA Decachlor...	8.317	9.112	12156769	16485736	10.943	10.231
Target Compounds							
12)	B 4,4'-DDE	5.700	6.370	1753140	2250910	1.034	0.948
16)	A 4,4'-DDD	6.222	0.000	393180	0	0.281	N.D. #
23)	Chlordane-1	0.000	5.026	0	1000457	N.D.	11.775 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
Data File : PD059559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2020 14:14
Operator : DD\AJ
Sample : L4225-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 06:05:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

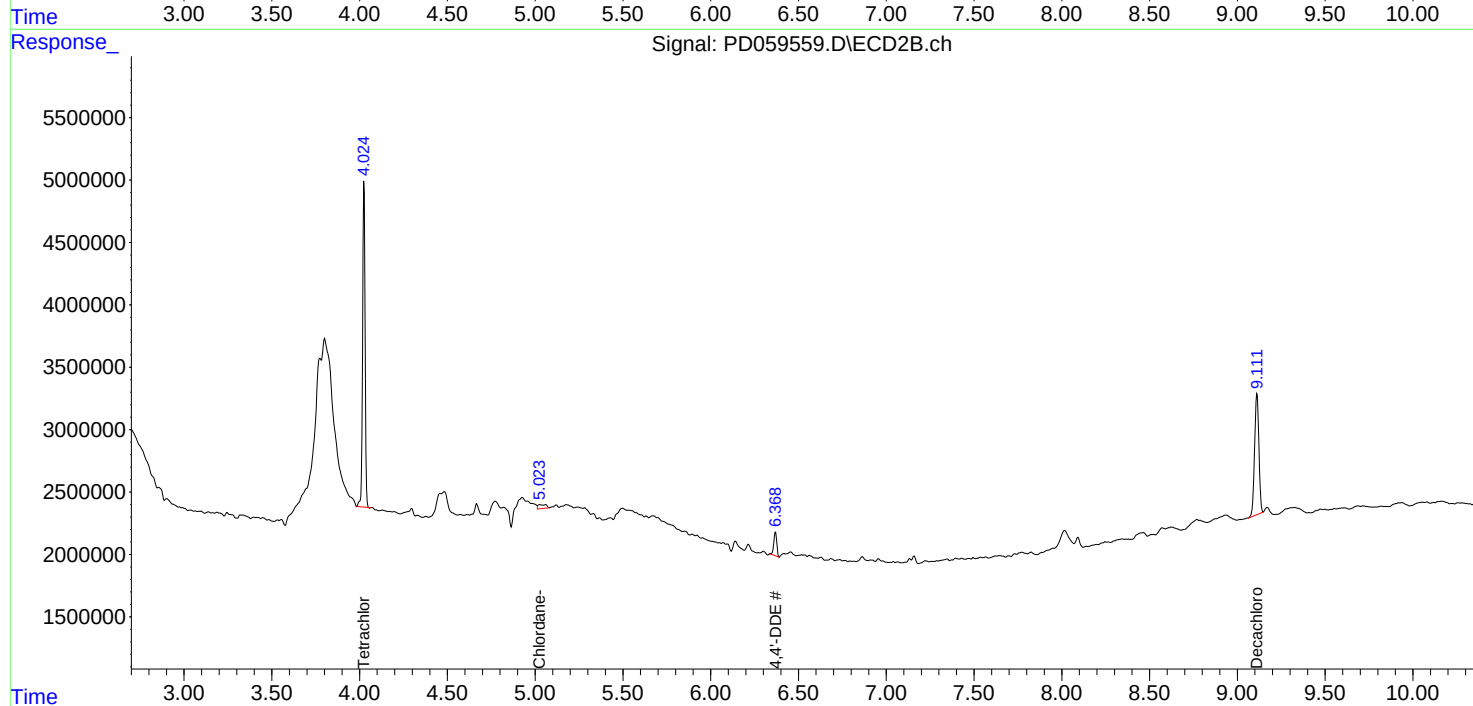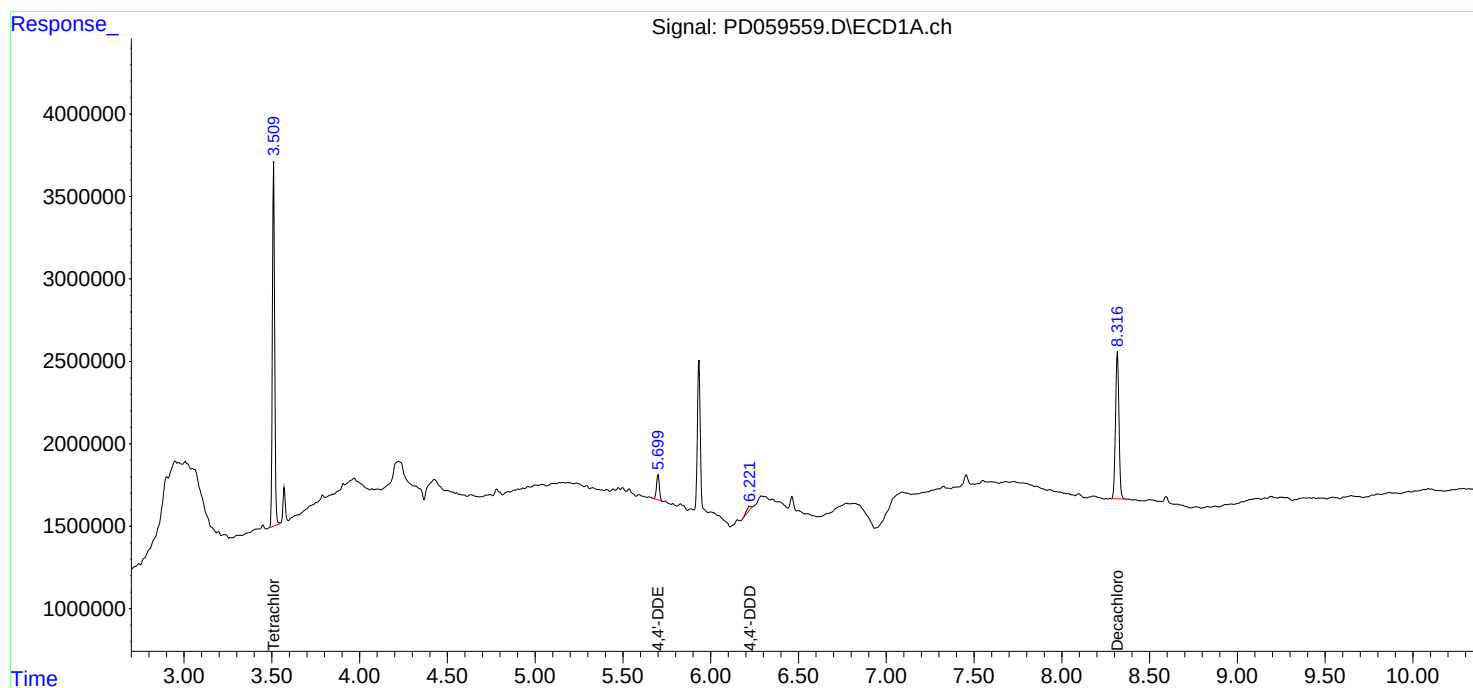


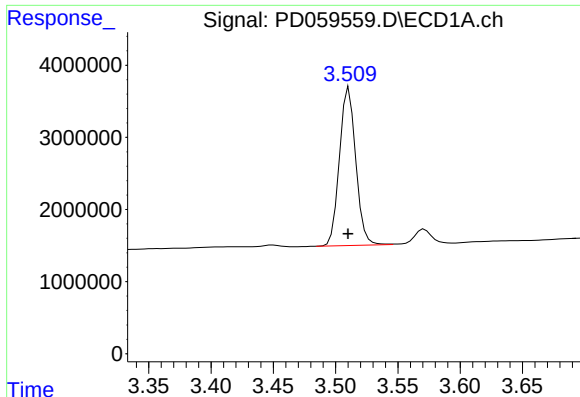

#1 Tetrachloro-m-xylene


R.T.: 3.511 min
Delta R.T.: 0.000 min
Response: 19973159
Conc: 13.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

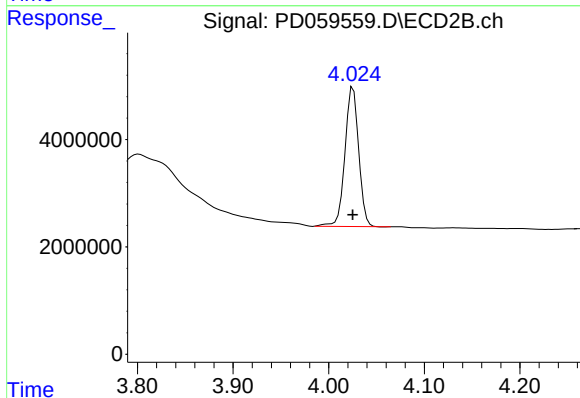


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 26003183
Conc: 11.96 ng/ml

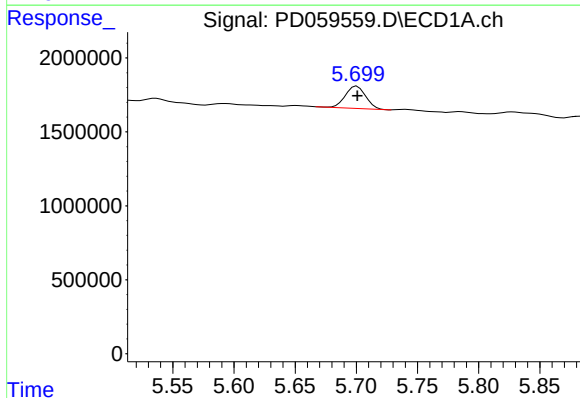


#12 4,4'-DDE

R.T.: 5.700 min
Delta R.T.: 0.000 min
Response: 1753140
Conc: 1.03 ng/ml

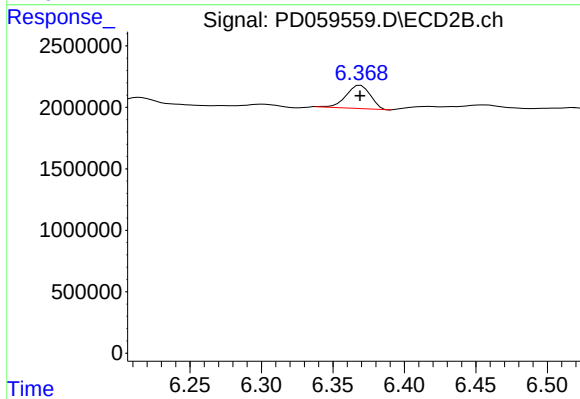

#12 4,4'-DDE


R.T.: 6.370 min
Delta R.T.: 0.000 min
Response: 2250910
Conc: 0.95 ng/ml

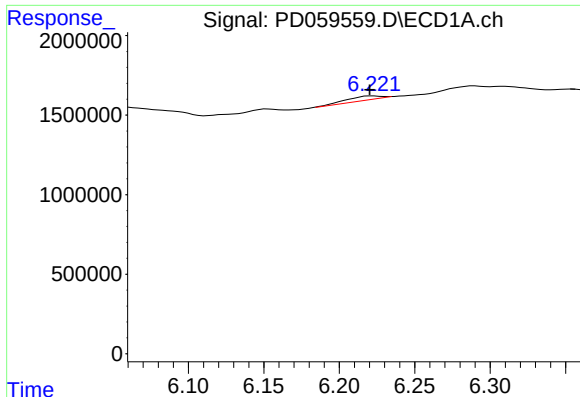

#16 4,4'-DDD


R.T.: 6.222 min
Delta R.T.: 0.002 min
Response: 393180
Conc: 0.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

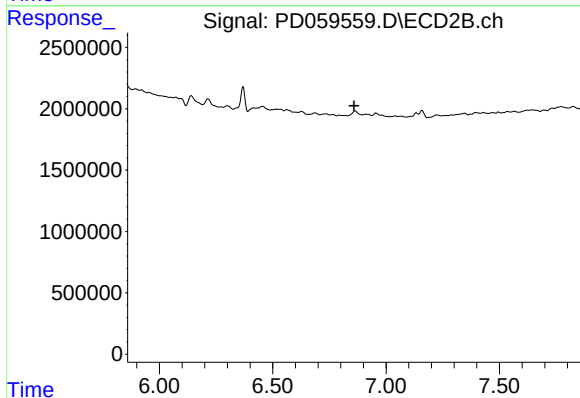


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.859 min
Response: 0
Conc: N.D.

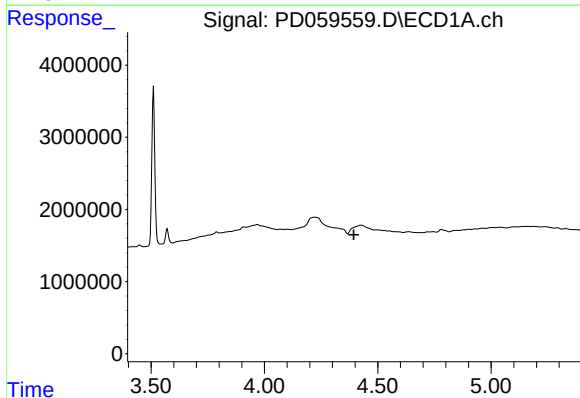


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.394 min
Response: 0
Conc: N.D.

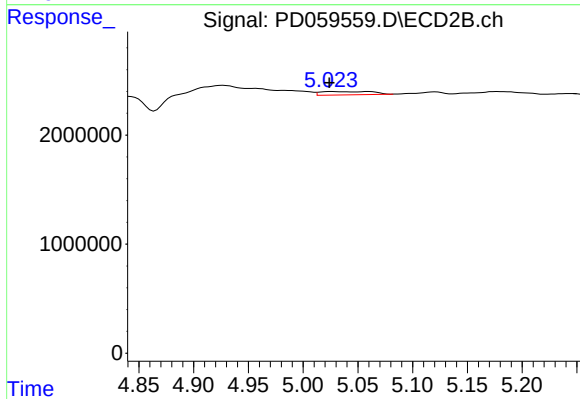

#23 Chlordane-1


R.T.: 5.026 min
Delta R.T.: 0.001 min
Response: 1000457
Conc: 11.77 ng/ml

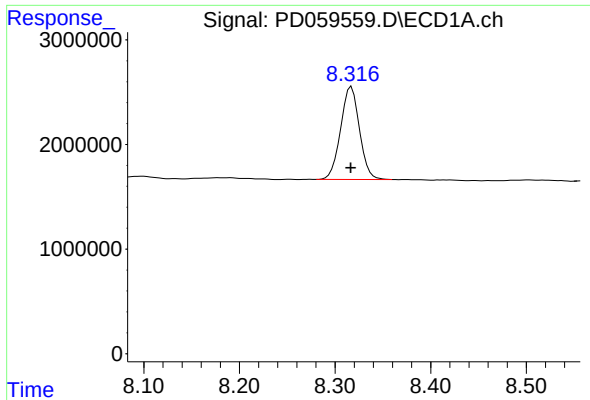

#28 Decachlorobiphenyl

R.T.: 8.317 min
Delta R.T.: 0.000 min
Response: 12156769
Conc: 10.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

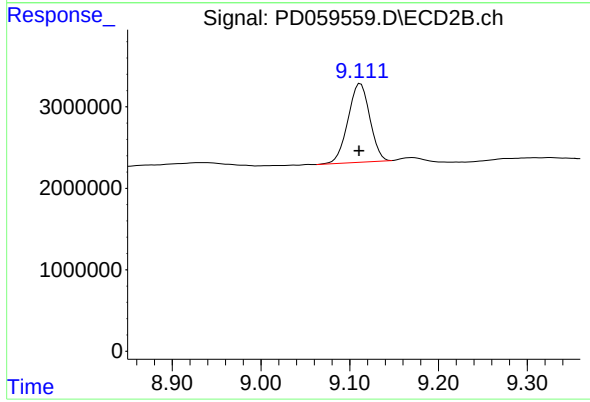

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.002 min
Response: 16485736
Conc: 10.23 ng/ml