

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
 Data File : PD059560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2020 14:28
 Operator : DD\AJ
 Sample : L4303-21
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 IDW-20201006

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 06:05:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.511	4.026	34923156	45340179	24.222	20.856
28)	SA Decachlor...	8.317	9.112	19463297	26624817	17.521	16.524
Target Compounds							
9)	A Endosulfan I	5.609f	0.000	1135574	0	0.702	N.D. #
23)	Chlordane-1	4.418f	0.000	1480588	0	28.498	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
Data File : PD059560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2020 14:28
Operator : DD\AJ
Sample : L4303-21
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
IDW-20201006

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 06:05:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

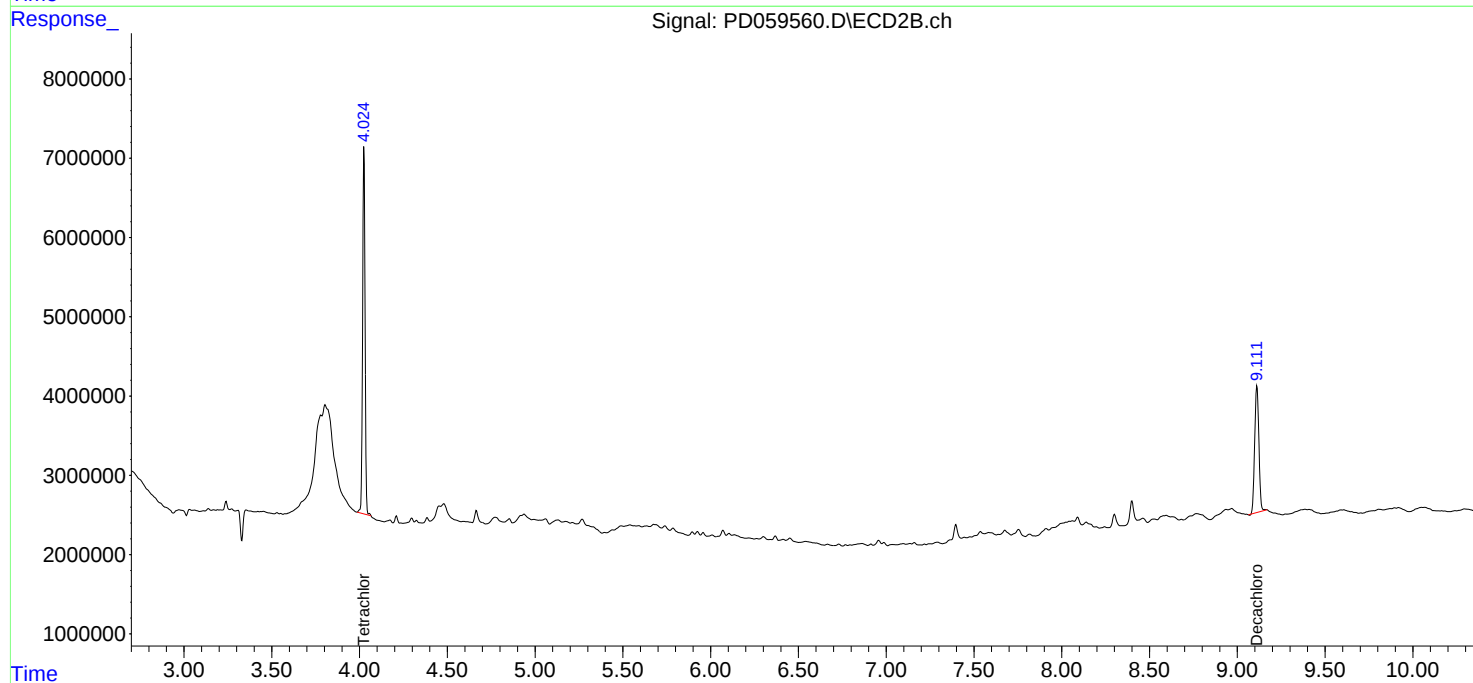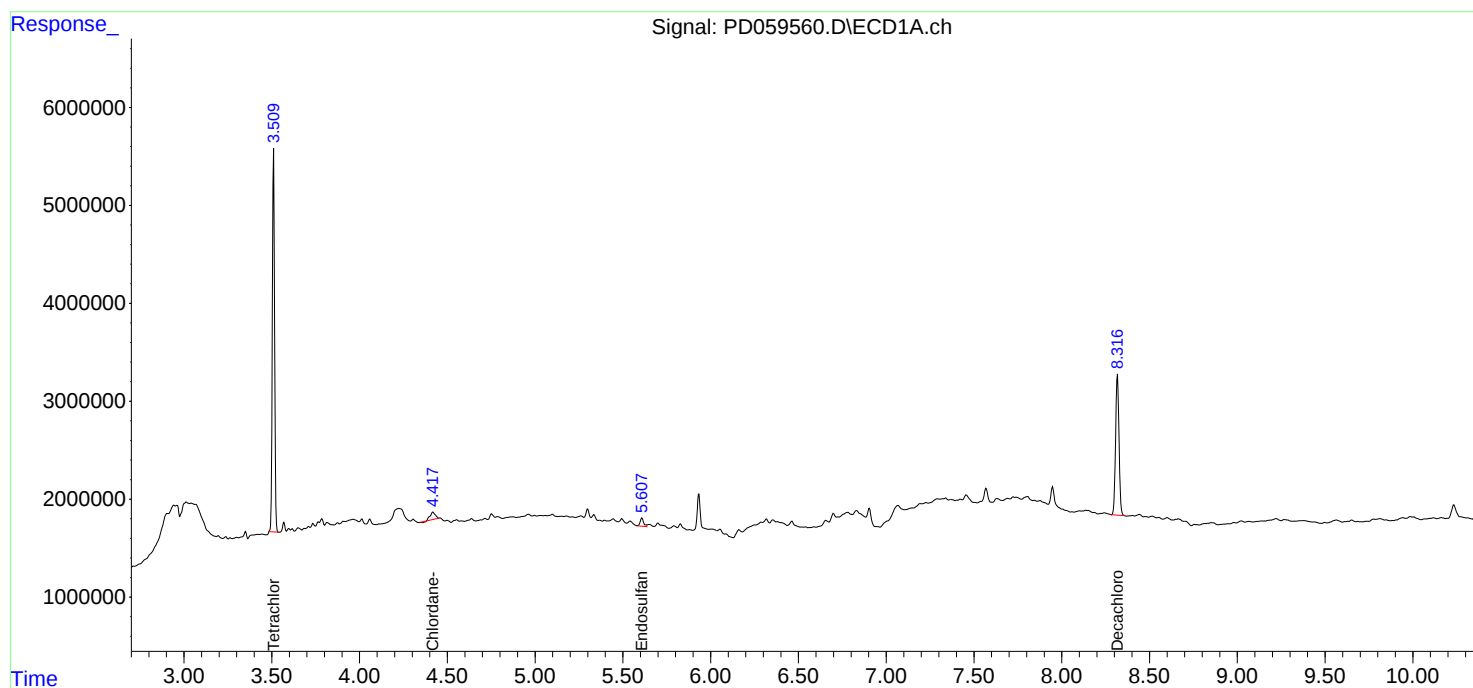


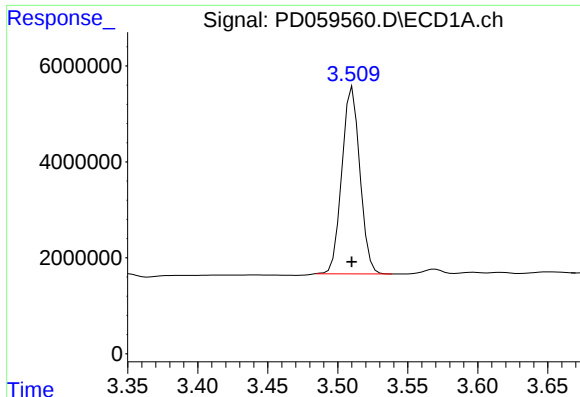

#1 Tetrachloro-m-xylene


R.T.: 3.511 min
Delta R.T.: 0.000 min
Response: 34923156
Conc: 24.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
IDW-20201006

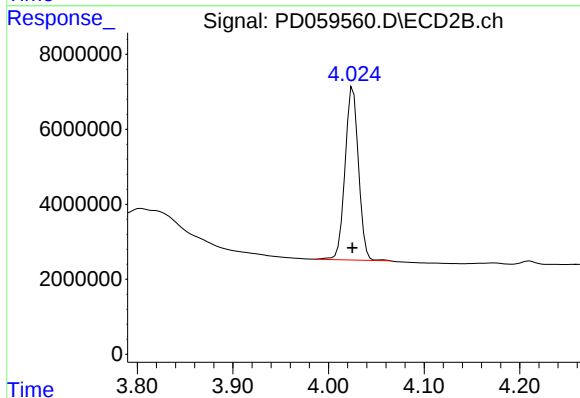


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 45340179
Conc: 20.86 ng/ml

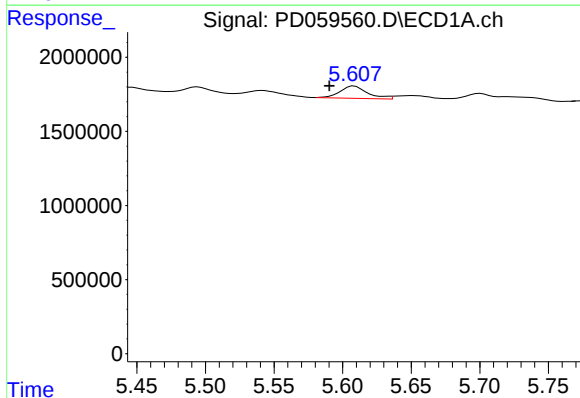


#9 Endosulfan I

R.T.: 5.609 min
Delta R.T.: 0.018 min
Response: 1135574
Conc: 0.70 ng/ml

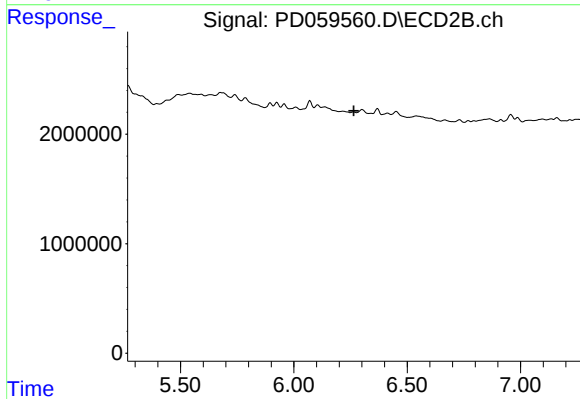

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.265 min
Response: 0
Conc: N.D.

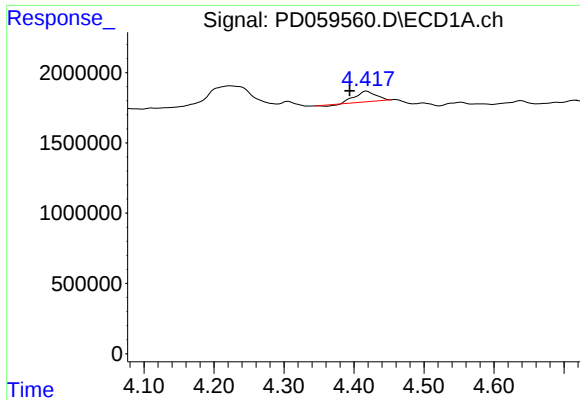

#23 Chlordane-1


R.T.: 4.418 min
Delta R.T.: 0.024 min
Response: 1480588
Conc: 28.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
IDW-20201006

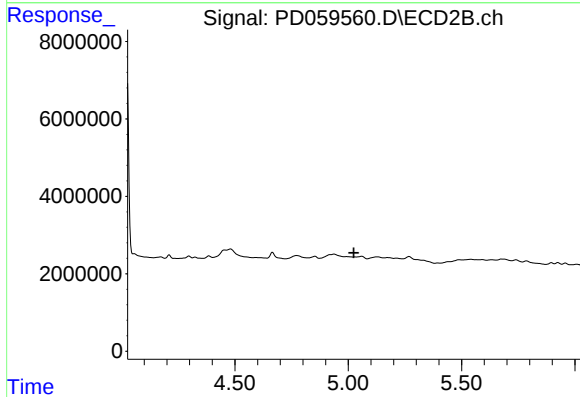


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.024 min
Response: 0
Conc: N.D.

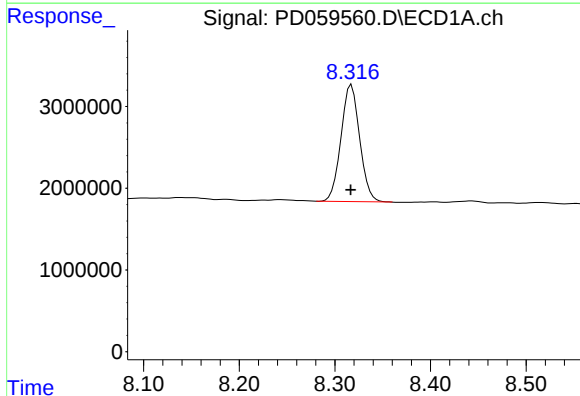

#28 Decachlorobiphenyl

R.T.: 8.317 min
Delta R.T.: 0.000 min
Response: 19463297
Conc: 17.52 ng/ml

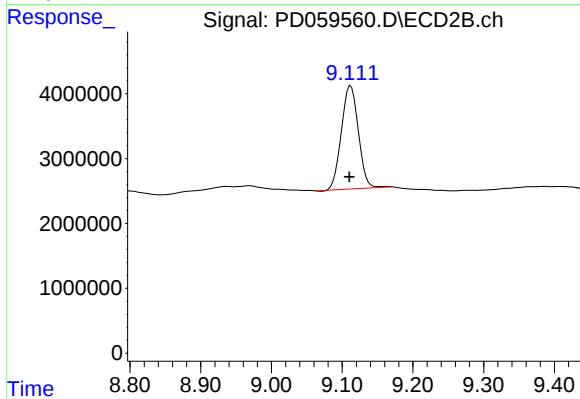

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.002 min
Response: 26624817
Conc: 16.52 ng/ml