

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
 Data File : PD059566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2020 16:18
 Operator : DD\AJ
 Sample : L4291-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PAV-B4-100620-10-20

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 06:06:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.518	4.026	21891875	33406021	15.184	15.366
28)	SA Decachlor...	8.325	9.115	13409859	19407182	12.072	12.044
Target Compounds							
6)	B beta-BHC	0.000	4.887f	0	2214326	N.D.	1.777 #
23)	Chlordane-1	4.394	0.000	2192405	0	42.199	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
Data File : PD059566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2020 16:18
Operator : DD\AJ
Sample : L4291-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PAV-B4-100620-10-20

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 06:06:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

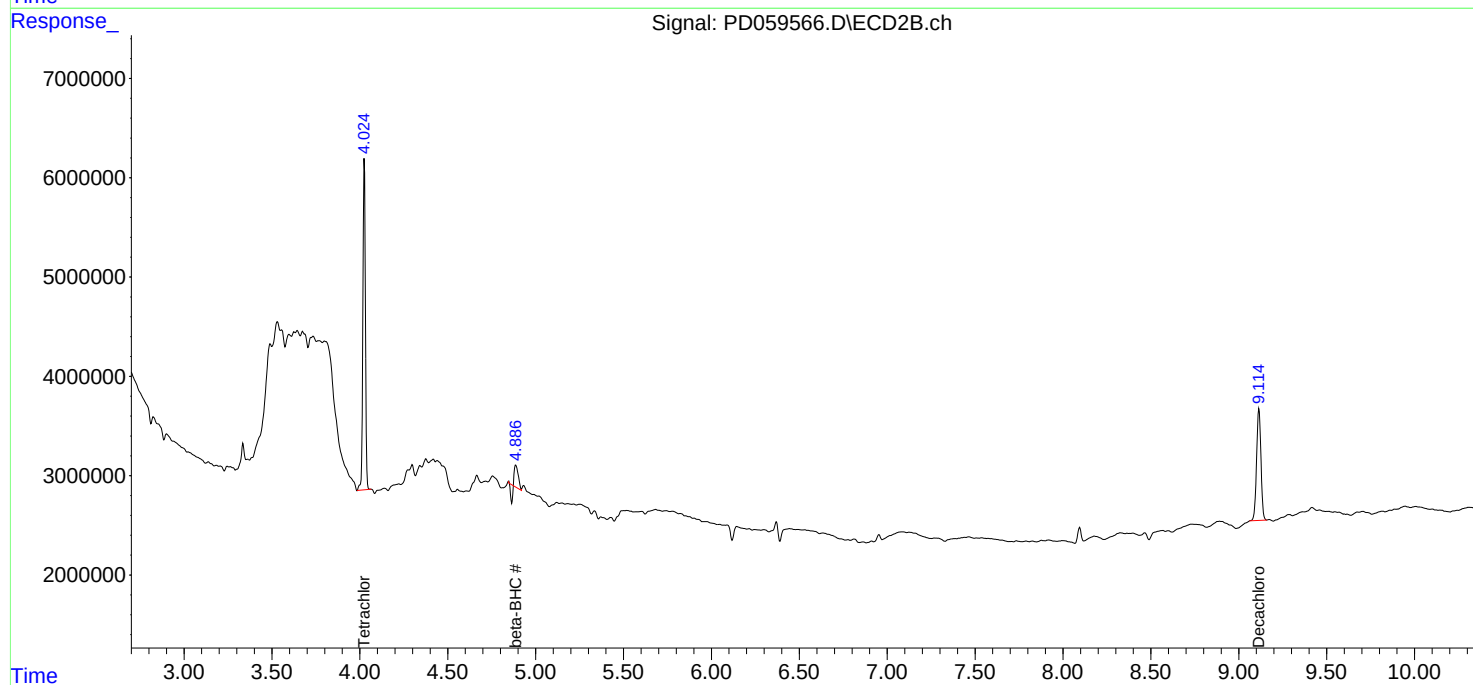


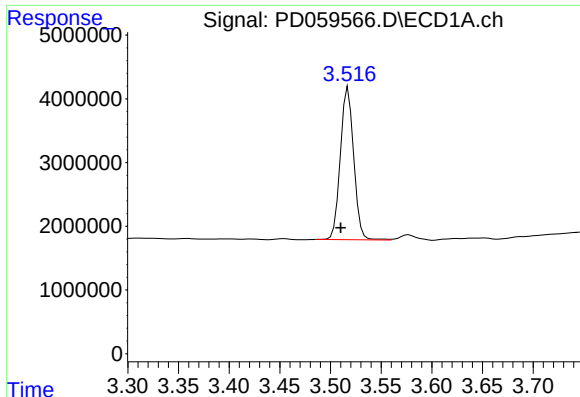

#1 Tetrachloro-m-xylene


R.T.: 3.518 min
Delta R.T.: 0.008 min
Response: 21891875
Conc: 15.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PAV-B4-100620-10-20

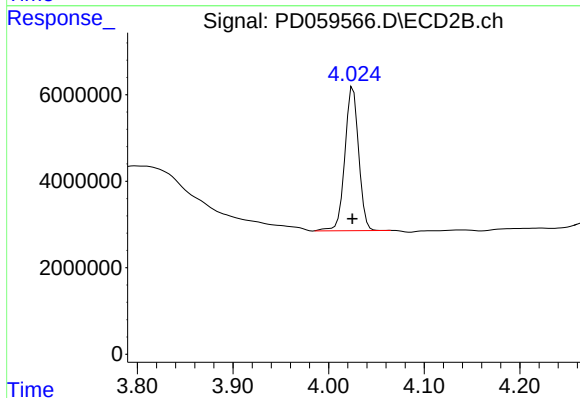


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 33406021
Conc: 15.37 ng/ml

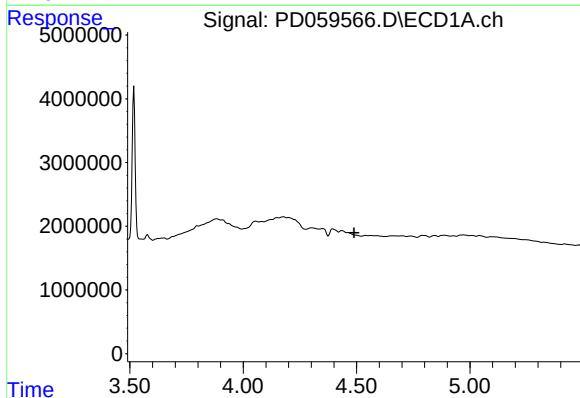


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.489 min
Response: 0
Conc: N.D.

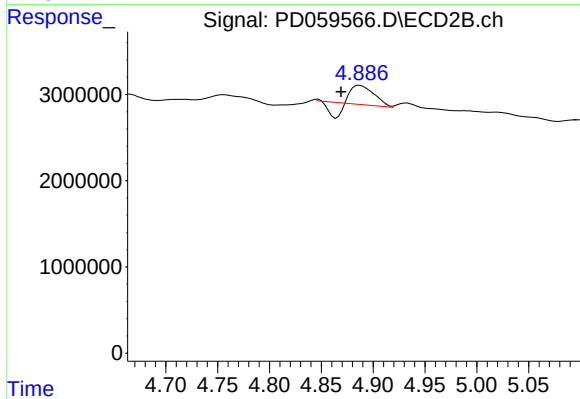

#6 beta-BHC


R.T.: 4.887 min
Delta R.T.: 0.018 min
Response: 2214326
Conc: 1.78 ng/ml

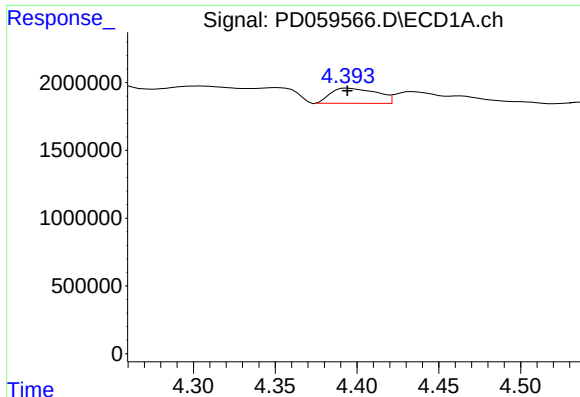

#23 Chlordane-1


R.T.: 4.394 min
Delta R.T.: 0.000 min
Response: 2192405
Conc: 42.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PAV-B4-100620-10-20

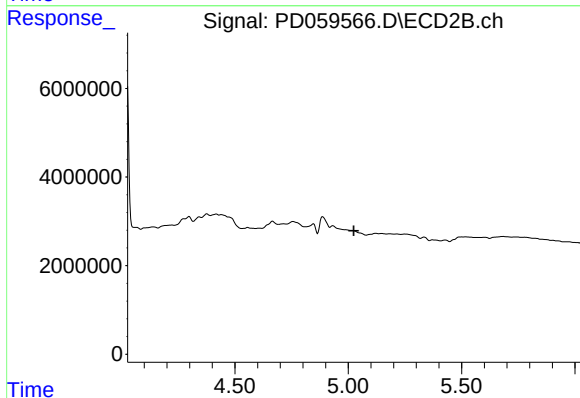


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.024 min
Response: 0
Conc: N.D.

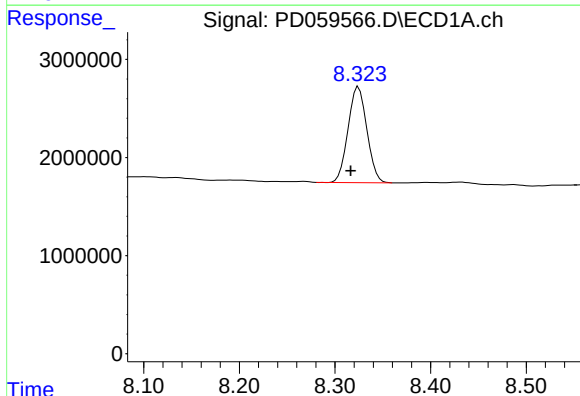

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: 0.008 min
Response: 13409859
Conc: 12.07 ng/ml

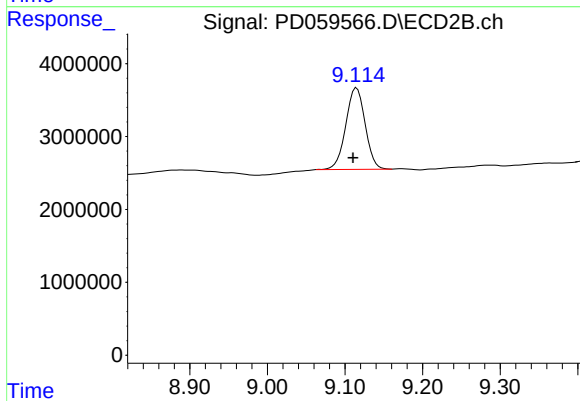

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.005 min
Response: 19407182
Conc: 12.04 ng/ml