

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
 Data File : PD059568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2020 16:46
 Operator : DD\AJ
 Sample : L4291-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PAV-B4-100620-0-10

Manual Integrations
 APPROVED

Ankita
 10/12/2020 9:15:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 06:06:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.510	4.025	20731368	30005256	14.379	13.802
28)	SA Decachlor...	8.316	9.111	13205624	17826475	11.888	11.063
Target Compounds							
12)	B 4,4'-DDE	5.701	6.366	3305844	3730526	1.949	1.571m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100820\
Data File : PD059568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2020 16:46
Operator : DD\AJ
Sample : L4291-03
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PAV-B4-100620-0-10


Manual Integrations
APPROVED

Ankita
10/12/2020 9:15:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 06:06:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

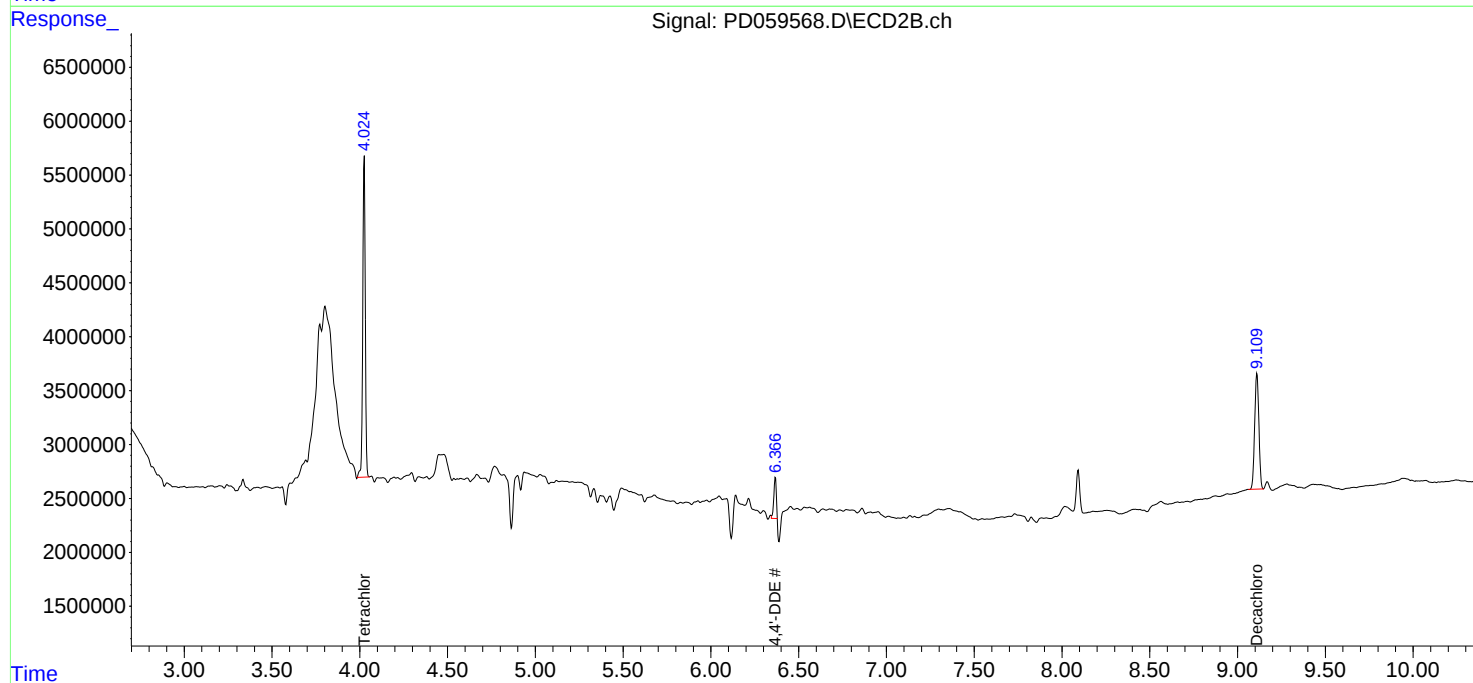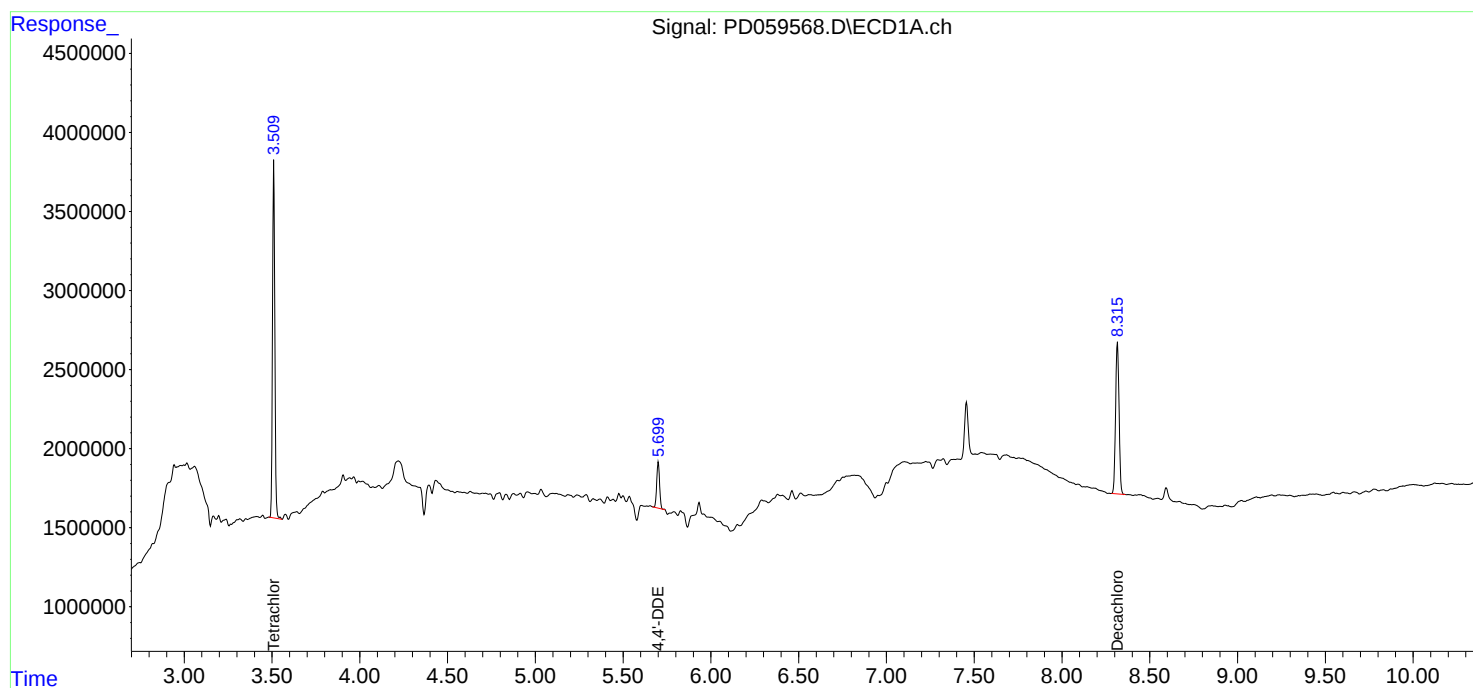

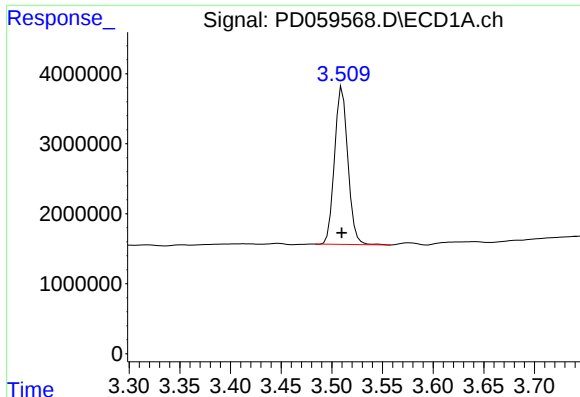


#1 Tetrachloro-m-xylene

R.T.: 3.510 min
Delta R.T.: 0.000 min
Response: 20731368
Conc: 14.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
PAV-B4-100620-0-10


Manual Integrations
APPROVED

Ankita
10/12/2020 9:15:53 AM

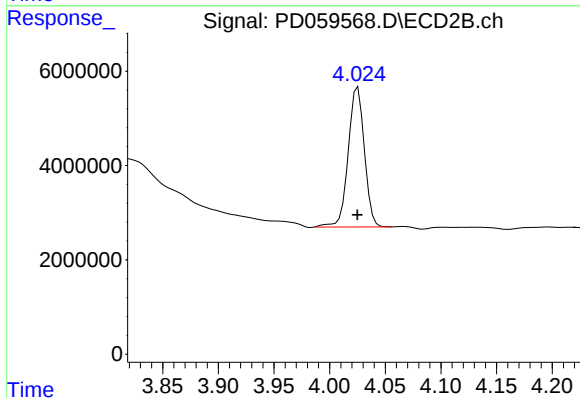


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 30005256
Conc: 13.80 ng/ml

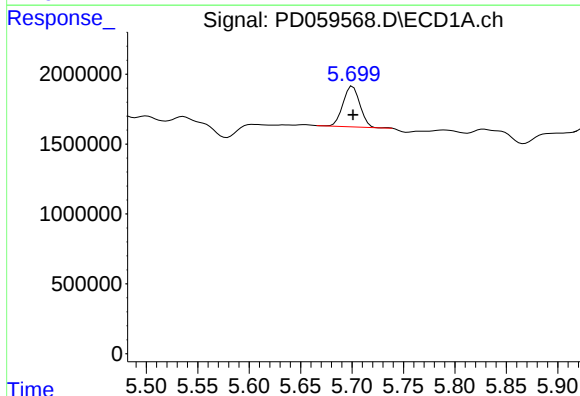


#12 4,4'-DDE

R.T.: 5.701 min
Delta R.T.: 0.000 min
Response: 3305844
Conc: 1.95 ng/ml

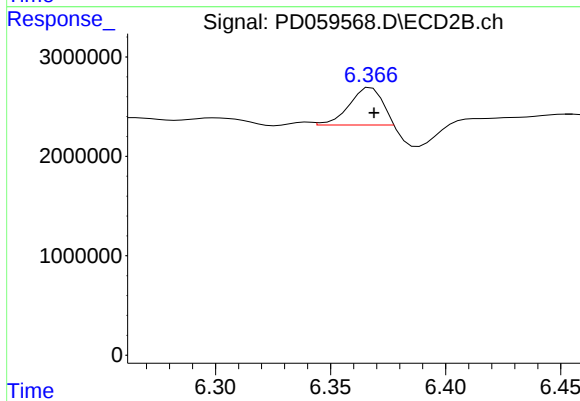

#12 4,4'-DDE

R.T.: 6.366 min
Delta R.T.: -0.003 min
Response: 3730526
Conc: 1.57 ng/ml m

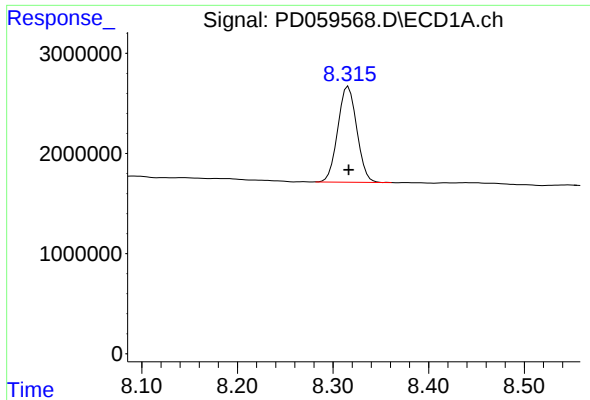


#28 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 13205624
Conc: 11.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PAV-B4-100620-0-10

Manual Integrations
APPROVED

Ankita
10/12/2020 9:15:53 AM

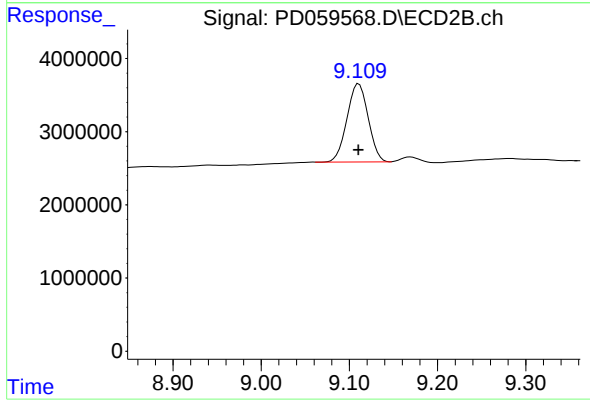

#28 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 17826475
Conc: 11.06 ng/ml