

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100821\
 Data File : PD066105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2021 11:38
 Operator : AR\AJ
 Sample : M4117-10DL 100X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-4(0-0.5)DL2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 01:17:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
12) B	4,4'-DDE	5.646	6.354	32047421	169.3E6	29.441 29.350
16) A	4,4'-DDD	6.161	6.848	2080679	13242573	2.121 2.695 #
17) MA	4,4'-DDT	6.401	7.146	67325009	300.6E6	61.166 59.511



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100821\
Data File : PD066105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2021 11:38
Operator : AR\AJ
Sample : M4117-10DL 100X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SB-4(0-0.5)DL2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 01:17:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

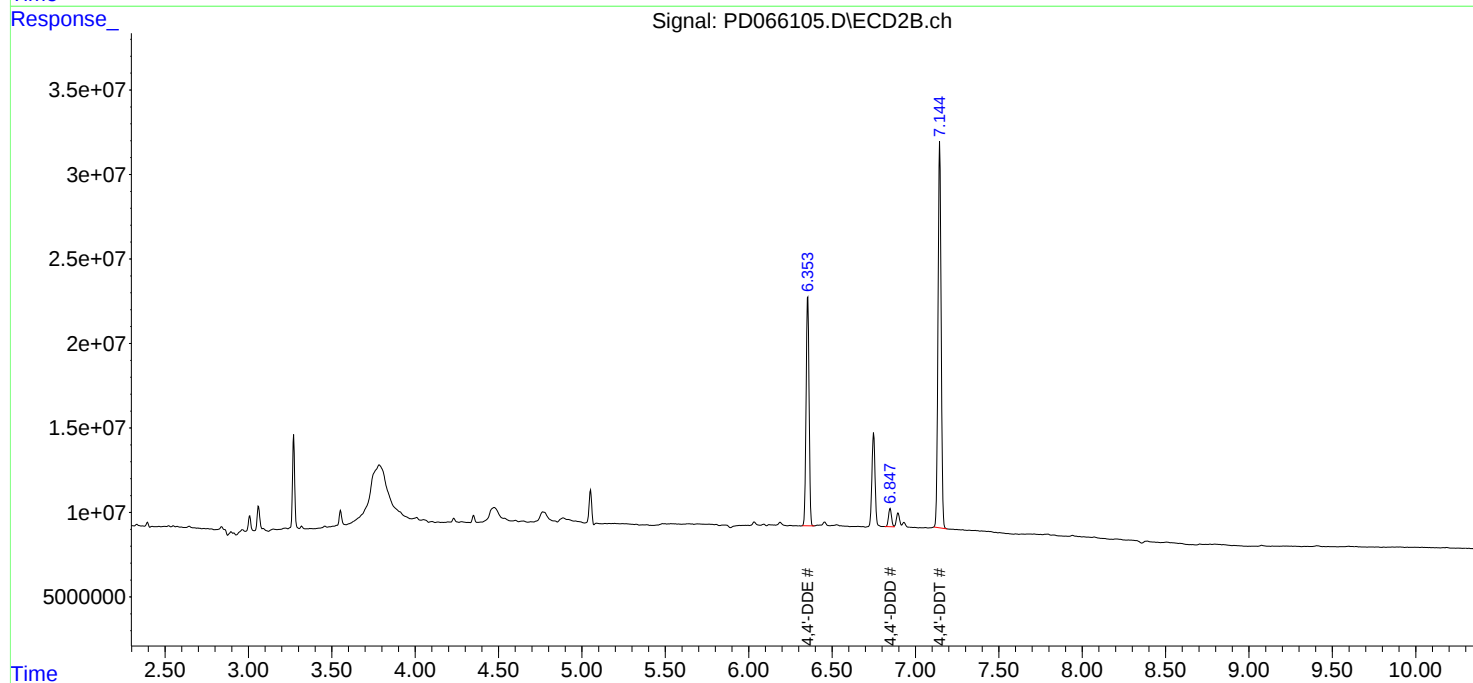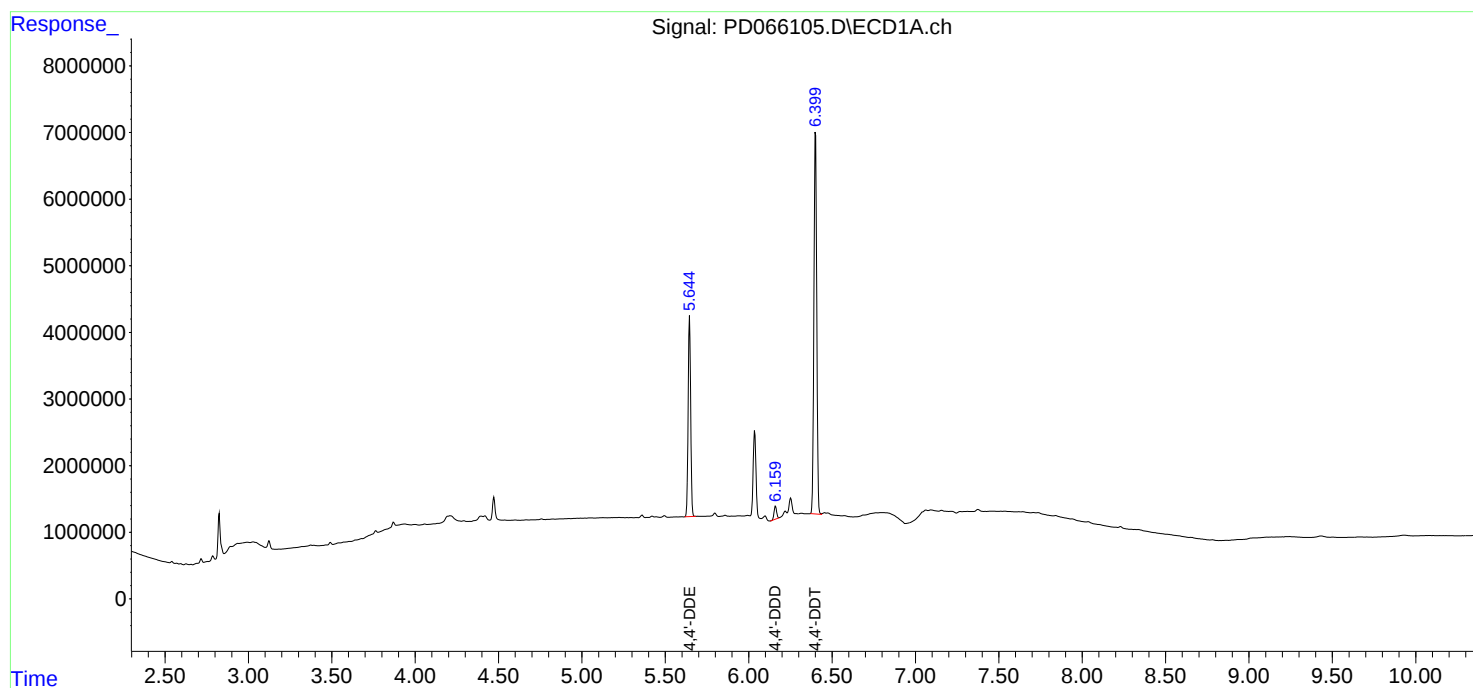


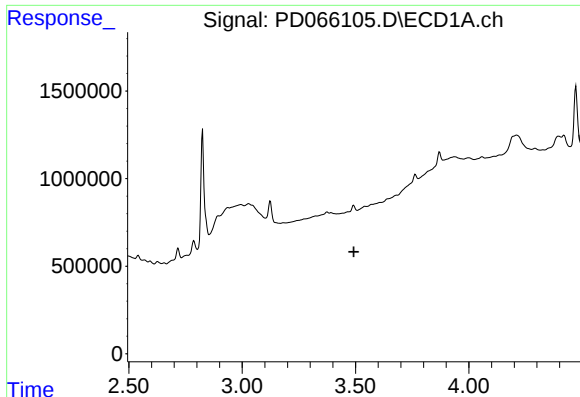

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.493 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SB-4(0-0.5)DL2

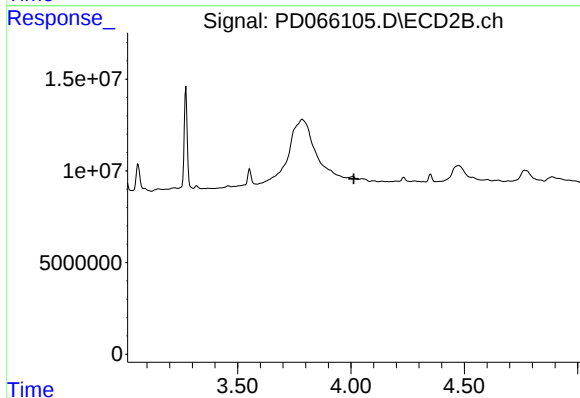


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.012 min
Response: 0
Conc: N.D.

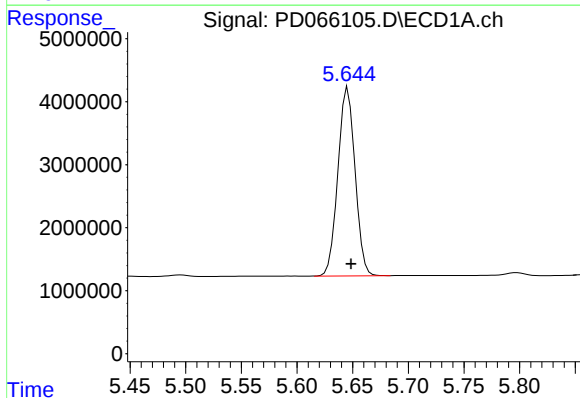


#12 4,4'-DDE

R.T.: 5.646 min
Delta R.T.: -0.003 min
Response: 32047421
Conc: 29.44 ng/ml

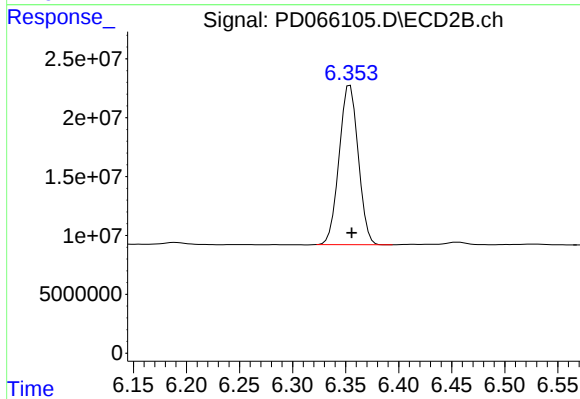

#12 4,4'-DDE


R.T.: 6.354 min
Delta R.T.: -0.001 min
Response: 169276690
Conc: 29.35 ng/ml

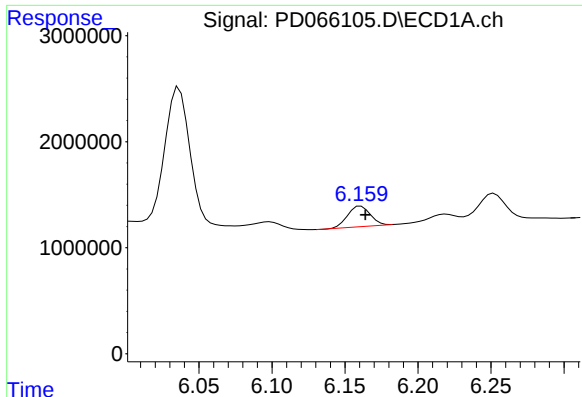

#16 4,4'-DDD


R.T.: 6.161 min
Delta R.T.: -0.003 min
Response: 2080679
Conc: 2.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-4(0-0.5)DL2

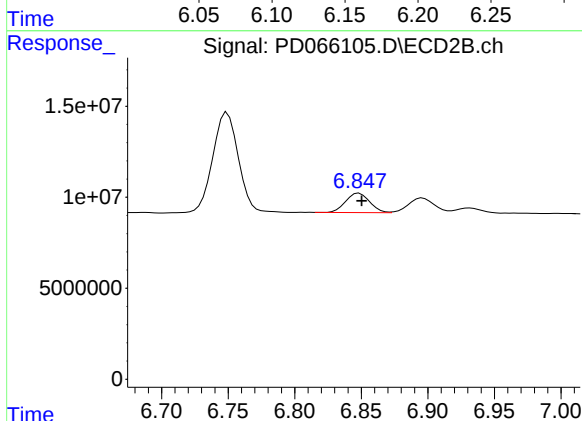


#16 4,4'-DDD

R.T.: 6.848 min
Delta R.T.: -0.002 min
Response: 13242573
Conc: 2.69 ng/ml

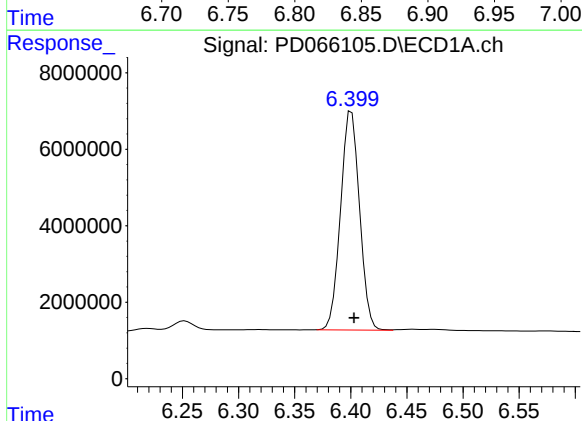


#17 4,4'-DDT

R.T.: 6.401 min
Delta R.T.: -0.002 min
Response: 67325009
Conc: 61.17 ng/ml

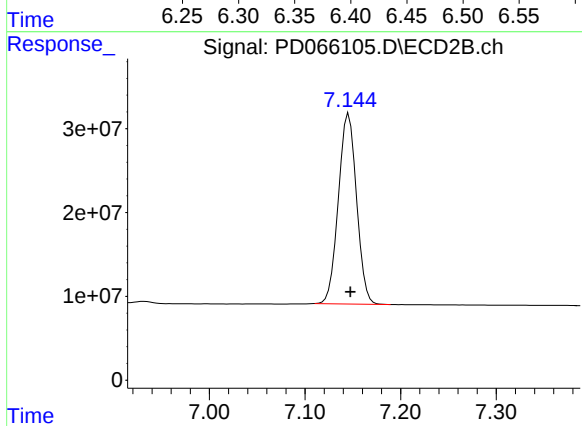

#17 4,4'-DDT


R.T.: 7.146 min
Delta R.T.: -0.002 min
Response: 300611437
Conc: 59.51 ng/ml

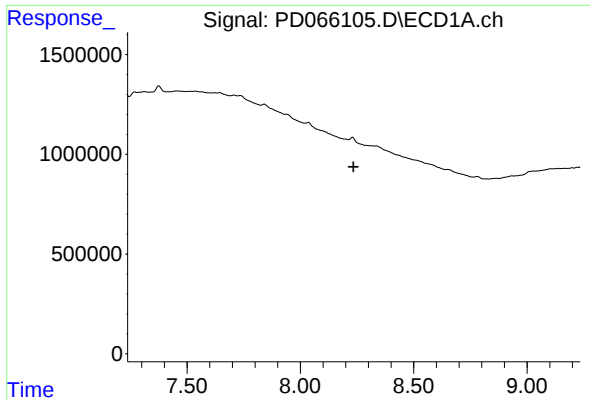

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.235 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SB-4(0-0.5)DL2

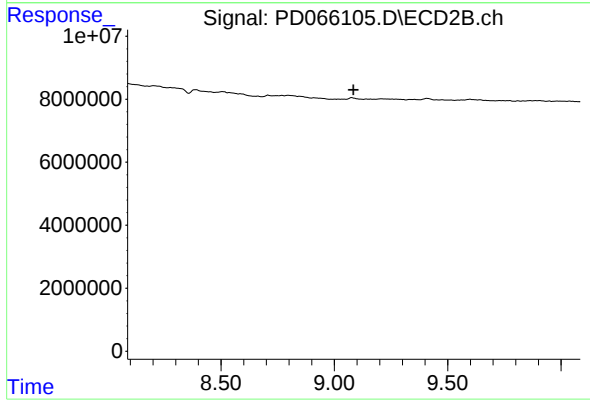

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.085 min
Response: 0
Conc: N.D.