

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100920\
 Data File : PD059615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2020 18:46
 Operator : DD\AJ
 Sample : L4291-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PAV-B4-100620-DP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:20:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.510	4.026	28806545	41121181	19.979	18.915
28) SA	Decachlor...	8.315	9.110	24327250	33461332	21.899	20.767
Target Compounds							
6) B	beta-BHC	4.458f	0.000	3925818	0	4.609	N.D. #
7) B	delta-BHC	0.000	5.063f	0	5845923	N.D.	2.126 #
23)	Chlordane-1	4.420f	0.000	2600303	0	50.050	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100920\
Data File : PD059615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2020 18:46
Operator : DD\AJ
Sample : L4291-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PAV-B4-100620-DP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:20:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

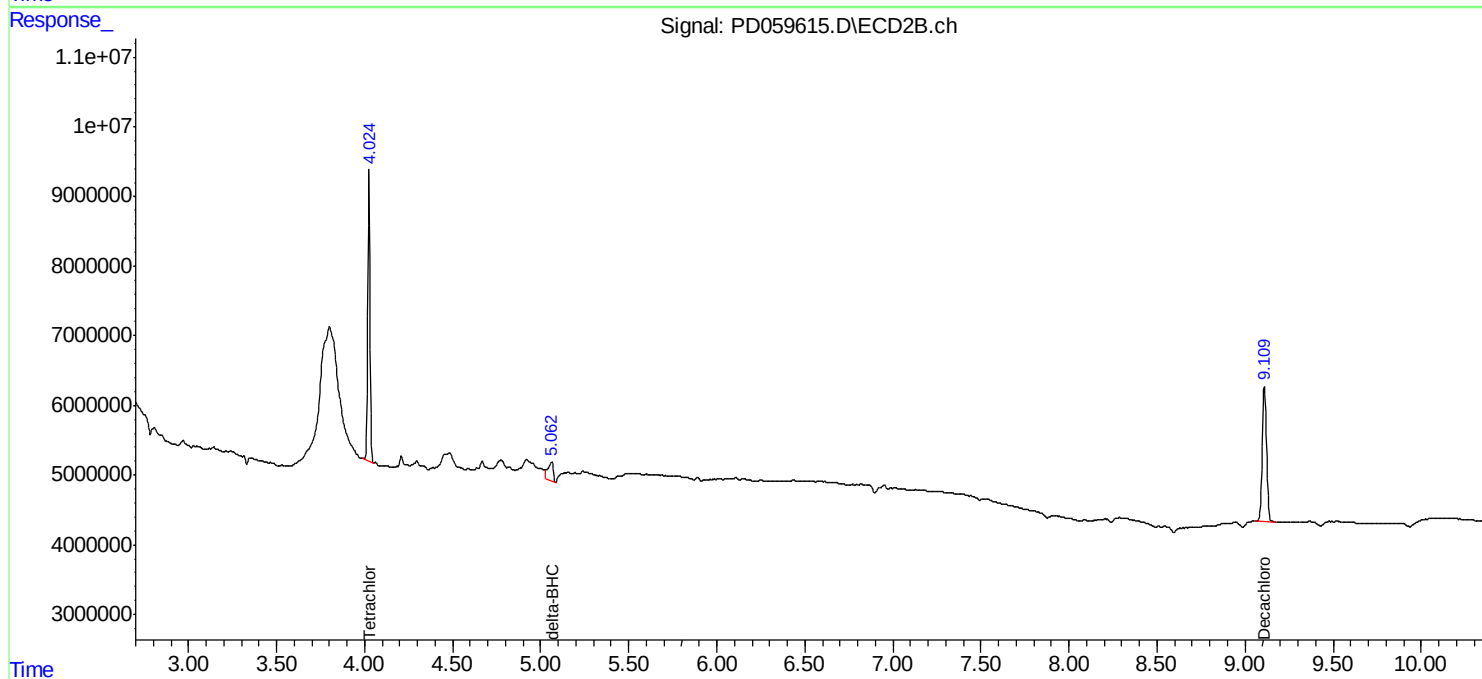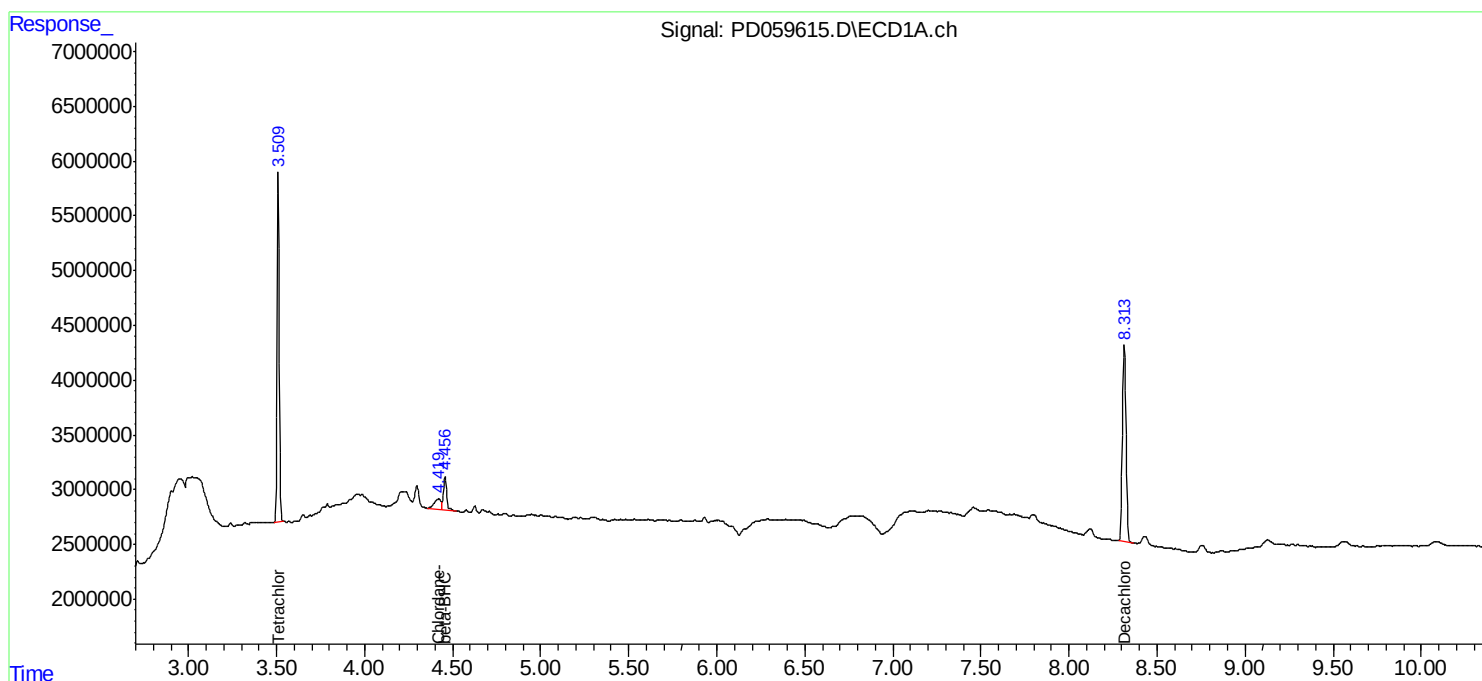


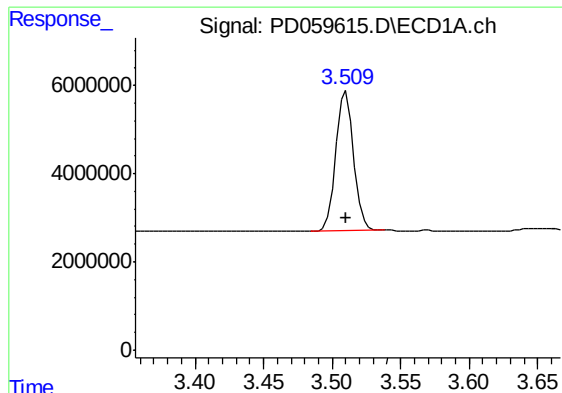

#1 Tetrachloro-m-xylene


R.T.: 3.510 min
Delta R.T.: 0.000 min
Response: 28806545
Conc: 19.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
PAV-B4-100620-DP

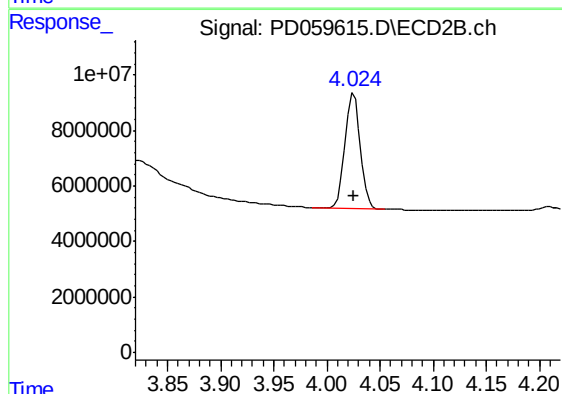


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 41121181
Conc: 18.92 ng/ml

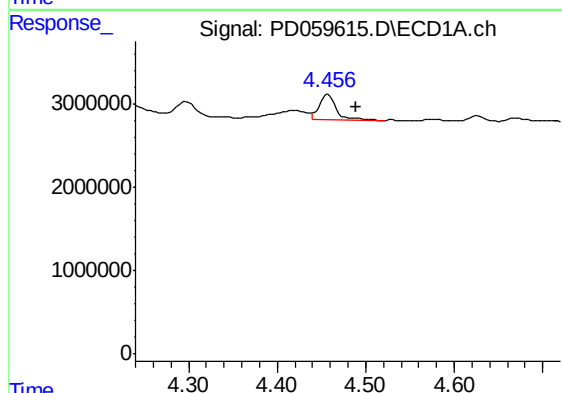


#6 beta-BHC

R.T.: 4.458 min
Delta R.T.: -0.032 min
Response: 3925818
Conc: 4.61 ng/ml

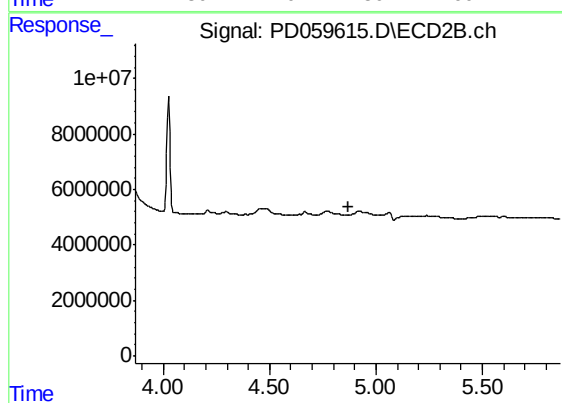

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.869 min
Response: 0
Conc: N.D.

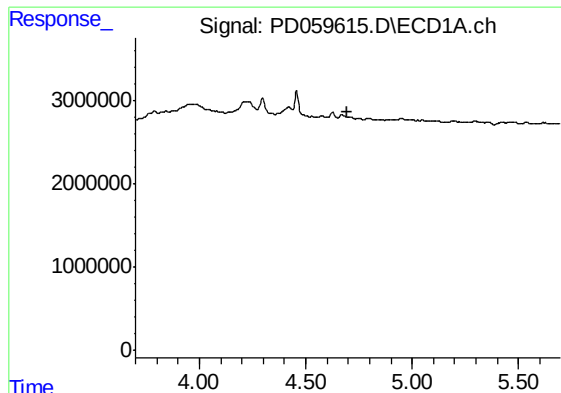

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.698 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PAV-B4-100620-DP

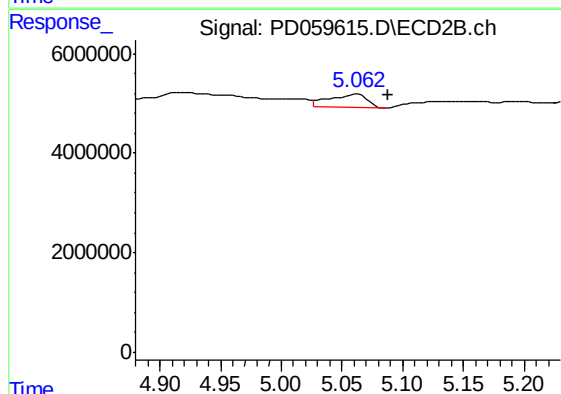


#7 delta-BHC

R.T.: 5.063 min
Delta R.T.: -0.025 min
Response: 5845923
Conc: 2.13 ng/ml

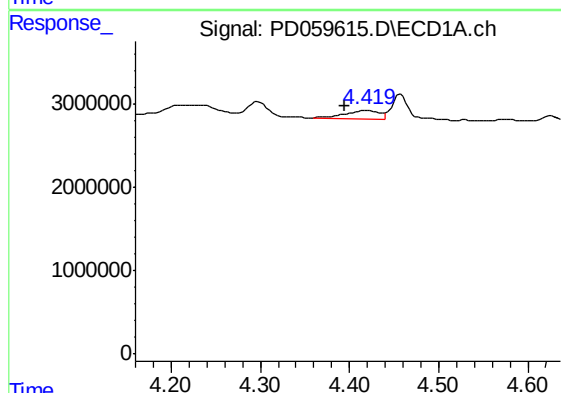


#23 Chlordane-1

R.T.: 4.420 min
Delta R.T.: 0.026 min
Response: 2600303
Conc: 50.05 ng/ml

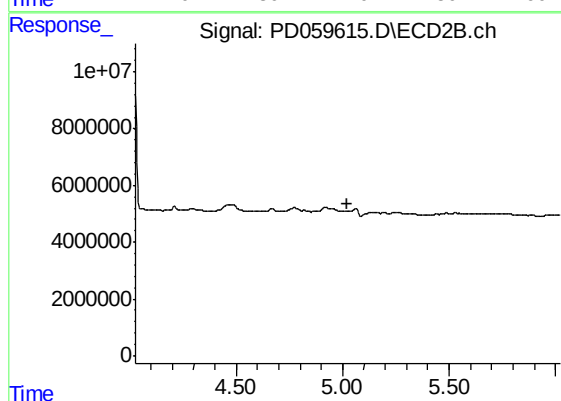

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.024 min
Response: 0
Conc: N.D.

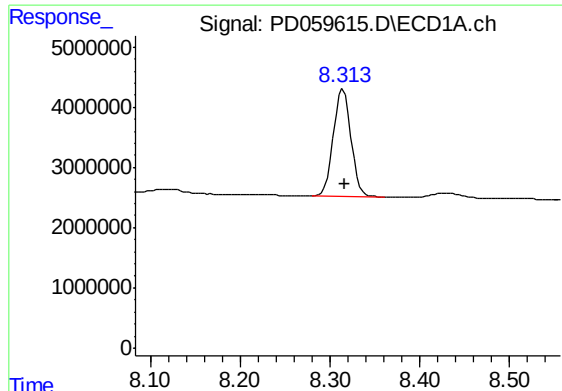

#28 Decachlorobiphenyl

R.T.: 8.315 min
Delta R.T.: -0.002 min
Response: 24327250
Conc: 21.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PAV-B4-100620-DP

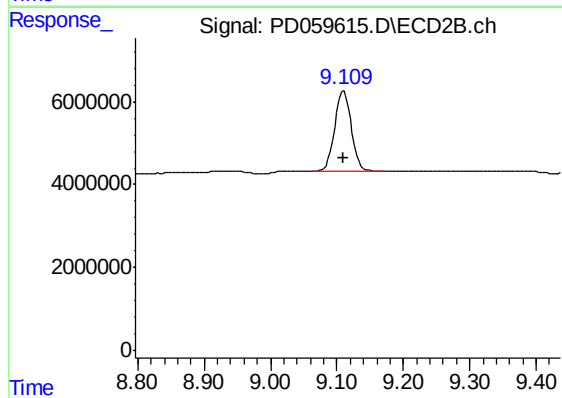

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 33461332
Conc: 20.77 ng/ml