

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100920\
 Data File : PD059616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2020 19:00
 Operator : DD\AJ
 Sample : L4292-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PAV-B13-100620-0-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:20:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.510	4.025	28670291	39433331	19.885	18.139
28) SA	Decachlor...	8.313	9.110	24084386	33748104	21.681	20.945
Target Compounds							
6) B	beta-BHC	4.458f	0.000	4168502	0	4.894	N.D. #
7) B	delta-BHC	0.000	5.064f	0	3595267	N.D.	1.308 #
23)	Chlordane-1	4.422f	0.000	1913408	0	36.829	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100920\
Data File : PD059616.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2020 19:00
Operator : DD\AJ
Sample : L4292-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PAV-B13-100620-0-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:20:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

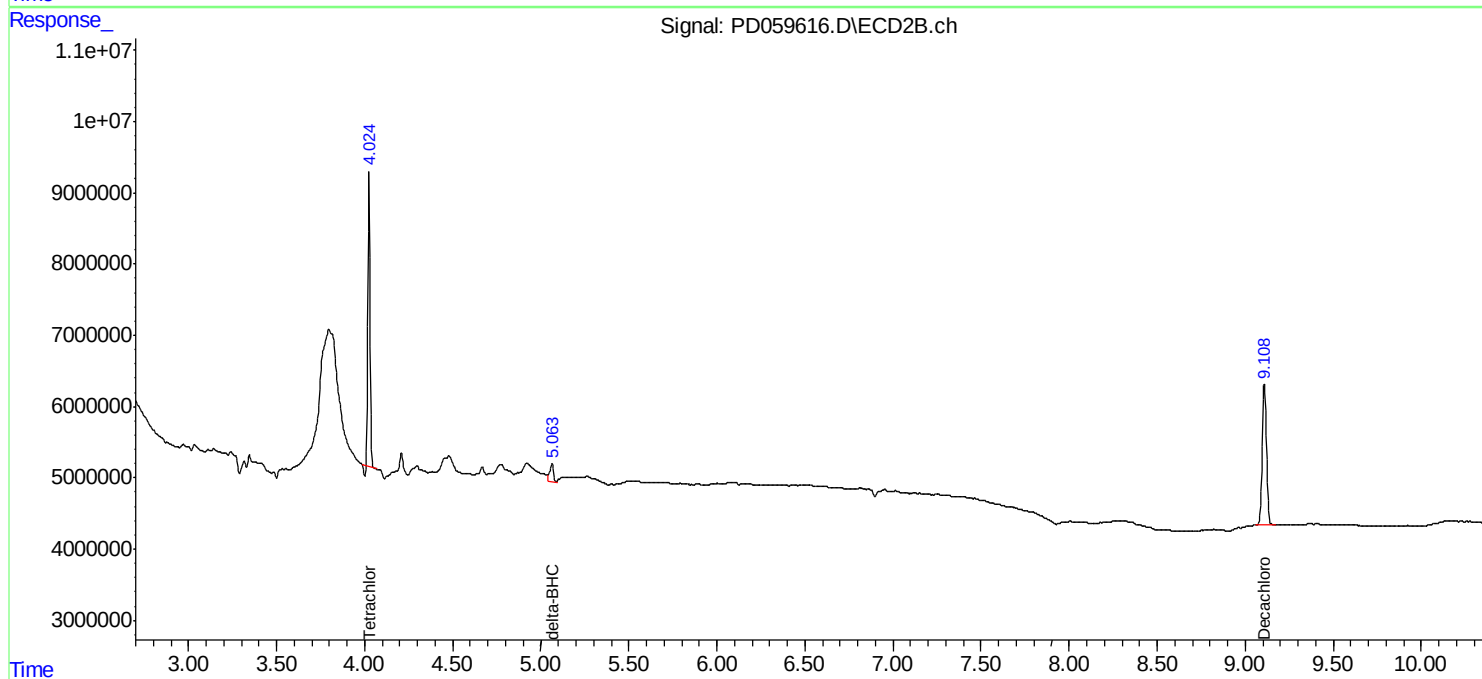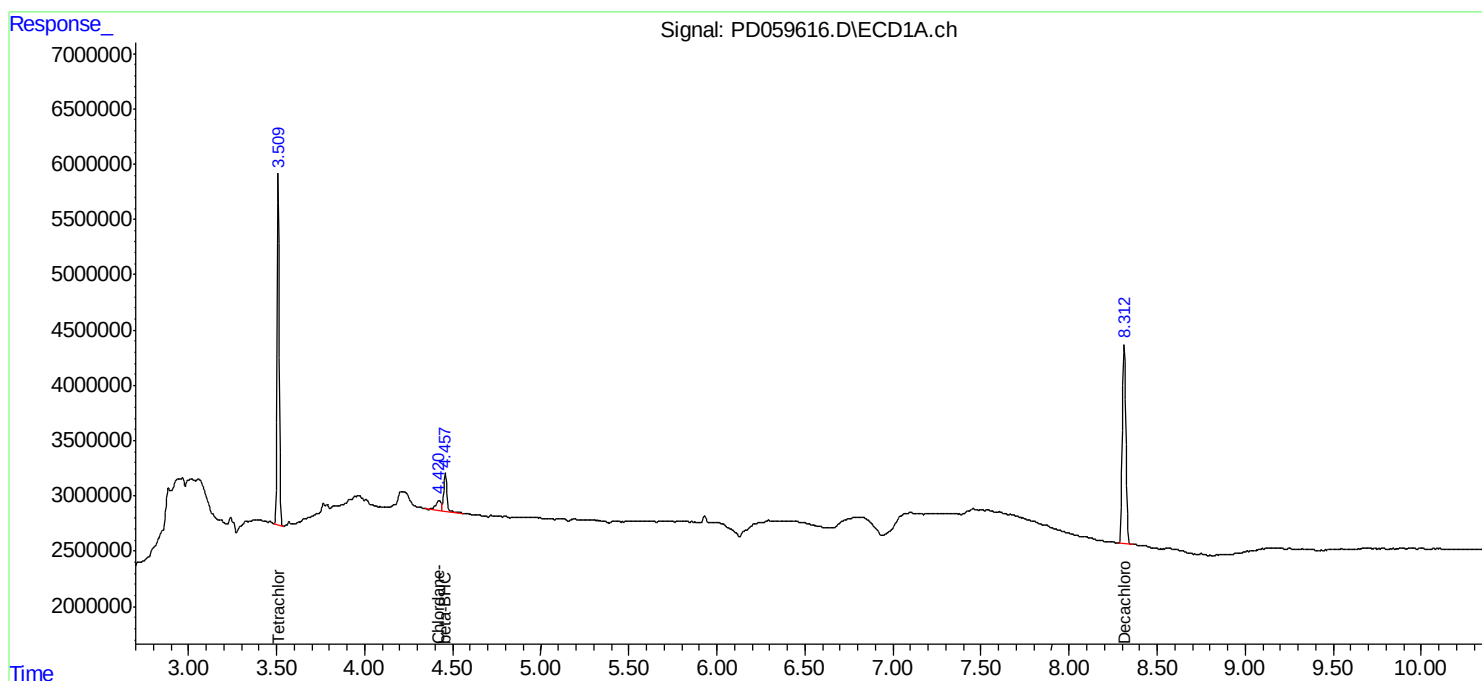


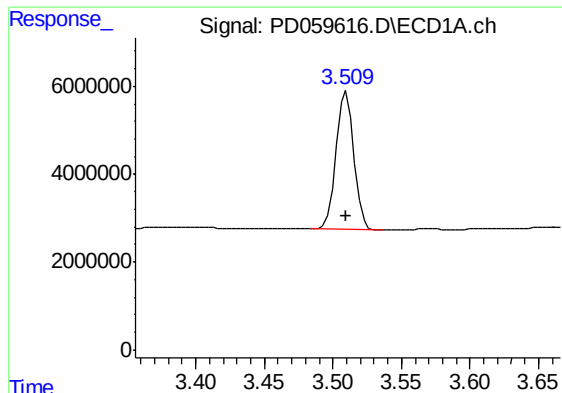

#1 Tetrachloro-m-xylene


R.T.: 3.510 min
Delta R.T.: 0.000 min
Response: 28670291
Conc: 19.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PAV-B13-100620-0-10

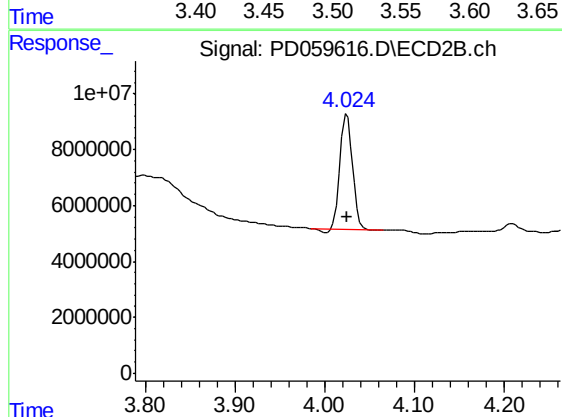


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 39433331
Conc: 18.14 ng/ml

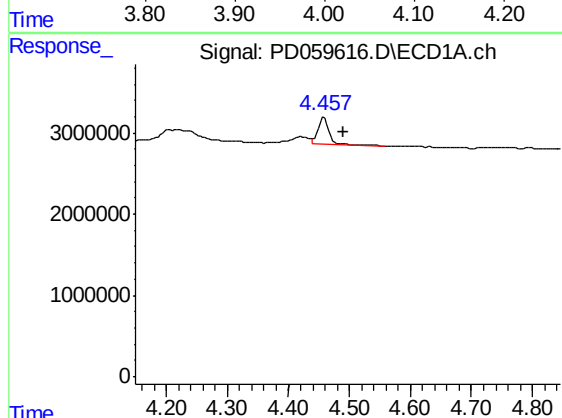


#6 beta-BHC

R.T.: 4.458 min
Delta R.T.: -0.031 min
Response: 4168502
Conc: 4.89 ng/ml

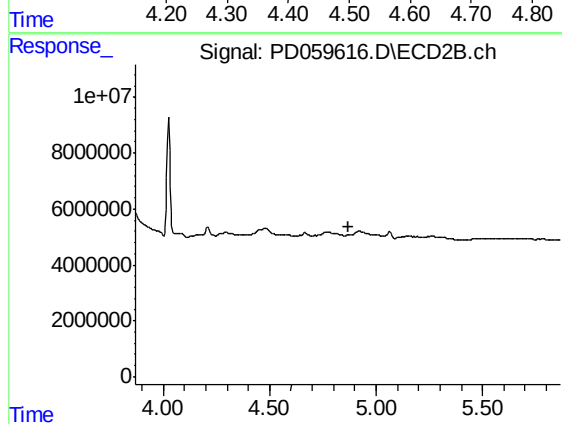

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.869 min
Response: 0
Conc: N.D.

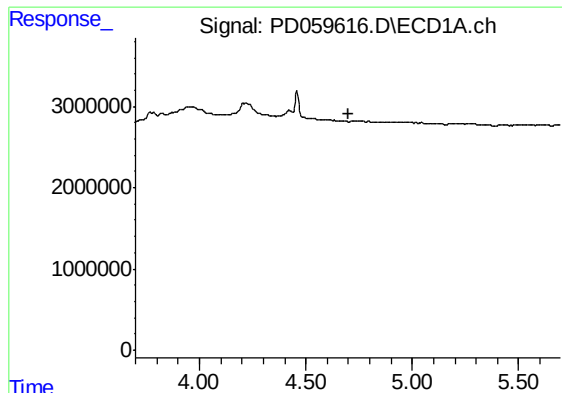

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.698 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PAV-B13-100620-0-10

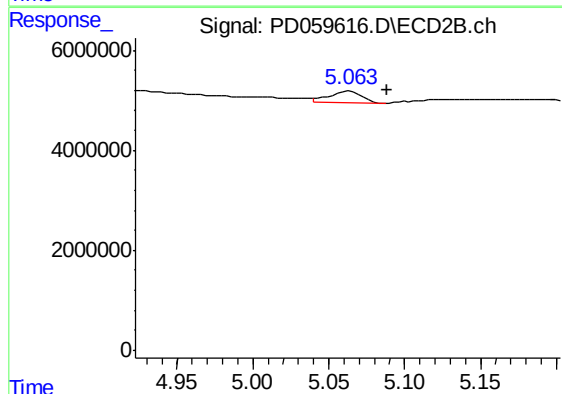


#7 delta-BHC

R.T.: 5.064 min
Delta R.T.: -0.024 min
Response: 3595267
Conc: 1.31 ng/ml

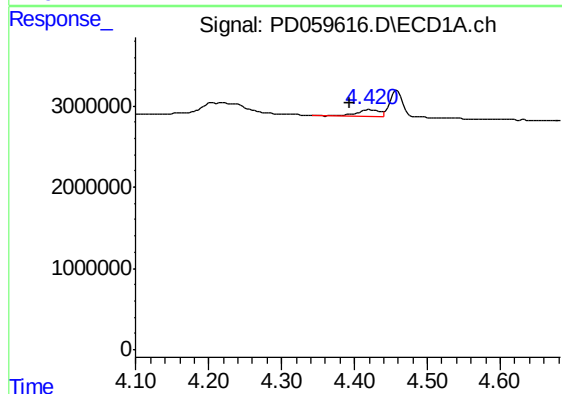


#23 Chlordane-1

R.T.: 4.422 min
Delta R.T.: 0.028 min
Response: 1913408
Conc: 36.83 ng/ml

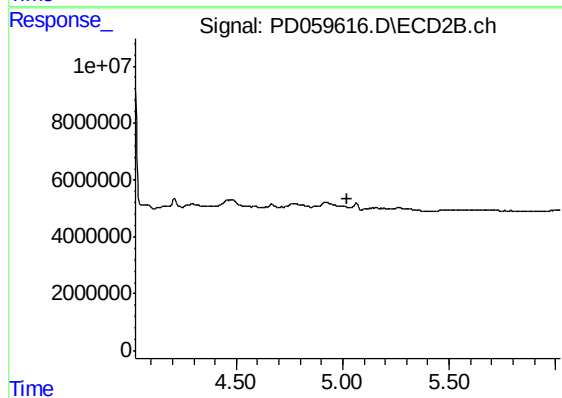

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.024 min
Response: 0
Conc: N.D.

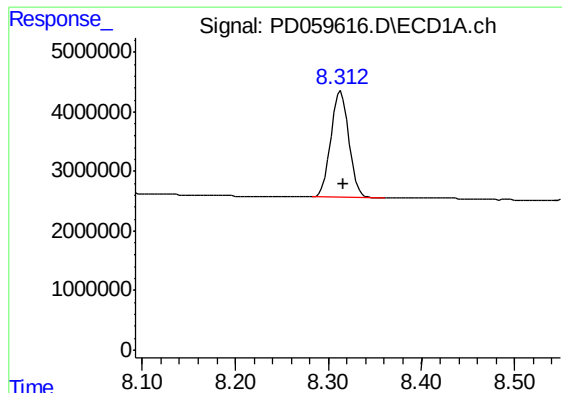

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: -0.003 min
Response: 24084386
Conc: 21.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PAV-B13-100620-0-10

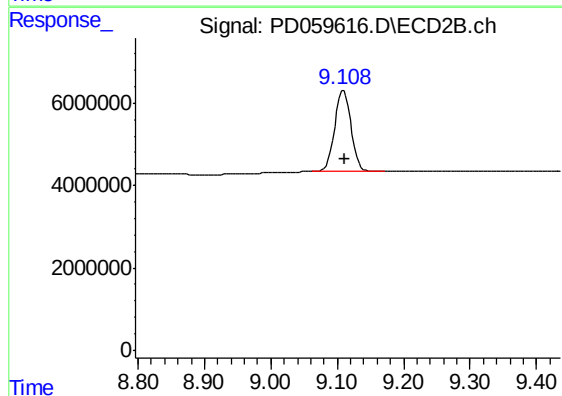

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 33748104
Conc: 20.94 ng/ml