

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100920\
 Data File : PD059618.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2020 19:28
 Operator : DD\AJ
 Sample : L4311-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PAV-B10-100720-0-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:20:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.510	4.025	28620853	40575074	19.851	18.664
28) SA	Decachlor...	8.313	9.110	24128192	33978134	21.720	21.087
Target Compounds							
6) B	beta-BHC	4.458f	0.000	3713817	0	4.361	N.D. #
7) B	delta-BHC	0.000	5.063f	0	2558062	N.D.	0.930 #
23)	Chlordane-1	4.418f	0.000	2199538	0	42.336	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100920\
Data File : PD059618.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2020 19:28
Operator : DD\AJ
Sample : L4311-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PAV-B10-100720-0-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:20:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

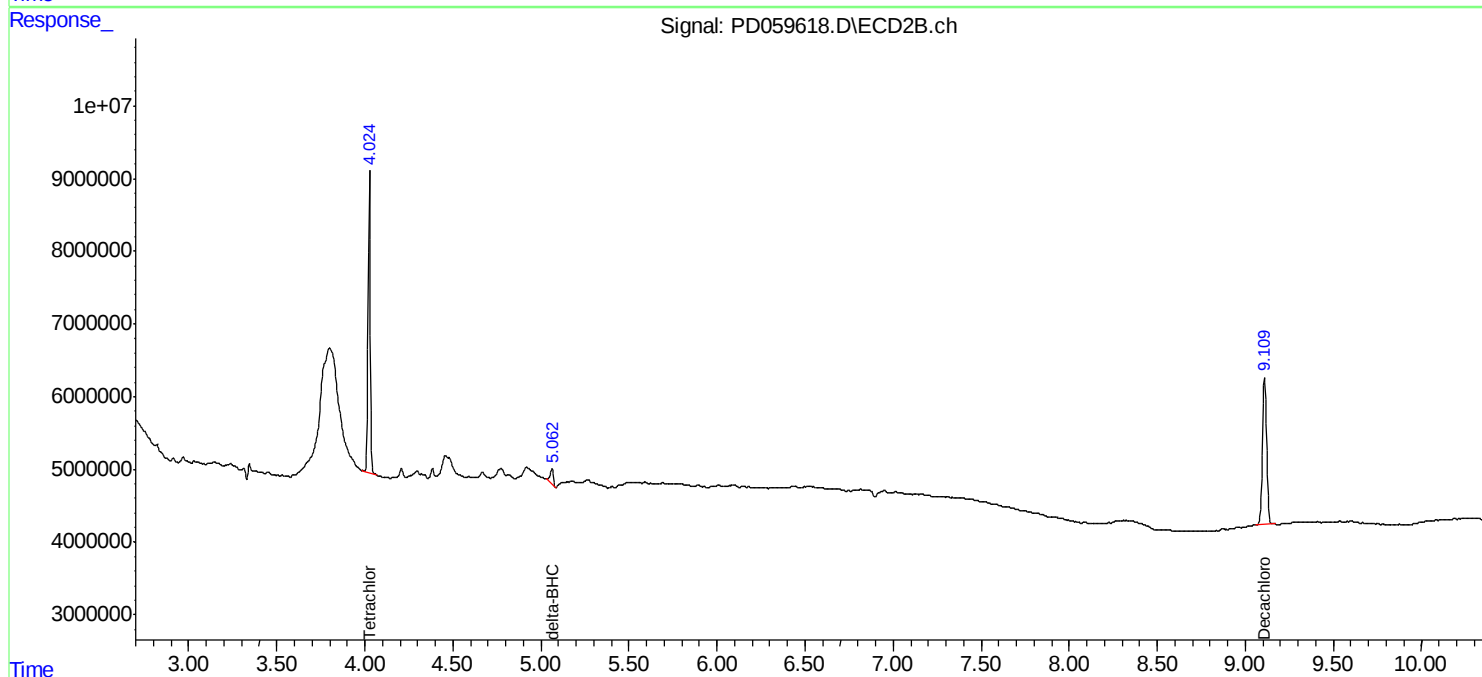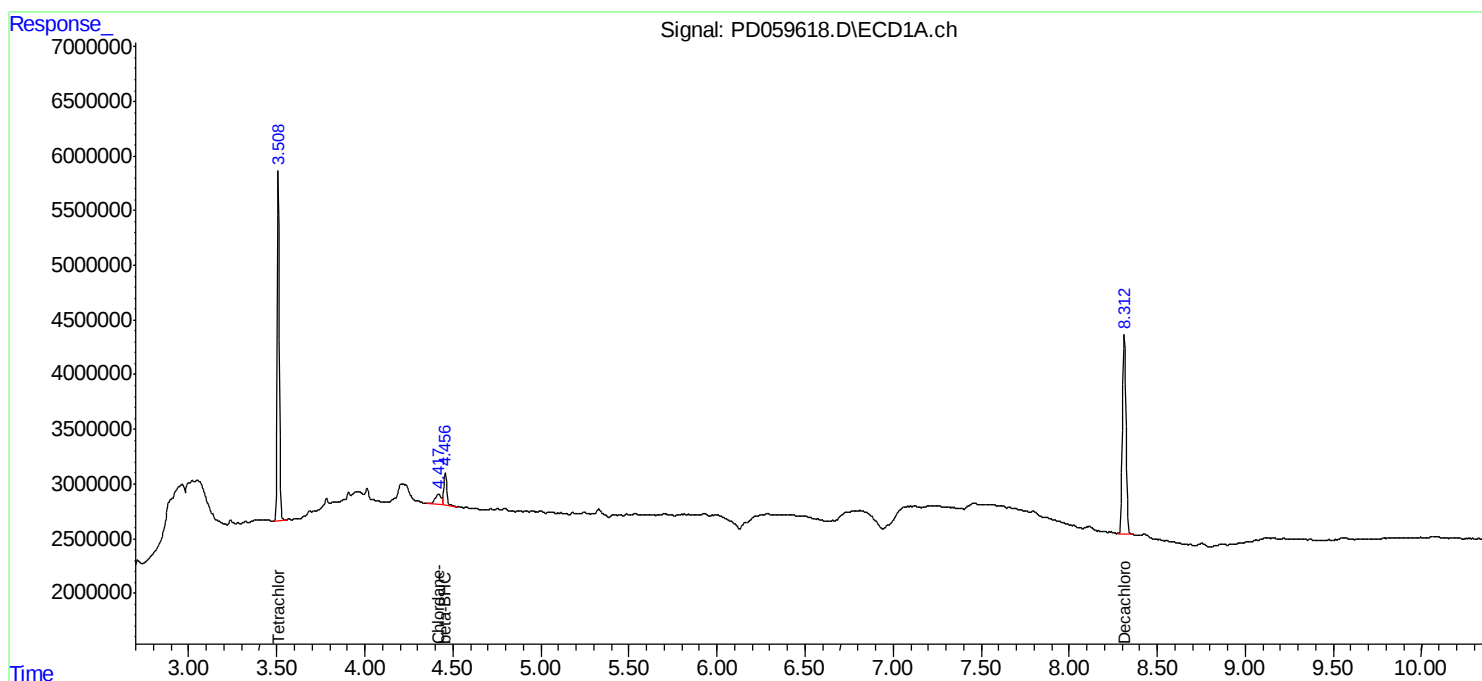


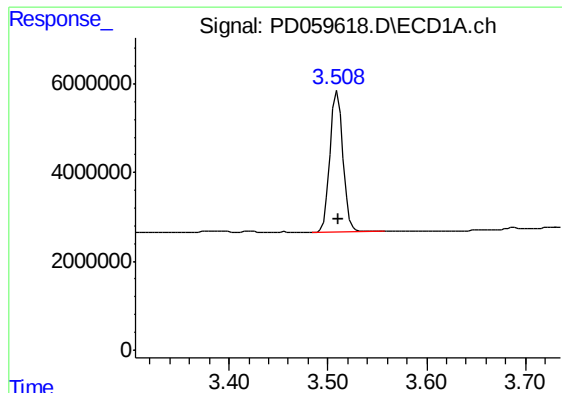

#1 Tetrachloro-m-xylene


R.T.: 3.510 min
Delta R.T.: 0.000 min
Response: 28620853
Conc: 19.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
PAV-B10-100720-0-10

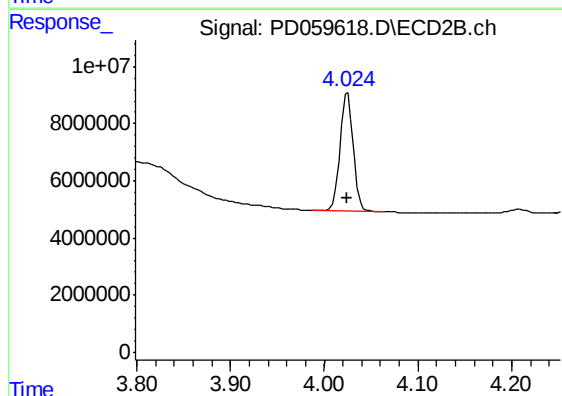


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 40575074
Conc: 18.66 ng/ml

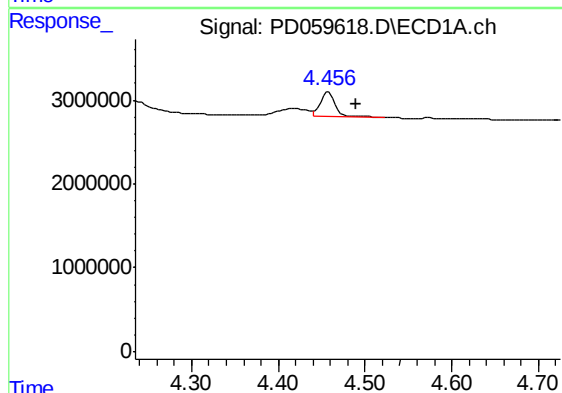


#6 beta-BHC

R.T.: 4.458 min
Delta R.T.: -0.032 min
Response: 3713817
Conc: 4.36 ng/ml

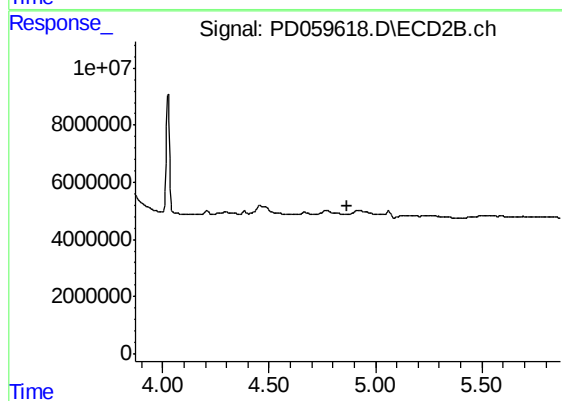

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.869 min
Response: 0
Conc: N.D.

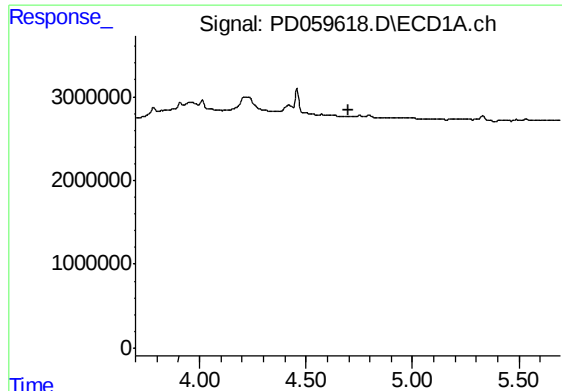

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.698 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PAV-B10-100720-0-10

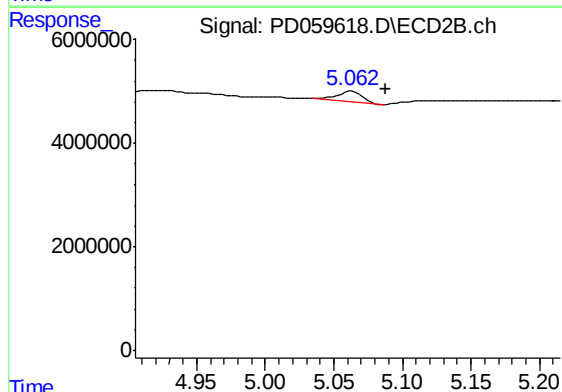


#7 delta-BHC

R.T.: 5.063 min
Delta R.T.: -0.025 min
Response: 2558062
Conc: 0.93 ng/ml

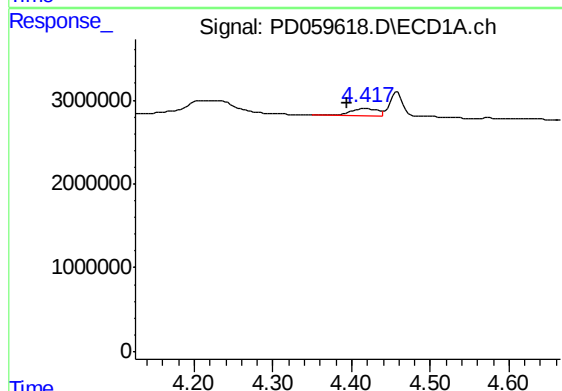


#23 Chlordane-1

R.T.: 4.418 min
Delta R.T.: 0.024 min
Response: 2199538
Conc: 42.34 ng/ml

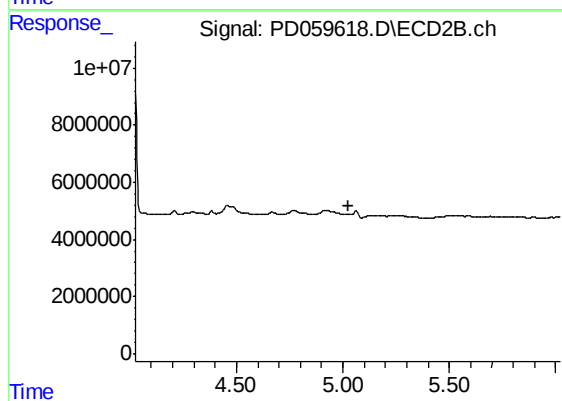

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.024 min
Response: 0
Conc: N.D.

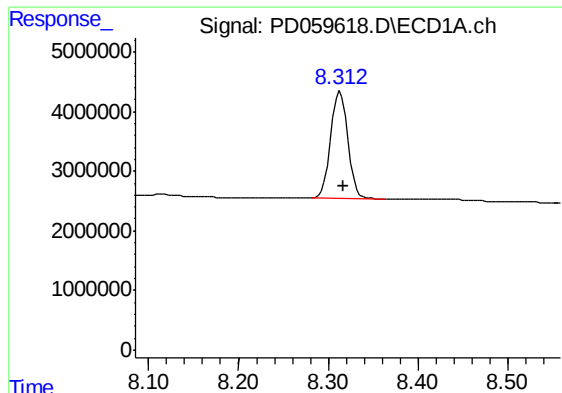

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: -0.003 min
Response: 24128192
Conc: 21.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PAV-B10-100720-0-10

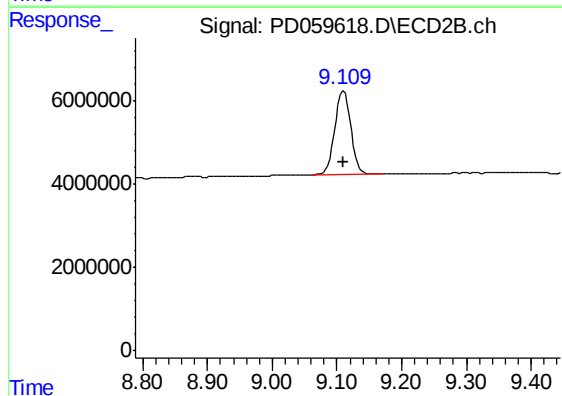

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 33978134
Conc: 21.09 ng/ml